


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW100218\
Data File : VW005766.D
Acq On : 02 Oct 2018 08:58
Operator : SY/AP
Sample : BFB87
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB87

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM092818S.M
Title : VOC Analysis
Last Update : Fri Oct 05 01:16:24 2018

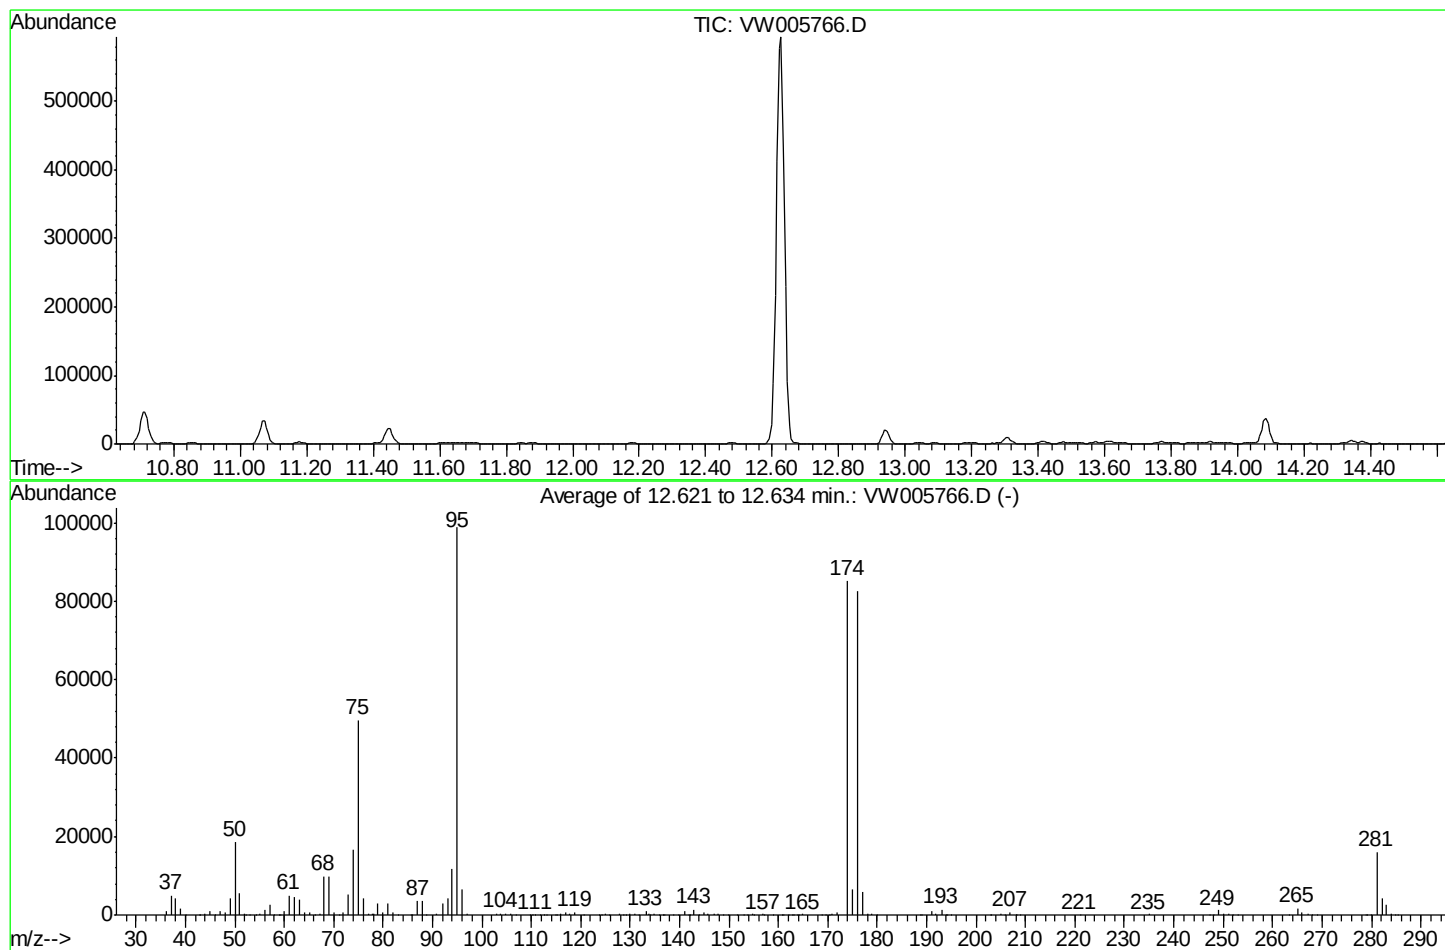

AutoFind: Scans 1758, 1759, 1760; Background Corrected with Scan 1750

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.9	18715	PASS
75	95	30	80	50.3	49693	PASS
95	95	100	100	100.0	98824	PASS
96	95	5	9	6.6	6543	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	86.2	85186	PASS
175	174	5	9	7.8	6662	PASS
176	174	95	101	96.9	82560	PASS
177	176	5	9	7.0	5772	PASS

Scan 1750 (12.573 min): VW005766.D
BFB87

m/z	Abundance
40.00	103.0
44.10	186.0
206.90	119.0

Instrument :
MSVOA_W
ClientSampleId :
BFB87

m/z	Abundance
36.00	1193.0
37.10	5718.0
38.10	4889.0
39.00	1791.0
39.90	156.0
40.10	159.0
42.80	122.0
43.90	690.0
45.00	1104.0
46.00	131.0
47.00	1240.0
48.10	796.0
49.00	4230.0
50.00	20656.0
51.00	6525.0
52.00	301.0
53.00	152.0
55.00	269.0
56.00	1667.0
57.00	3161.0
57.90	109.0
58.90	388.0
60.00	1179.0
61.00	5606.0
62.00	5055.0
63.10	4623.0
64.00	717.0
65.10	777.0
67.20	299.0
68.00	11157.0
69.00	10600.0
70.00	817.0
71.00	79.0
72.10	606.0
73.00	6584.0
74.00	18896.0
75.00	52800.0
76.00	4761.0
77.10	540.0
77.90	324.0
78.90	3253.0
80.00	779.0
80.90	3220.0
81.90	773.0
83.00	98.0
85.50	110.0
87.00	4080.0
88.00	4081.0
90.90	531.0
92.00	3243.0
93.00	4341.0
94.00	12421.0
95.00	105192.0
96.00	7161.0
96.90	330.0
102.90	520.0
103.90	587.0
104.90	275.0
105.90	405.0
106.80	84.0
109.80	138.0
110.10	126.0
110.80	176.0
111.90	192.0
112.50	56.0
113.00	93.0
114.90	178.0
115.10	180.0
115.90	337.0
116.90	810.0
117.80	617.0
118.80	849.0
120.70	98.0
123.70	59.0
125.00	579.0
128.00	343.0
128.80	148.0
130.00	296.0
130.90	218.0
131.80	72.0
133.10	1817.0
133.80	583.0
134.80	348.0
136.00	78.0
136.90	169.0
138.80	54.0
139.80	86.0
141.00	1133.0
142.10	174.0
142.90	1738.0
143.80	109.0
144.90	690.0

Instrument :
MSVOA_W
ClientSampleId :
BFB87

145.80	206.0
147.00	322.0
147.80	382.0
149.00	171.0
149.80	180.0
151.70	90.0
153.80	133.0
154.80	267.0
156.90	249.0
159.00	93.0
161.10	245.0
162.10	112.0
162.80	355.0
163.70	59.0
165.00	285.0
168.80	70.0
170.90	299.0
171.90	697.0
174.00	84432.0
175.00	7103.0
175.90	80736.0
177.00	5882.0
178.10	235.0
178.90	577.0
180.00	117.0
189.10	152.0
191.10	1752.0
191.90	353.0
193.00	2059.0
194.00	311.0
194.90	181.0
202.90	289.0
205.00	482.0
205.90	146.0
207.00	1150.0
208.00	303.0
208.90	234.0
221.00	191.0
235.00	143.0
247.10	71.0
247.90	75.0
249.00	1660.0
250.00	476.0
251.10	673.0
252.00	301.0
253.00	111.0
263.30	66.0
265.00	2804.0
266.00	740.0
267.10	568.0
267.90	112.0
278.80	207.0
279.20	221.0
281.10	22144.0
282.10	5848.0
283.10	3791.0
284.20	667.0
284.90	205.0

Instrument :
MSVOA_W
ClientSampleId :
BFB87

m/z	Abundance
36.10	790.0
37.00	3785.0
38.00	3413.0
39.10	1514.0
40.00	85.0
42.90	129.0
43.90	430.0
45.10	732.0
47.20	763.0
48.00	466.0
49.00	3495.0
50.00	14498.0
51.00	4326.0
52.20	195.0
53.00	136.0
54.20	56.0
55.00	256.0
56.00	1042.0
57.10	1794.0
58.70	67.0
59.90	816.0
61.00	3850.0
62.00	3589.0
63.00	2968.0
64.00	453.0
65.00	454.0
67.20	252.0
68.00	7908.0
69.00	8027.0
70.10	604.0
72.10	295.0
73.00	3711.0
74.00	13394.0
75.00	40120.0
76.10	3534.0
77.00	294.0
77.80	374.0
78.90	2232.0
80.00	739.0
80.90	2175.0
81.80	383.0
82.90	70.0
86.00	164.0
86.90	2806.0
87.90	2747.0
88.80	89.0
91.00	289.0
92.00	2314.0
93.00	3693.0
94.00	9701.0
95.00	81232.0
96.00	4939.0
97.00	117.0
103.00	205.0
103.70	270.0
104.70	106.0
105.80	419.0
106.90	86.0
110.10	81.0
110.90	88.0
113.00	94.0
115.10	142.0
115.80	388.0
116.90	471.0
117.90	318.0
118.90	564.0
124.20	53.0
125.00	196.0
125.60	109.0
127.90	340.0
128.60	100.0
129.10	113.0
130.00	259.0
130.90	188.0
133.00	535.0
134.10	117.0
135.00	155.0
135.90	65.0
136.70	126.0
137.00	125.0
141.00	892.0
141.70	118.0
143.00	1110.0
144.90	389.0
145.90	125.0
146.90	210.0
147.90	299.0
148.80	116.0
149.90	81.0
155.00	209.0
157.10	178.0
158.90	129.0

Instrument :
MSVOA_W
ClientSampleId :
BFB87

160.80	168.0
163.00	146.0
165.00	57.0
171.00	306.0
171.90	707.0
174.00	75928.0
175.00	5781.0
176.00	74520.0
177.00	5008.0
177.90	189.0
178.90	154.0
180.00	77.0
189.00	84.0
191.00	657.0
191.90	228.0
192.90	648.0
194.00	64.0
194.90	75.0
203.00	136.0
205.00	222.0
207.00	494.0
208.10	86.0
235.00	148.0
248.90	589.0
250.00	193.0
251.00	352.0
252.10	52.0
265.00	967.0
266.00	267.0
266.90	166.0
268.00	68.0
278.80	120.0
279.80	91.0
281.10	8980.0
282.10	2438.0
282.90	1397.0
284.10	240.0
285.20	119.0

Instrument :
MSVOA_W
ClientSampleId :
BFB87

m/z	Abundance
36.10	1273.0
37.00	5419.0
38.10	4476.0
39.00	1950.0
39.90	156.0
43.00	151.0
44.00	878.0
45.10	1067.0
46.10	112.0
47.10	1292.0
48.00	794.0
49.00	4942.0
50.00	20992.0
51.00	6247.0
52.00	294.0
52.80	102.0
55.00	444.0
56.00	1722.0
57.00	3231.0
57.90	94.0
59.10	170.0
60.00	1025.0
61.00	5387.0
62.00	5567.0
63.00	4373.0
64.10	839.0
65.00	733.0
66.20	61.0
67.10	444.0
68.00	10769.0
69.10	10610.0
70.00	669.0
71.00	75.0
71.90	609.0
73.00	5569.0
74.00	17848.0
75.00	56160.0
76.00	4770.0
77.00	563.0
78.10	533.0
78.90	3225.0
79.90	887.0
80.90	3153.0
82.00	656.0
82.90	151.0
86.00	210.0
87.00	4046.0
87.90	3971.0
90.90	587.0
92.00	3309.0
93.00	5091.0
94.00	13455.0
95.00	110048.0
96.00	7530.0
97.00	254.0
103.00	253.0
103.90	468.0
104.90	253.0
105.80	330.0
106.90	108.0
109.80	205.0
110.80	78.0
111.90	147.0
113.00	80.0
114.70	236.0
115.80	463.0
117.00	894.0
117.80	516.0
118.90	865.0
123.70	77.0
125.00	624.0
125.80	158.0
127.90	343.0
129.00	254.0
129.80	463.0
130.90	253.0
133.20	911.0
134.90	332.0
137.00	220.0
141.00	1233.0
142.10	169.0
142.90	1583.0
143.80	108.0
145.00	543.0
145.80	268.0
147.10	266.0
147.90	241.0
148.90	240.0
149.90	179.0
151.70	102.0
153.00	53.0
154.80	291.0

Instrument :
MSVOA_W
ClientSampleId :
BFB87

156.90	340.0
158.80	244.0
160.80	259.0
163.00	240.0
164.20	60.0
164.90	198.0
168.70	60.0
169.50	112.0
170.30	104.0
170.80	248.0
172.00	867.0
173.90	95200.0
175.00	7103.0
176.00	92424.0
177.00	6428.0
178.00	258.0
178.80	334.0
180.00	86.0
188.80	97.0
190.90	958.0
191.90	230.0
193.00	1449.0
194.20	274.0
195.00	182.0
203.10	139.0
205.00	406.0
207.00	1047.0
208.20	152.0
208.90	114.0
221.10	83.0
235.10	253.0
247.10	55.0
248.90	1340.0
249.90	355.0
251.10	471.0
251.90	161.0
253.10	98.0
265.10	1387.0
266.00	528.0
267.10	630.0
267.90	119.0
269.00	109.0
279.00	211.0
281.10	17272.0
282.10	4828.0
283.10	3034.0
284.00	542.0
284.90	175.0

Instrument :
MSVOA_W
ClientSampleId :
BFB87