


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW100220\
Data File : VW016759.D
Acq On : 02 Oct 2020 13:29
Operator : SY/VA
Sample : L4201-20
Misc : 3.52G/10ML/MSVOA W/SOIL
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampled :
COAM3

Manual Integrations
APPROVED

MMDadoda
10/5/2020 5:06:07 PM

Quant Time: Oct 03 05:36:26 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM091520S.M
Quant Title : VOC Analysis
QLast Update : Sat Oct 03 04:48:41 2020
Response via : Initial Calibration

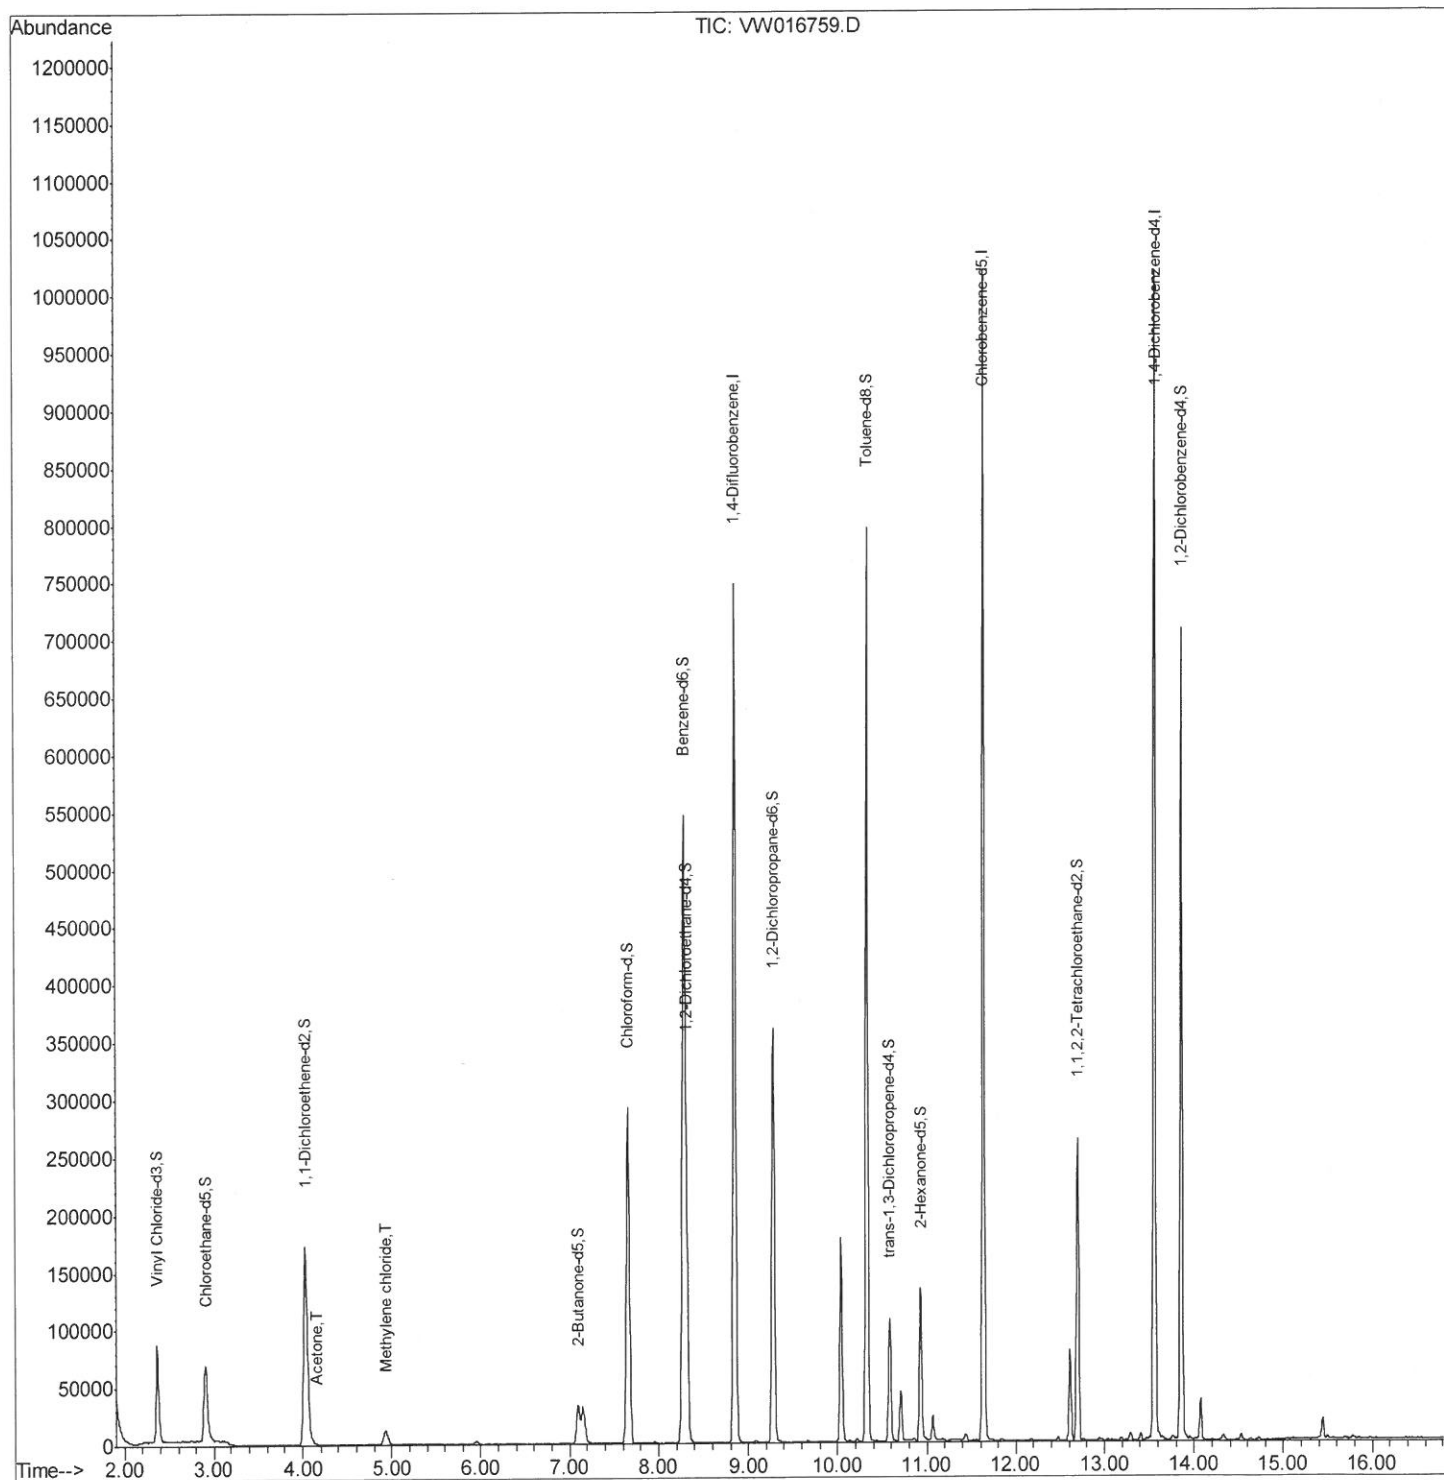

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW100220\
 Data File : VW016759.D
 Acq On : 02 Oct 2020 13:29
 Operator : SY/VA
 Sample : L4201-20
 Misc : 3.52G/10ML/MSVOA W/SOIL
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_W
ClientSampleId :
 C0AM3

Manual Integrations
APPROVED

MMDadoda
 10/5/2020 5:06:07 PM

Quant Time: Oct 03 04:56:50 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM091520S.M
 Quant Title : VOC Analysis
 QLast Update : Sat Oct 03 04:48:41 2020
 Response via : Initial Calibration

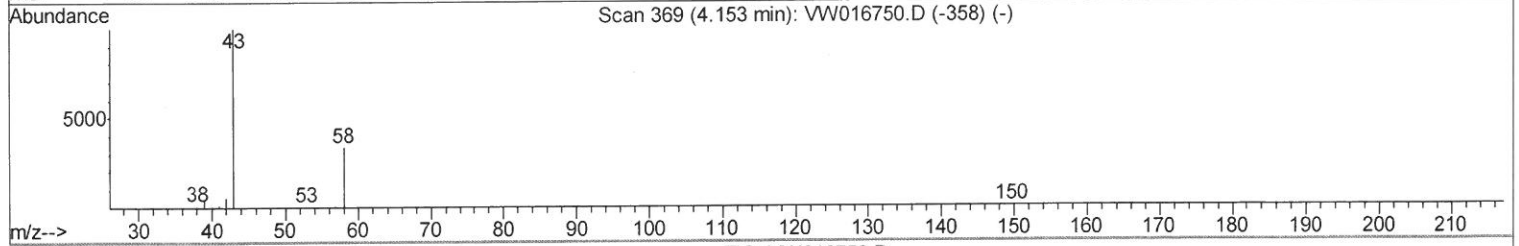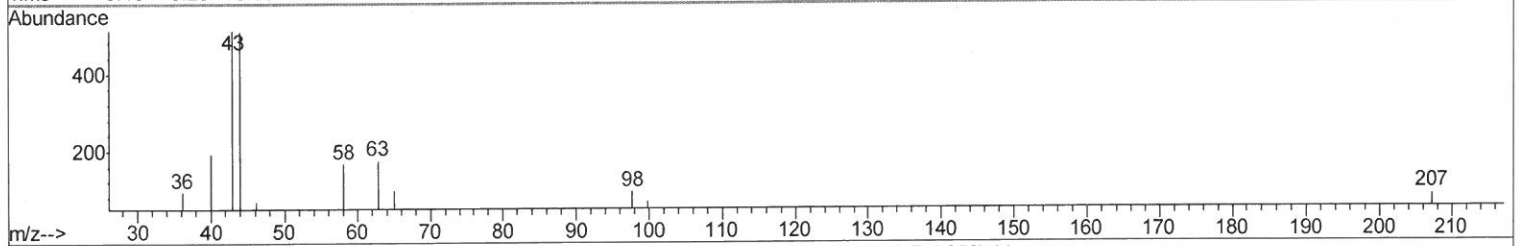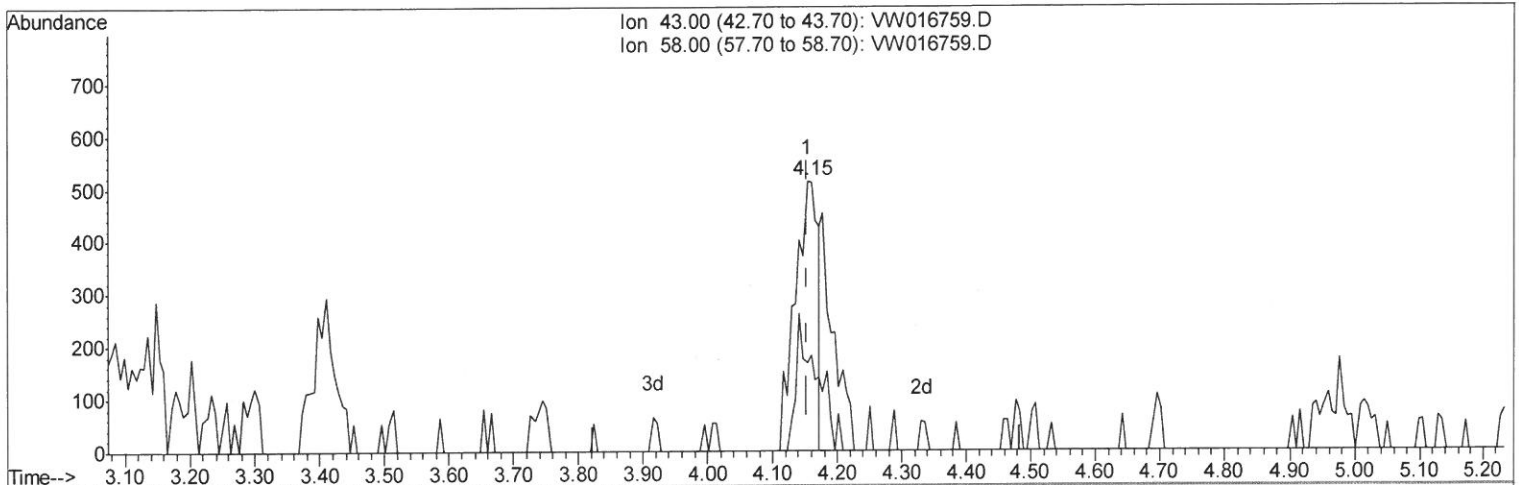

TIC: VW016759.D

(13) Acetone (T)

4.154min (+0.000) 0.92ug/L

response 1271

Ion	Exp%	Act%
43.00	100	100
58.00	30.10	21.95
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW100220\
 Data File : VW016759.D
 Acq On : 02 Oct 2020 13:29
 Operator : SY/VA
 Sample : L4201-20
 Misc : 3.52G/10ML/MSVOA W/SOIL
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AM3

Manual Integrations
 APPROVED

MMDadoda
 10/5/2020 5:06:07 PM

Quant Time: Oct 03 04:56:50 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM091520S.M
 Quant Title : VOC Analysis
 QLast Update : Sat Oct 03 04:48:41 2020
 Response via : Initial Calibration

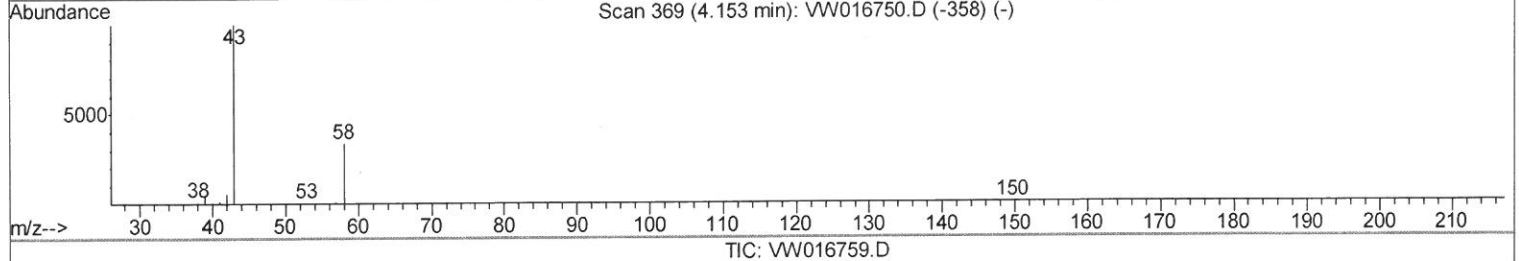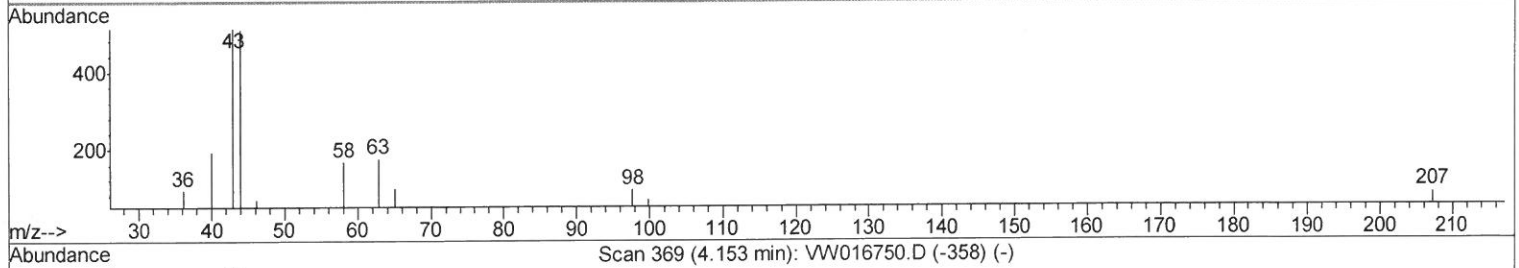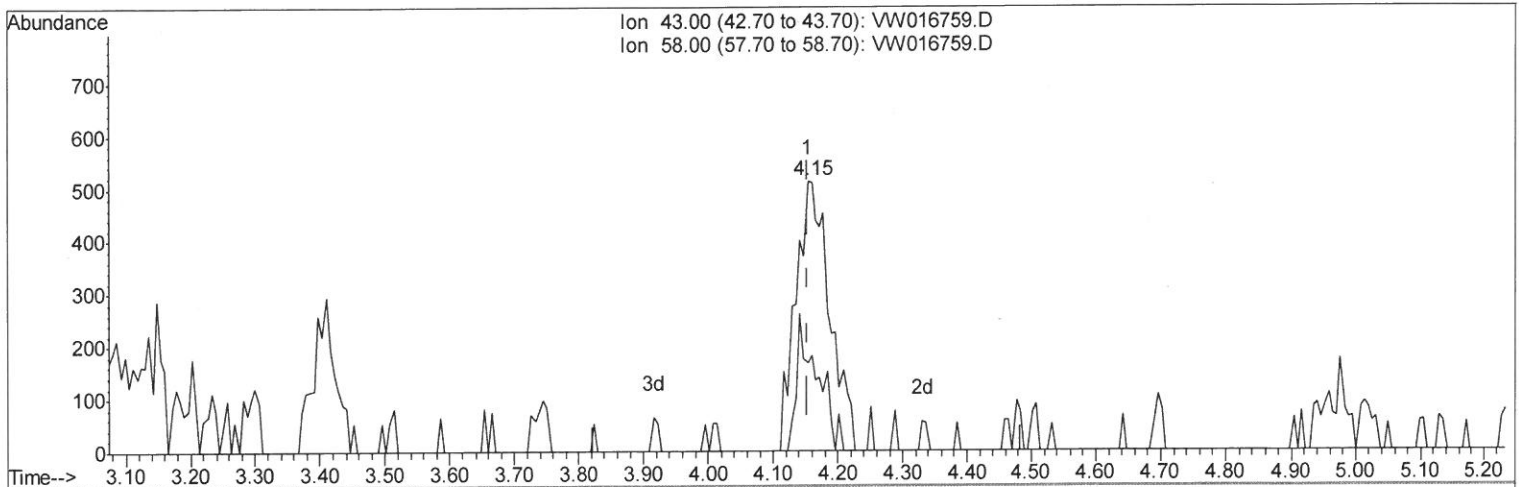

(13) Acetone (T)

4.154min (+0.000) 1.35ug/L m

710109/20 sy

response 1871

Ion	Exp%	Act%
43.00	100	100
58.00	30.10	14.91
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW100220\
 Data File : VW016759.D
 Acq On : 02 Oct 2020 13:29
 Operator : SY/VA
 Sample : L4201-20
 Misc : 3.52G/10ML/MSVOA W/SOIL
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AM3

Manual Integrations
 APPROVED

MMDadoda
 10/5/2020 5:06:07 PM

Quant Time: Oct 03 05:36:26 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM091520S.M
 Quant Title : VOC Analysis
 QLast Update : Sat Oct 03 04:48:41 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	669230	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	596459	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	287141	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.37	65	104727	16.17	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	64.68%
7) Chloroethane-d5	2.90	69	104411	19.74	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	78.96%
10) 1,1-Dichloroethene-d2	4.03	63	179962	12.43	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	49.72%
20) 2-Butanone-d5	7.09	46	56700	32.10	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	64.20%
24) Chloroform-d	7.66	84	304166	21.73	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	86.92%
26) 1,2-Dichloroethane-d4	8.31	65	144786	20.15	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	80.60%
29) Benzene-d6	8.28	84	586690	21.93	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	87.72%
33) 1,2-Dichloropropane-d6	9.28	67	166131	22.92	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	91.68%
37) Toluene-d8	10.33	98	542951	20.63	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	82.52%
38) trans-1,3-Dichloropropene-	10.58	79	62482	17.10	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	68.40%
39) 2-Hexanone-d5	10.93	63	46787	35.48	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	70.96%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	122590	19.87	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	79.48%
61) 1,2-Dichlorobenzene-d4	13.86	152	206880	22.55	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	90.20%

Target Compounds

13) Acetone	4.15	43	1871m	1.352	ug/L	Ovalue 10/19/20 57
16) Methylene chloride	4.93	84	10591	1.026	ug/L	88

(#) = qualifier out of range (m) = manual integration (+) = signals summed