

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW100318\
 Data File : VW005828.D
 Acq On : 03 Oct 2018 22:53
 Operator : SY/AP
 Sample : J5181-12
 Misc : 2.62G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 JLC41

Quant Time: Oct 15 08:06:10 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM092818S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Oct 04 07:04:02 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	257863	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	259938	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.57	152	126358	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	40010	12.17	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	48.68%
7) Chloroethane-d5	2.90	69	36971	14.42	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	57.68%
10) 1,1-Dichloroethene-d2	4.01	63	74728	10.41	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	41.64%#
20) 2-Butanone-d5	7.09	46	45963	43.55	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	87.10%
24) Chloroform-d	7.65	84	138314	20.88	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	83.52%
26) 1,2-Dichloroethane-d4	8.31	65	89382	22.28	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	89.12%
29) Benzene-d6	8.27	84	230624	17.92	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	71.68%
33) 1,2-Dichloropropane-d6	9.27	67	71542	19.24	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	76.96%
37) Toluene-d8	10.33	98	206053	16.22	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	64.88%
38) trans-1,3-Dichloropropene-	10.58	79	33869	17.34	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	69.36%
39) 2-Hexanone-d5	10.93	63	34194	39.26	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	78.52%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	78645	21.77	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	87.08%
61) 1,2-Dichlorobenzene-d4	13.86	152	96735	21.64	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	86.56%


Target Compounds					Qvalue
13) Acetone	4.14	43	3400	3.094 ug/L	84
16) Methylene chloride	4.92	84	40508	9.527 ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_W\DATA\VW100318\
Data File : VW005828.D
Acq On : 03 Oct 2018 22:53
Operator : SY/AP
Sample : J5181-12
Misc : 2.62G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
JLC41

Quant Time: Oct 15 08:06:10 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM092818S.M
Quant Title : VOC Analysis
QLast Update : Thu Oct 04 07:04:02 2018
Response via : Initial Calibration




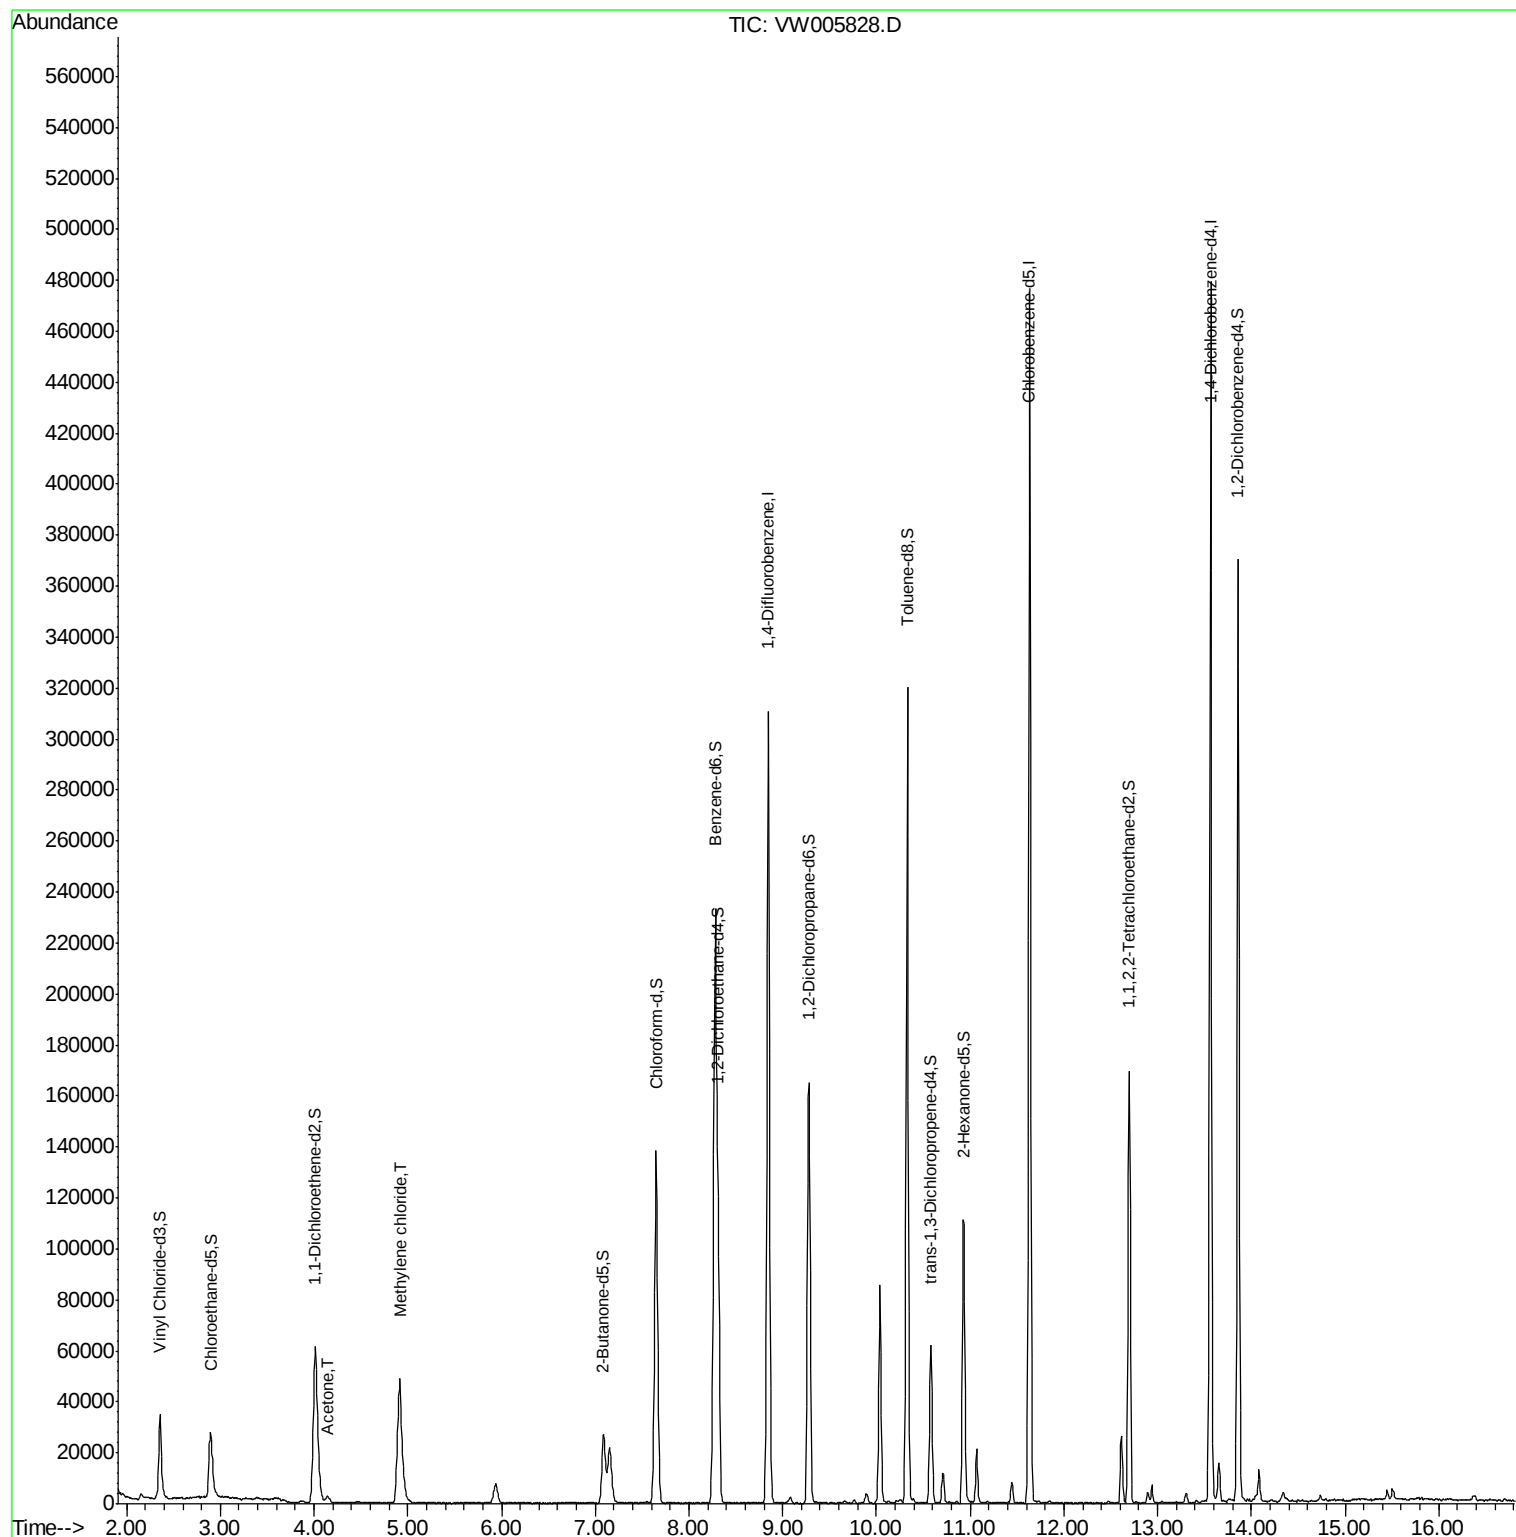


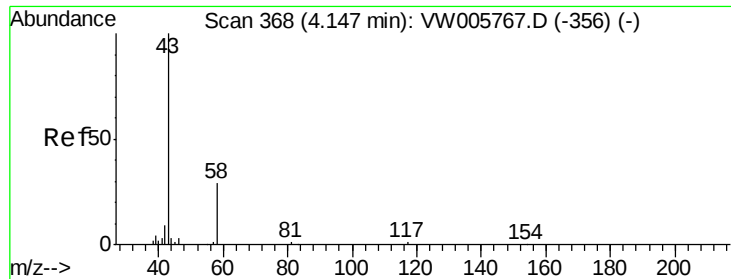

#13
Acetone
Concen: 3.094 ug/L
RT: 4.14 min Scan# 367
Delta R.T. 0.02 min
Lab File: VW005828.D
Acq: 03 Oct 2018 22:53

Instrument :
MSVOA_W
ClientSampled :
JLC41

Tgt Ion: 43 Resp: 3400
Ion Ratio Lower Upper
43 100
58 22.6 0.0 31.8

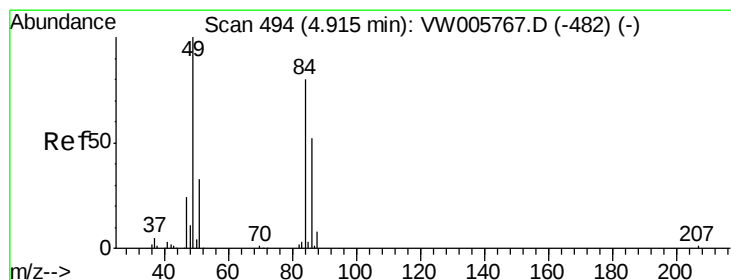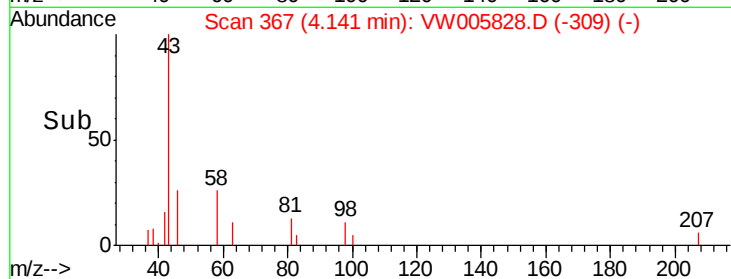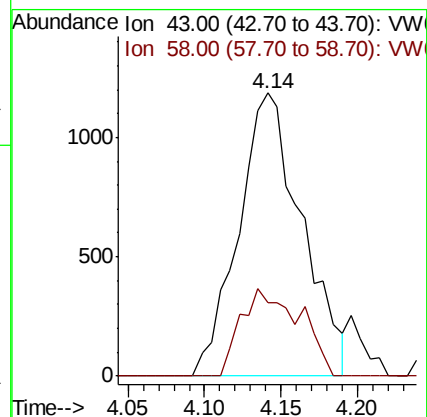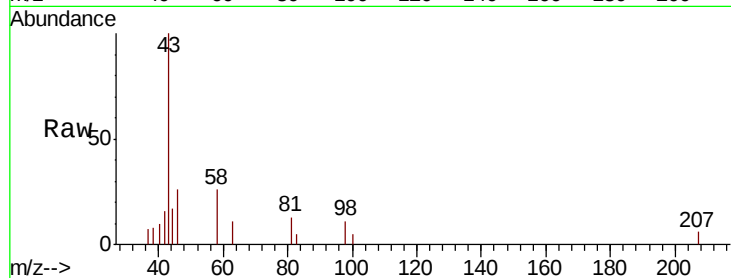

#16
Methylene chloride
Concen: 9.527 ug/L
RT: 4.92 min Scan# 494
Delta R.T. 0.01 min
Lab File: VW005828.D
Acq: 03 Oct 2018 22:53

Tgt Ion: 84 Resp: 40508
Ion Ratio Lower Upper
84 100
49 119.2 87.2 162.0
86 64.8 43.2 80.2

