

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW100319\
 Data File : VW013428.D
 Acq On : 03 Oct 2019 19:10
 Operator : SY/VA
 Sample : K5205-04
 Misc : 6.58G/5ML/MSVOA W/SOIL
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 RBR-200028-RT-3425

Quant Time: Oct 04 09:39:12 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W100119S.M
 Quant Title : SW846 8260
 QLast Update : Wed Oct 02 11:49:57 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.95	168	41206	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.85	114	53819	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.63	117	44511	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.56	152	13823	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.31	65	15896	51.67	ug/l	0.00
Spiked Amount 50.000			Recovery	=	103.34%	
35) Dibromofluoromethane	7.88	113	15583	55.18	ug/l	0.00
Spiked Amount 50.000			Recovery	=	110.36%	
50) Toluene-d8	10.32	98	63070	53.82	ug/l	0.00
Spiked Amount 50.000			Recovery	=	107.64%	
62) 4-Bromofluorobenzene	12.62	95	17205	43.96	ug/l	0.00
Spiked Amount 50.000			Recovery	=	87.92%	
Target Compounds						
16) Acetone	4.12	43	10729	113.766	ug/l	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW100319\
Data File : VW013428.D
Acq On : 03 Oct 2019 19:10
Operator : SY/VA
Sample : K5205-04
Misc : 6.58G/5ML/MSVOA W/SOIL
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
RBR-200028-RT-3425

Quant Time: Oct 04 09:39:12 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\82W100119S.M
Quant Title : SW846 8260
QLast Update : Wed Oct 02 11:49:57 2019
Response via : Initial Calibration

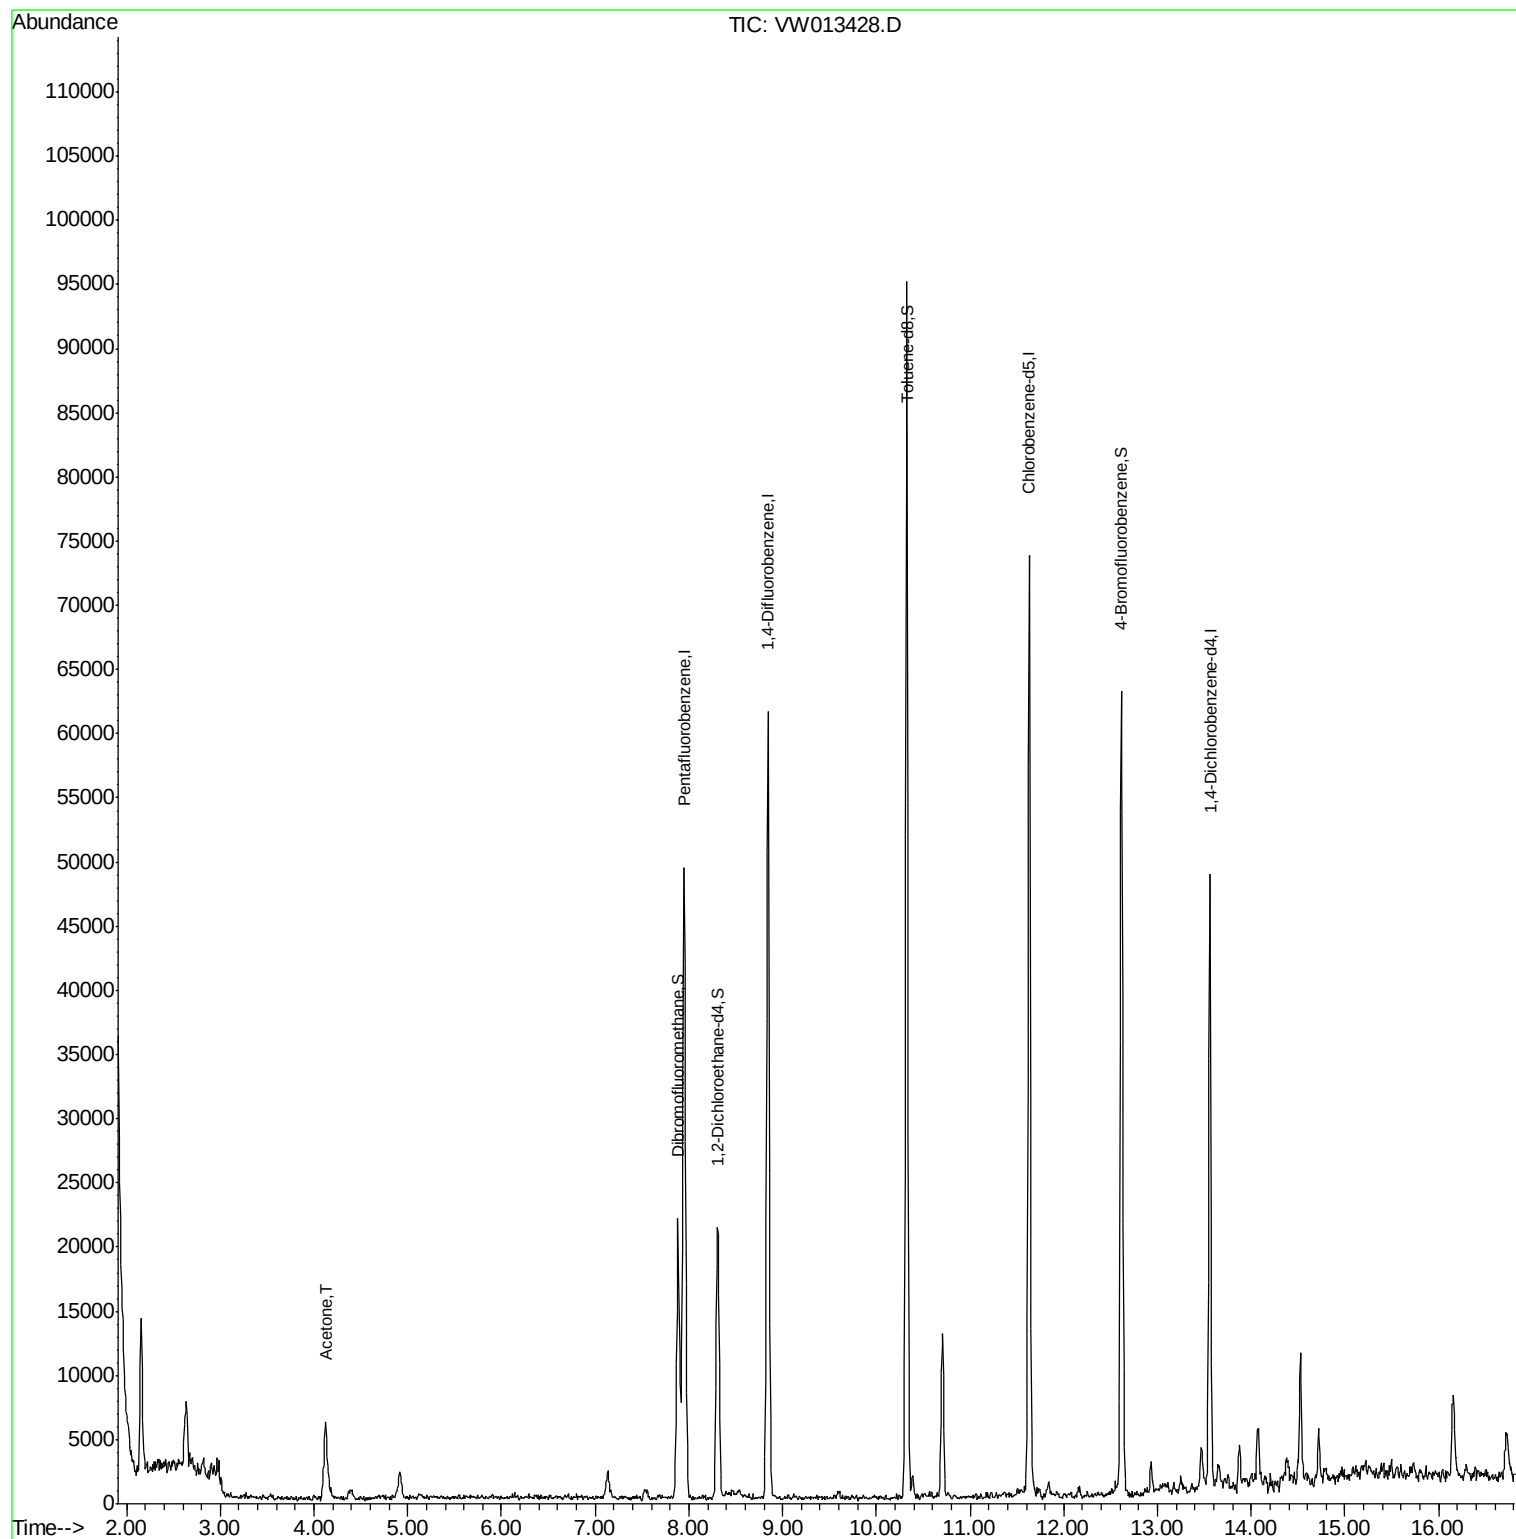

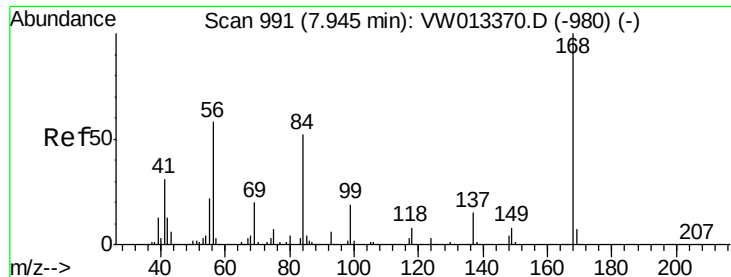

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.95 min Scan# 991

Delta R.T. 0.00 min

Lab File: VW013428.D

Acq: 03 Oct 2019 19:10

Instrument :

MSVOA_W

ClientSampleId :


RBR-200028-RT-3425

Tot Ion:168 Resp: 41206

Ion Ratio Lower Upper




168 100

99 48.1 40.2 60.4



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VW

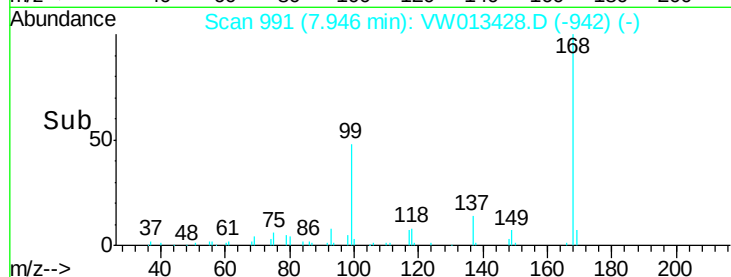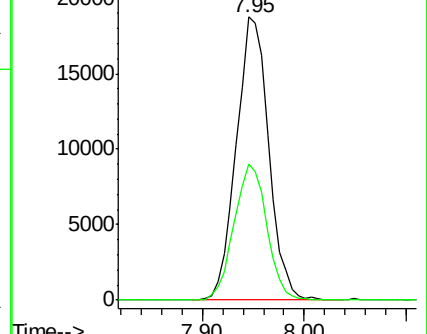

#16

Acetone

Concen: 113.766 ug/l

RT: 4.12 min Scan# 363

Delta R.T. 0.00 min

Lab File: VW013428.D


Acq: 03 Oct 2019 19:10

Tgt Ion: 43 Resp: 10729

Ion Ratio Lower Upper



43 100


58 30.8 24.1 36.1



Abundance Ion 43.00 (42.70 to 43.70): VW

Ion 58.00 (57.70 to 58.70): VW



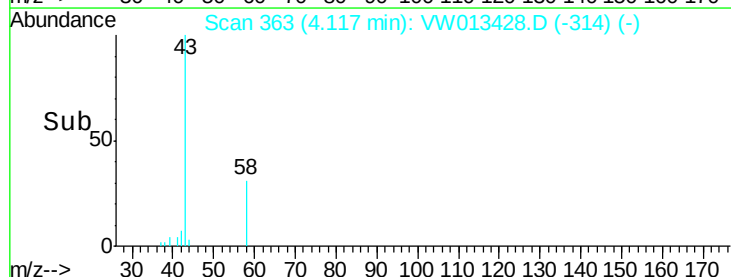
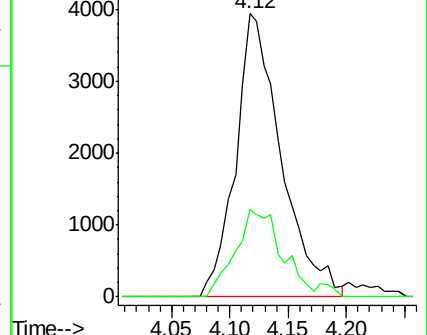


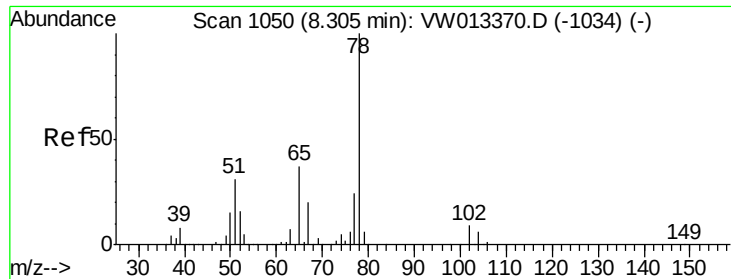

#33
 1,2-Dichloroethane-d4
 Concen: 51.665 ug/l
 RT: 8.31 min Scan# 1050
 Delta R.T. 0.00 min
 Lab File: VW013428.D
 Acq: 03 Oct 2019 19:10




Instrument :
 MSVOA_W
 ClientSampleId :
 RBR-200028-RT-3425


Tot Ion: 65 Resp: 15896
 Ion Ratio Lower Upper
 65 100
 67 55.5 0.0 106.2

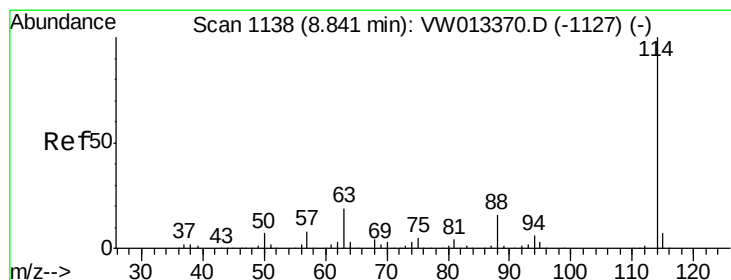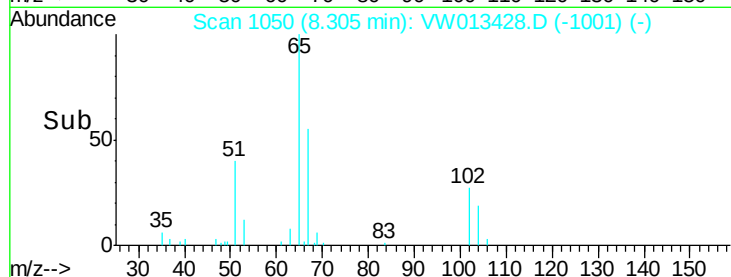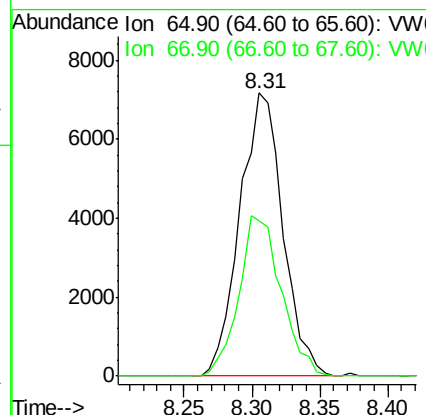

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.85 min Scan# 1139
 Delta R.T. 0.01 min
 Lab File: VW013428.D
 Acq: 03 Oct 2019 19:10

Tgt Ion: 114 Resp: 53819
 Ion Ratio Lower Upper
 114 100
 63 19.2 0.0 41.4
 88 15.1 0.0 32.0

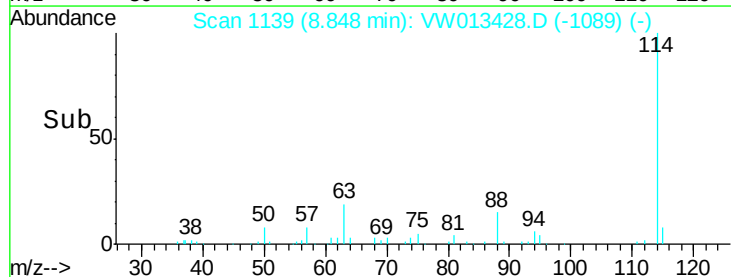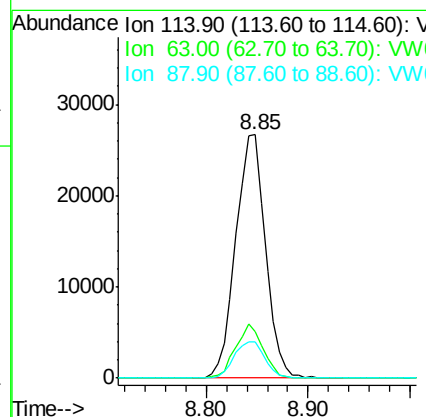

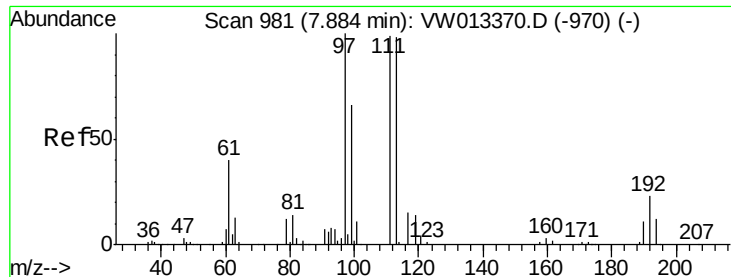

#35

Dibromofluoromethane

Concen: 55.180 ug/l

RT: 7.88 min Scan# 981

Delta R.T. 0.00 min

Lab File: VW013428.D

Acq: 03 Oct 2019 19:10

Instrument :

MSVOA_W

ClientSampleId :

RBR-200028-RT-3425


Tot Ion:113 Resp: 15583

Ion Ratio Lower Upper

113 100

111 101.5 81.9 122.9




192 25.3 19.1 28.7

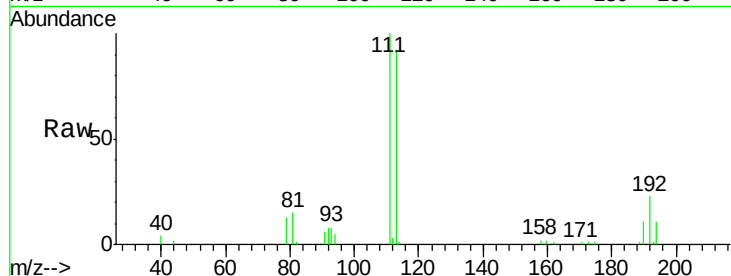

Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

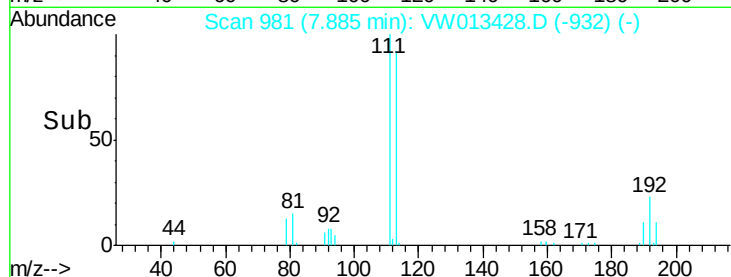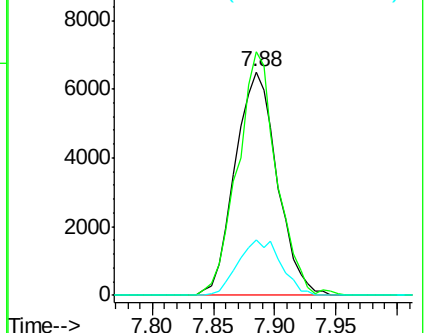

#50

Toluene-d8

Concen: 53.818 ug/l

RT: 10.32 min Scan# 1381

Delta R.T. 0.00 min

Lab File: VW013428.D


Acq: 03 Oct 2019 19:10

Tgt Ion: 98 Resp: 63070

Ion Ratio Lower Upper



98 100


100 65.0 52.9 79.3



Abundance Ion 98.00 (97.70 to 98.70): VW

Ion 100.00 (99.70 to 100.70): VW

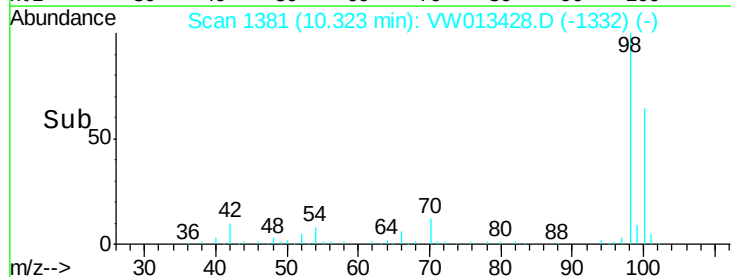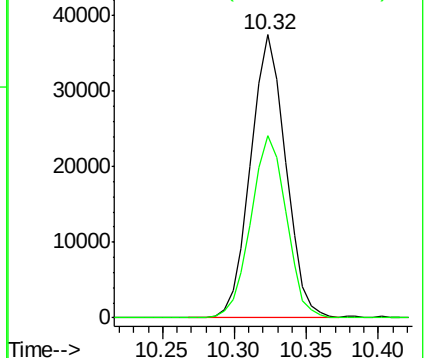

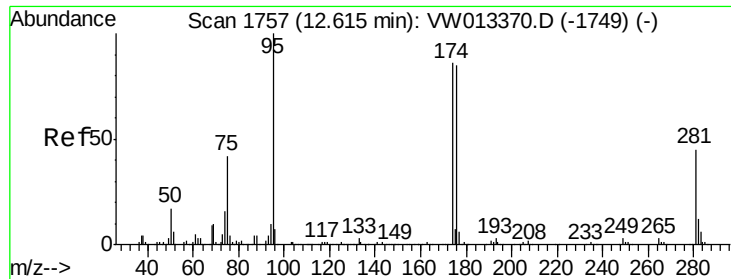

#62

4-Bromofluorobenzene

Concen: 43.964 ug/l

RT: 12.62 min Scan# 1757

Delta R.T. 0.00 min

Lab File: VW013428.D

Acq: 03 Oct 2019 19:10

Instrument :

MSVOA_W

ClientSampleId :

RBR-200028-RT-3425


Tot Ion: 95 Resp: 17205

Ion Ratio Lower Upper

95 100

174 91.8 0.0 178.4




176 86.5 0.0 172.2

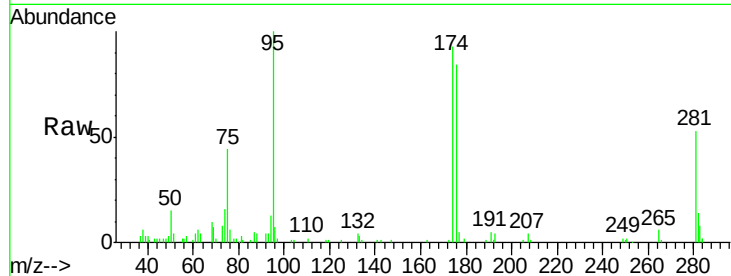

Abundance Ion 94.90 (94.60 to 95.60): VW

Ion 173.80 (173.50 to 174.50): VW

Ion 175.80 (175.50 to 176.50): VW

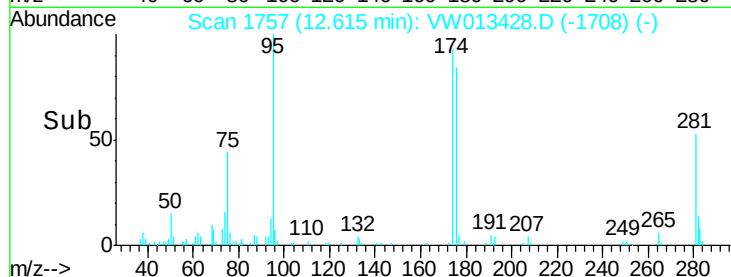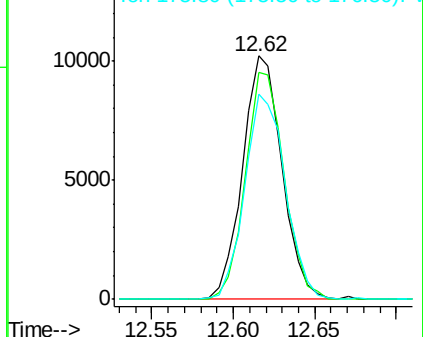

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.63 min Scan# 1596

Delta R.T. 0.00 min

Lab File: VW013428.D

Acq: 03 Oct 2019 19:10


Tgt Ion: 117 Resp: 44511

Ion Ratio Lower Upper

117 100

82 51.8 45.9 68.9



119 34.4 26.2 39.2




Abundance Ion 116.90 (116.60 to 117.60): VW

Ion 82.00 (81.70 to 82.70): VW

Ion 118.90 (118.60 to 119.60): VW

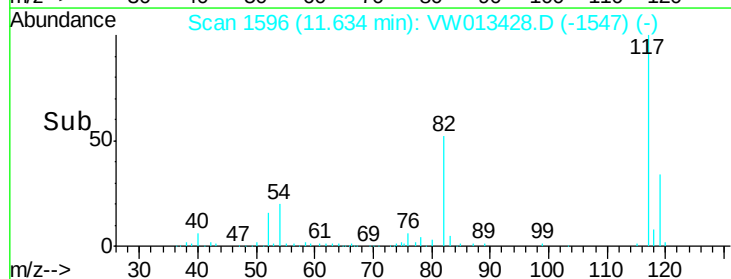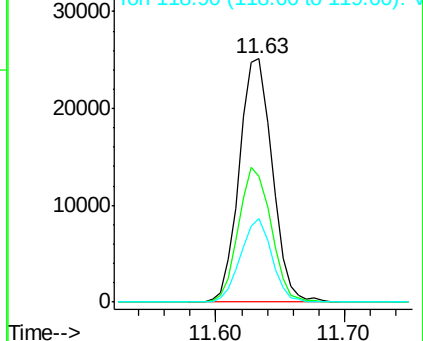

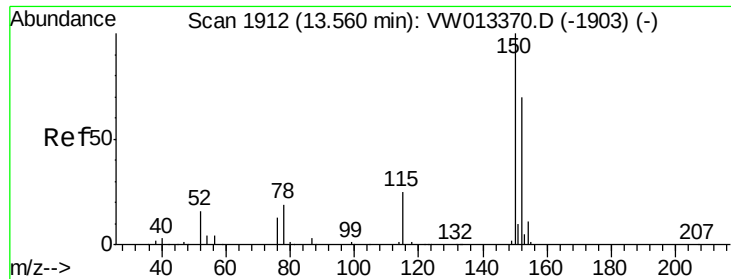

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.56 min Scan# 1912

Delta R.T. 0.00 min

Lab File: VW013428.D


Acq: 03 Oct 2019 19:10

Instrument :

MSVOA_W

ClientSampleId :

RBR-200028-RT-3425




Tot Ion:152 Resp: 13823

Ion Ratio Lower Upper

152 100

115 57.7 27.3 81.9

150 158.4 0.0 349.0

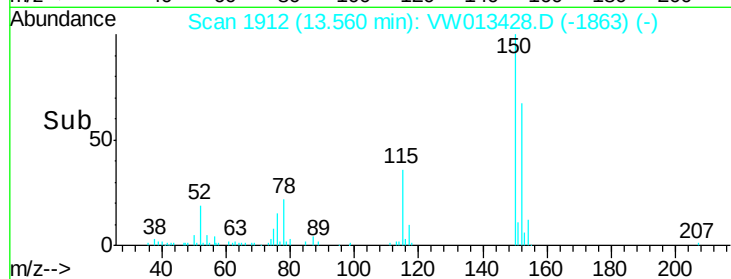

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

