


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW100418\  
Data File : VW005832.D  
Acq On : 04 Oct 2018 02:20  
Operator : SY/AP  
Sample : BFB  
Misc : 5.00G/5ML/MSVOA W/SOIL  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
MSVOA\_W  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_W\METHOD\82W100418S.M  
Title : SW846 8260  
Last Update : Thu Oct 04 07:08:57 2018

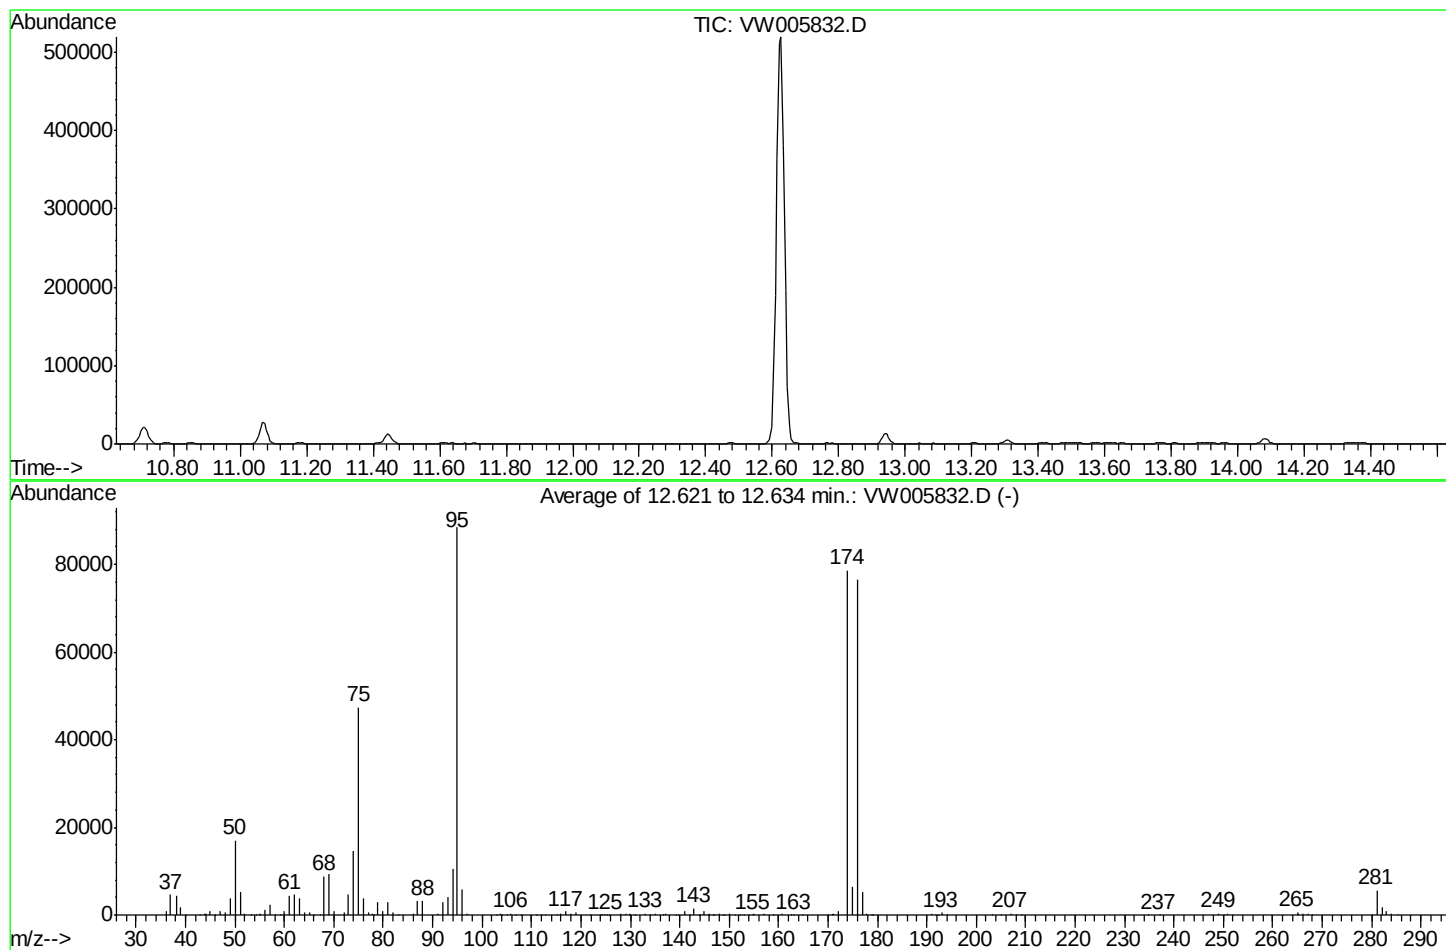

AutoFind: Scans 1758, 1759, 1760; Background Corrected with Scan 1749

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 19.3      | 17033   | PASS             |
| 75          | 95           | 30           | 60           | 53.6      | 47442   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 88464   | PASS             |
| 96          | 95           | 5            | 9            | 6.6       | 5875    | PASS             |
| 173         | 174          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 174         | 95           | 50           | 100          | 89.0      | 78709   | PASS             |
| 175         | 174          | 5            | 9            | 8.0       | 6331    | PASS             |
| 176         | 174          | 95           | 101          | 97.1      | 76458   | PASS             |
| 177         | 176          | 5            | 9            | 6.8       | 5183    | PASS             |