


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW100419\
Data File : VW013430.D
Acq On : 04 Oct 2019 10:08
Operator : SY/VA
Sample : BFB
Misc : 5.00G/5ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W100119S.M
Title : SW846 8260
Last Update : Wed Oct 02 11:49:57 2019

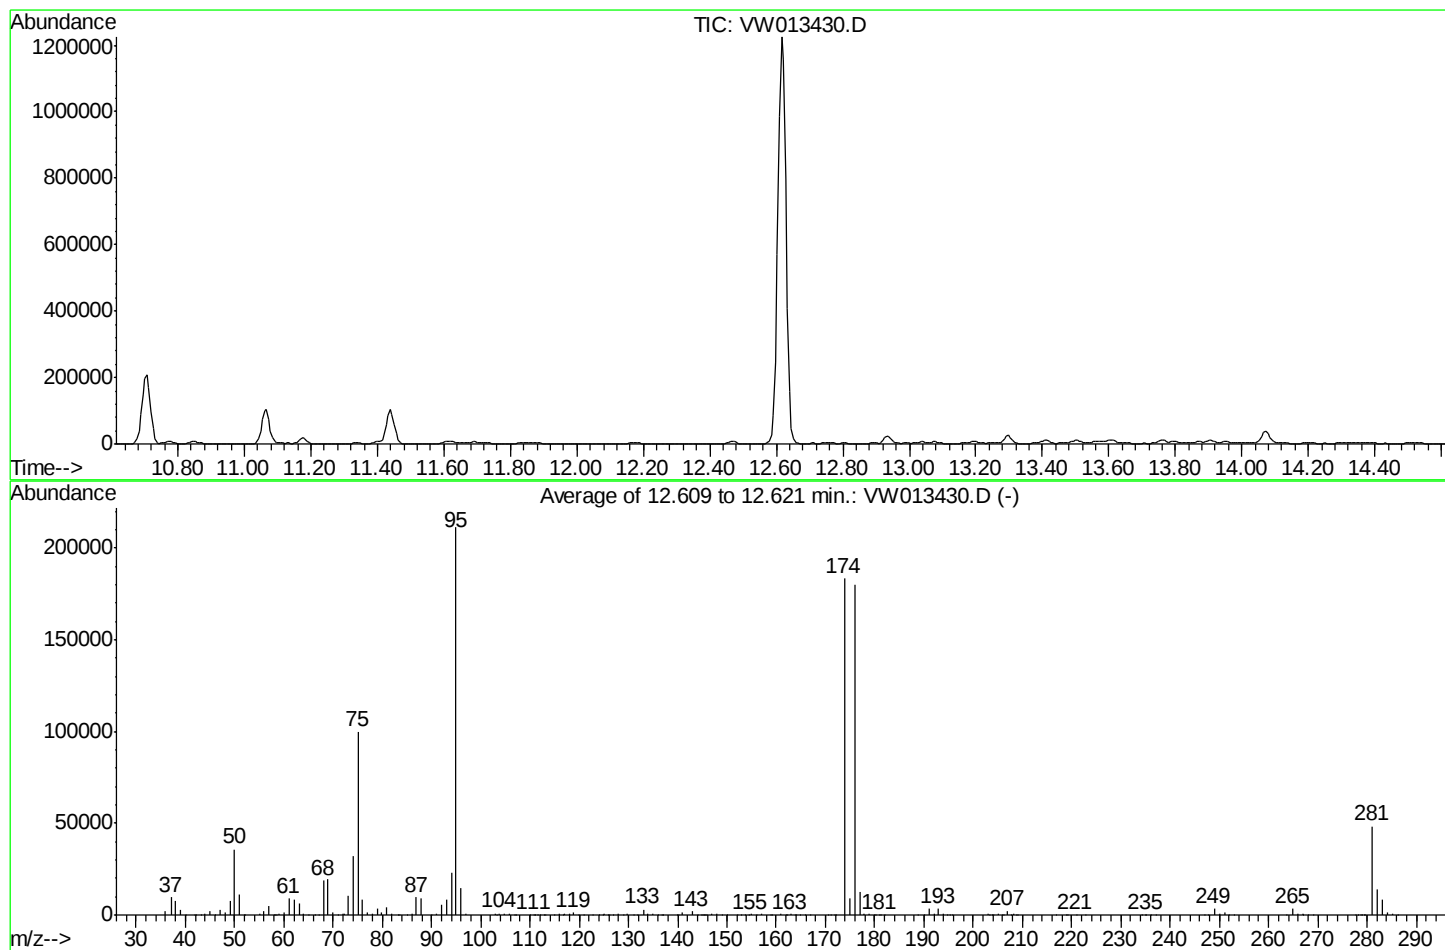

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1748

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	35800	PASS
75	95	30	60	47.3	100002	PASS
95	95	100	100	100.0	211285	PASS
96	95	5	9	6.8	14403	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	86.8	183360	PASS
175	174	5	9	5.0	9211	PASS
176	174	95	101	98.1	179818	PASS
177	176	5	9	7.2	12871	PASS