




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100523\
 Data File : VW027238.D
 Acq On : 05 Oct 2023 16:06
 Operator : SY/MD
 Sample : 04747-20
 Misc : 3.42g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EX849

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 10/07/2023
 Supervised By :Mahesh Dadoda 10/09/2023

10/07/2023
 Supervised By :Mahesh
 Dadoda

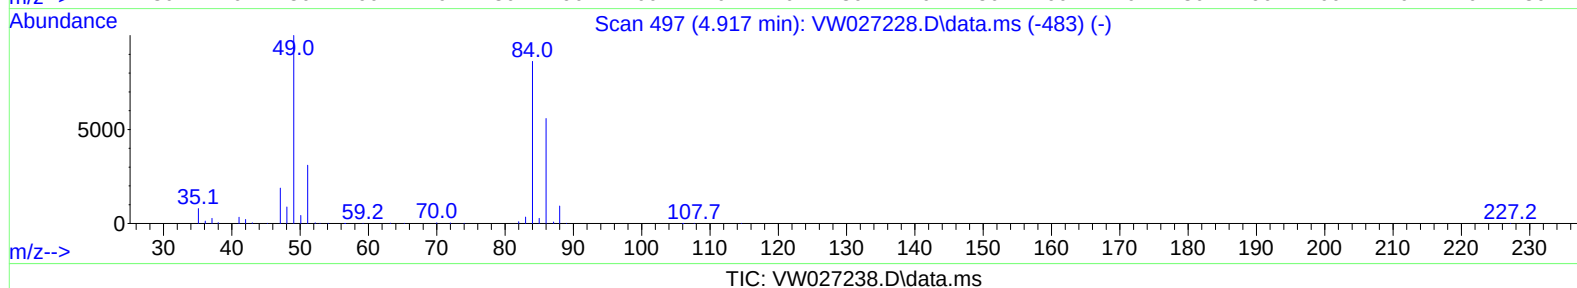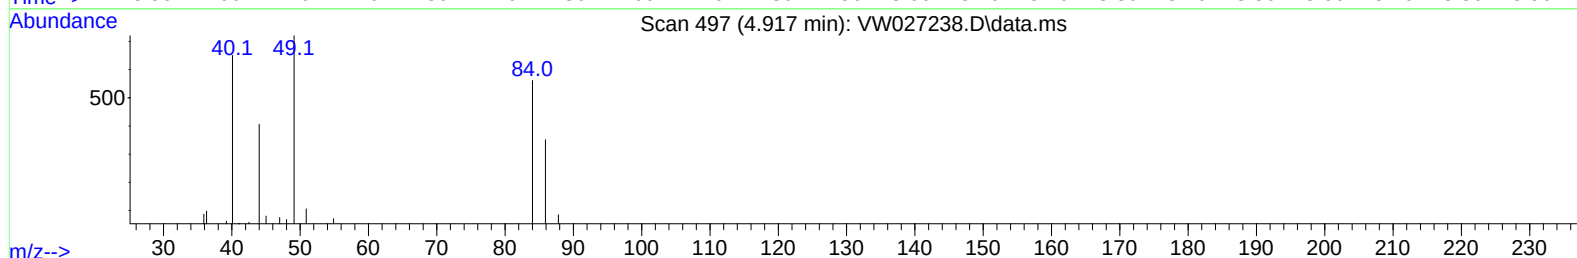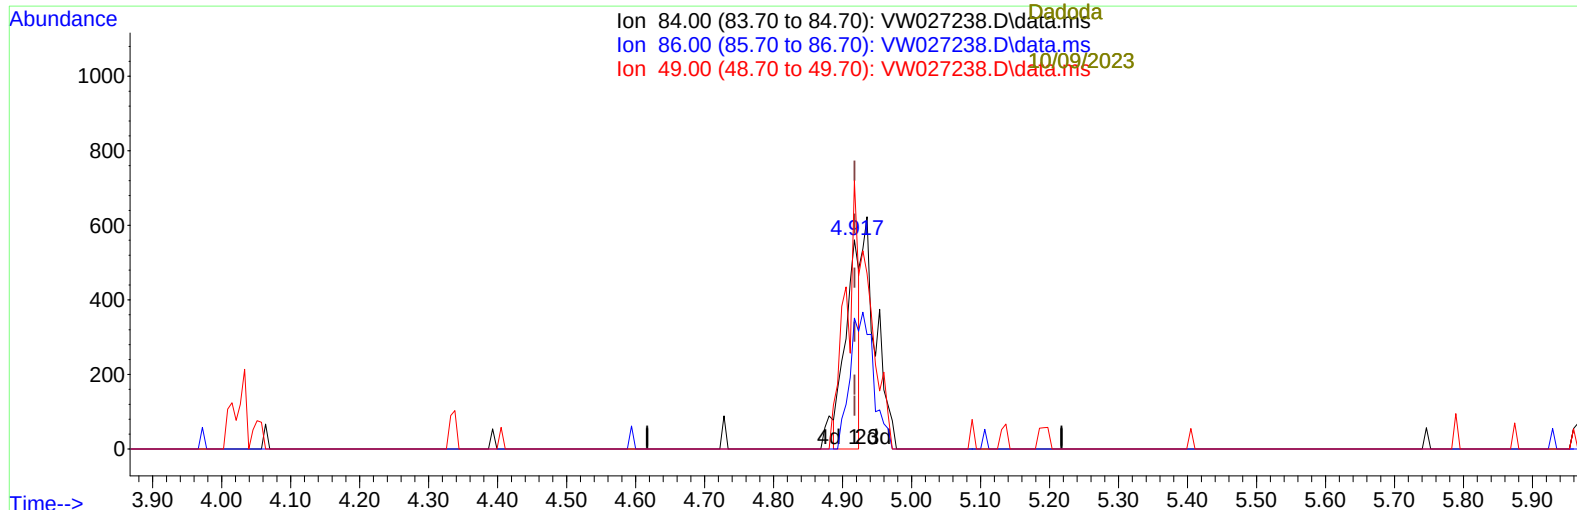

(16) Methylene chloride (T)

4.917min (-0.000) 1.98 ug/L

response 799

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	64.50	62.57
49.00	115.60	128.34
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100523\
Data File : VW027238.D
Acq On : 05 Oct 2023 16:06
Operator : SY/MD
Sample : 04747-20
Misc : 3.42g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EX849




Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 10/07/2023
Supervised By :Mahesh Dadoda 10/09/2023

Quant Time: Oct 06 01:25:59 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092723SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Oct 04 22:49:04 2023
Response via : Initial Calibration

10/07/2023
Supervised By :Mahesh
Dadoda

10/09/2023

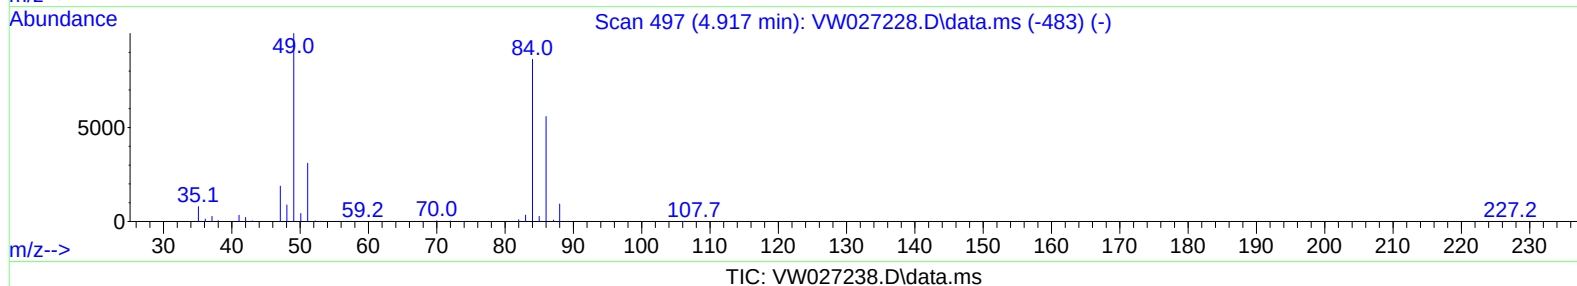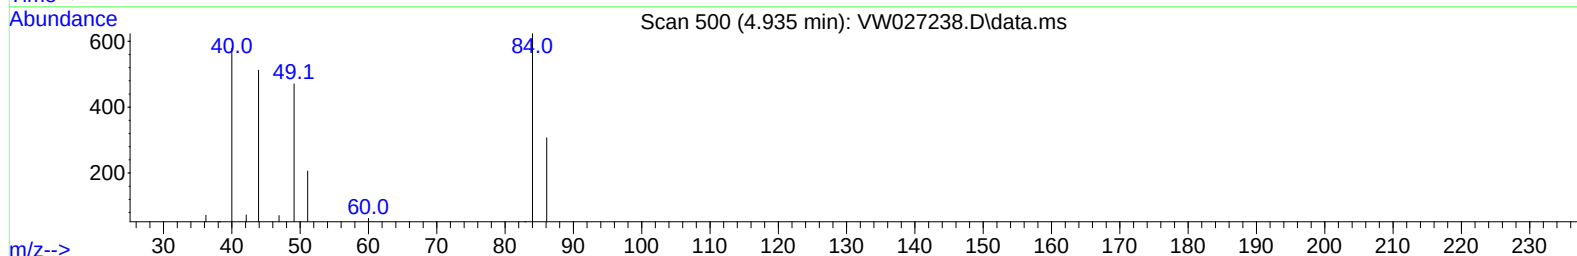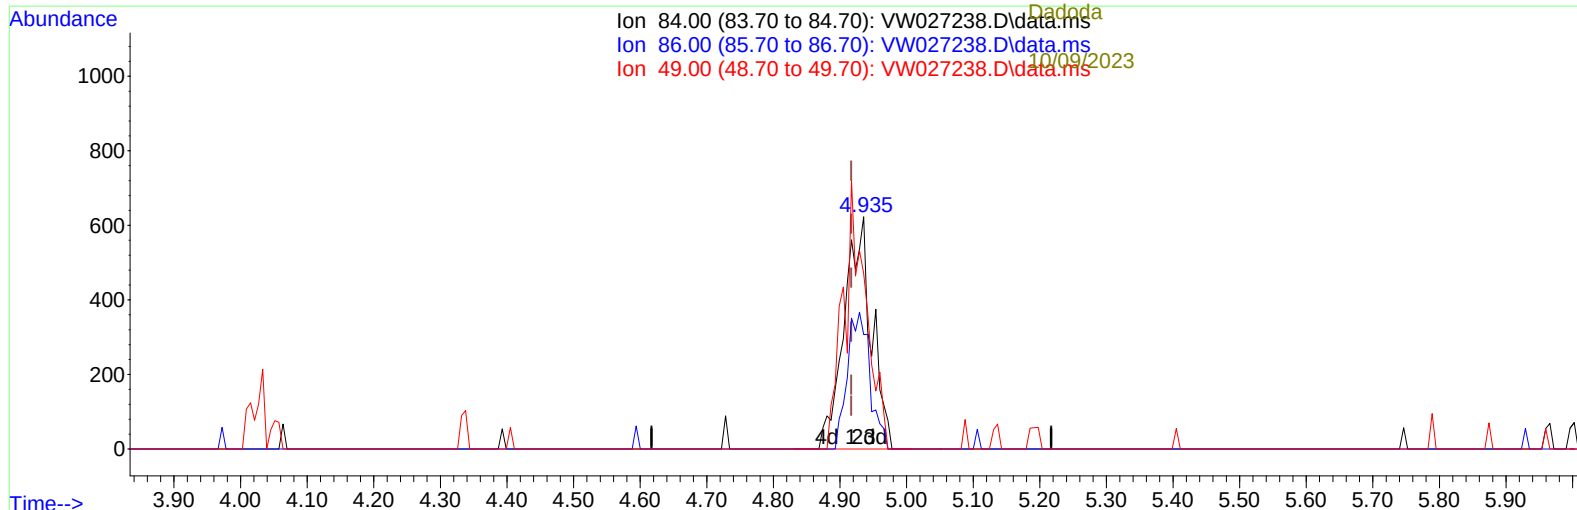

TIC: VW027238.D\data.ms

(16) Methylene chloride (T)

4.935min (+ 0.018) 4.40 ug/L m

response 1778

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	64.50	49.28
49.00	115.60	75.60#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100523\
Data File : VW027238.D
Acq On : 05 Oct 2023 16:06
Operator : SY/MD
Sample : 04747-20
Misc : 3.42g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EX849




Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 10/07/2023
Supervised By :Mahesh Dadoda 10/09/2023

Quant Time: Oct 06 01:25:59 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092723SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Oct 04 22:49:04 2023
Response via : Initial Calibration

10/07/2023
Supervised By :Mahesh
Dadoda

10/09/2023

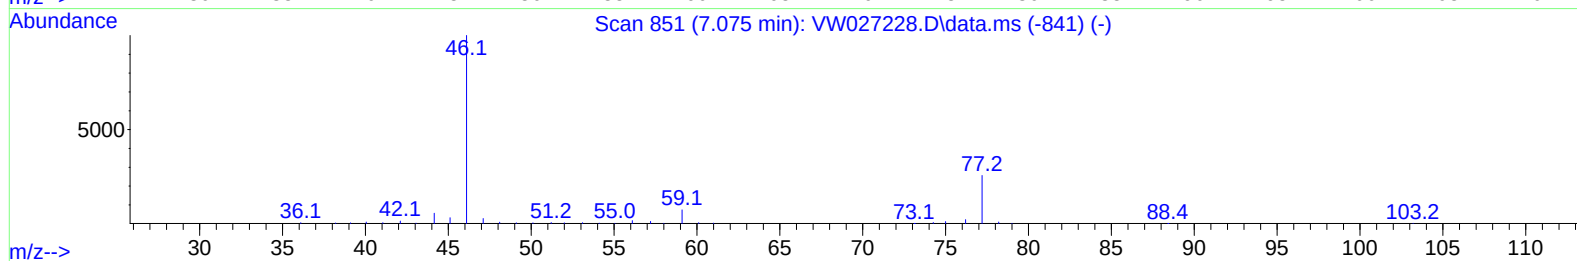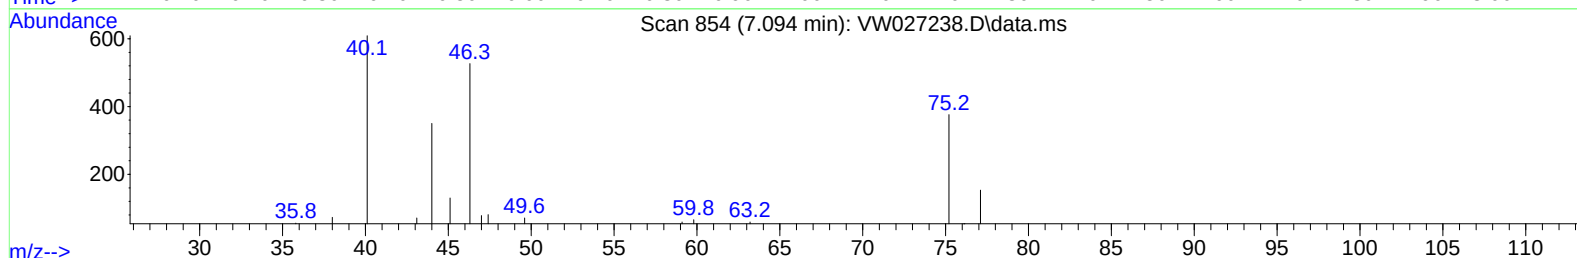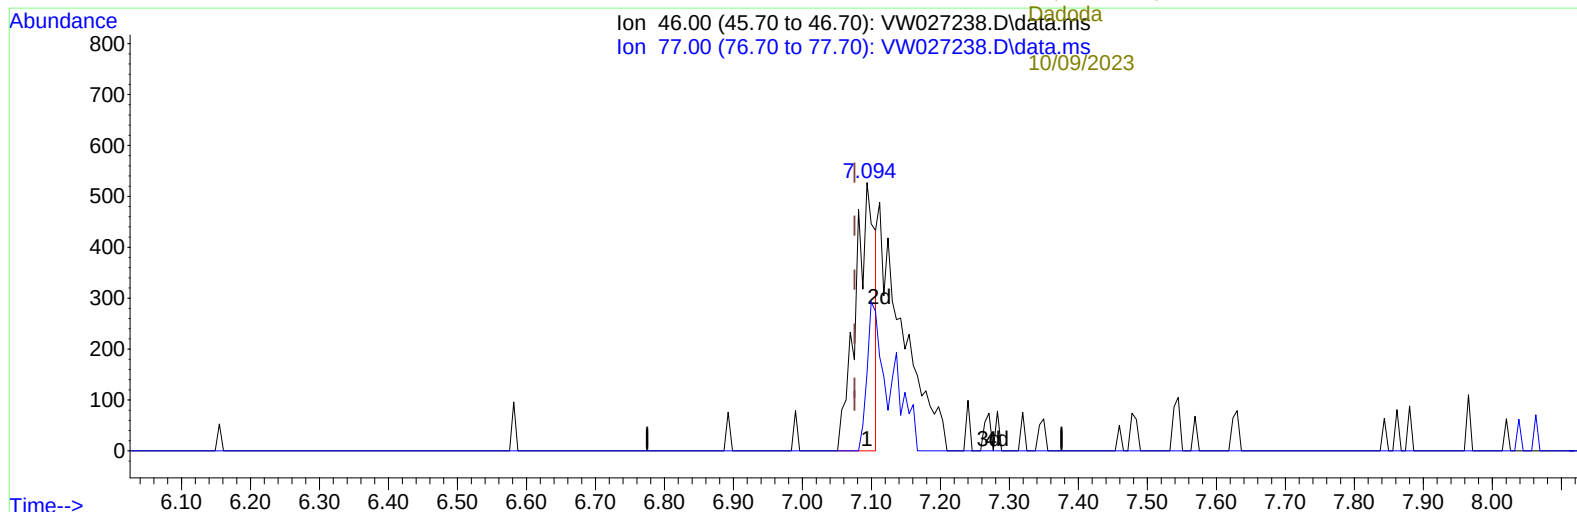

TIC: VW027238.D\data.ms

(21) 2-Butanone-d5 (S)

7.094min (+ 0.018) 15.24 ug/L

response 1021

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	25.90	42.31#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100523\
 Data File : VW027238.D
 Acq On : 05 Oct 2023 16:06
 Operator : SY/MD
 Sample : 04747-20
 Misc : 3.42g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1




Instrument :
 MSVOA_W
 ClientSampleId :
 EX849

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 10/07/2023
 Supervised By :Mahesh Dadoda 10/09/2023

10/07/2023
 Supervised By :Mahesh
 Dadoda

10/09/2023

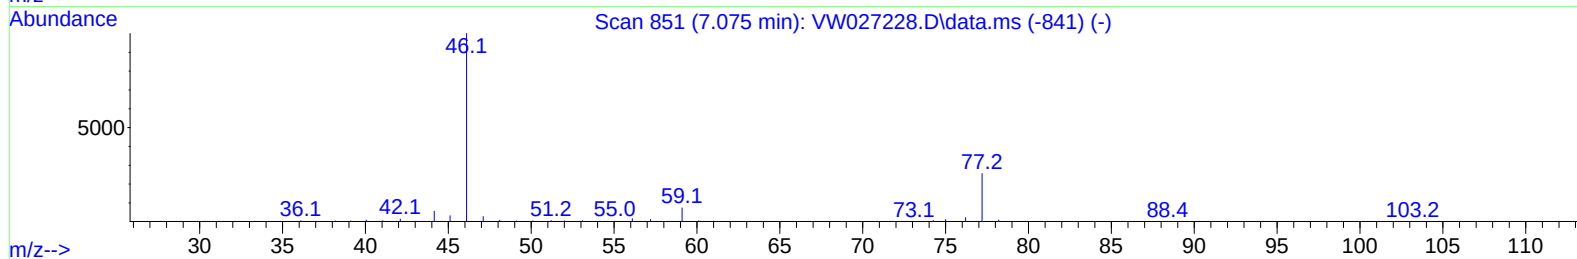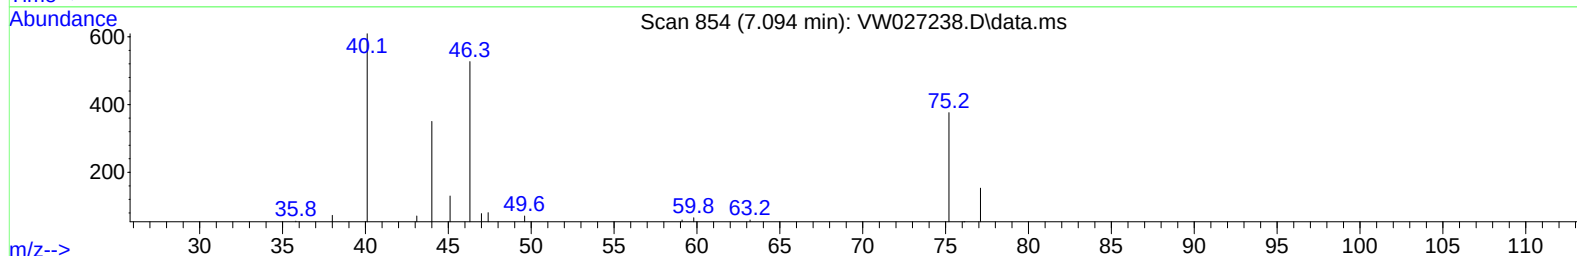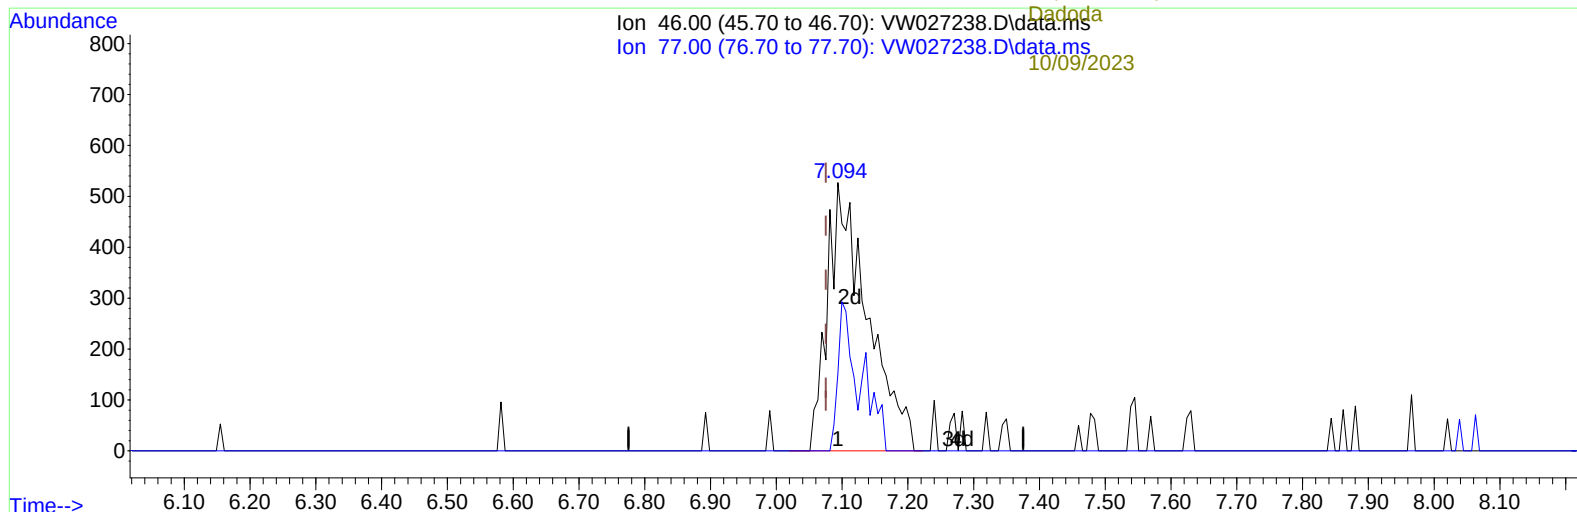

TIC: VW027238.D\data.ms

(21) 2-Butanone-d5 (S)

7.094min (+ 0.018) 33.26 ug/L m

response 2229

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	25.90	19.38
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100523\
 Data File : VW027238.D
 Acq On : 05 Oct 2023 16:06
 Operator : SY/MD
 Sample : 04747-20
 Misc : 3.42g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EX849

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 10/07/2023
 Supervised By :Mahesh Dadoda 10/09/2023

Quant Time: Oct 06 01:25:59 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092723SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Oct 04 22:49:04 2023
 Response via : Initial Calibration

10/07/2023
 Supervised By :Mahesh
 Dadoda

10/09/2023

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	20631	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	17949	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.562	152	5280	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.351	65	10954	33.793	ug/L	-0.02
Spiked Amount	25.000	Range 30 - 150	Recovery	= 135.160%		
7) Chloroethane-d5	2.899	69	8834	34.482	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	= 137.920%		
11) 1,1-Dichloroethene-d2	4.039	65	3707	27.526	ug/L	0.02
Spiked Amount	25.000	Range 45 - 110	Recovery	= 110.120%#		
21) 2-Butanone-d5	7.094	46	2229m	33.264	ug/L	0.02
Spiked Amount	50.000	Range 20 - 135	Recovery	= 66.520%		
24) Chloroform-d	7.648	84	15997	26.494	ug/L	0.00
Spiked Amount	25.000	Range 40 - 150	Recovery	= 105.960%		
26) 1,2-Dichloroethane-d4	8.313	65	9355	32.329	ug/L	0.00
Spiked Amount	25.000	Range 70 - 130	Recovery	= 129.320%		
32) Benzene-d6	8.276	84	34639	31.489	ug/L	0.00
Spiked Amount	25.000	Range 20 - 135	Recovery	= 125.960%		
36) 1,2-Dichloropropane-d6	9.270	67	11423	34.686	ug/L	0.00
Spiked Amount	25.000	Range 70 - 120	Recovery	= 138.760%#		
41) Toluene-d8	10.325	98	21648	22.301	ug/L	0.00
Spiked Amount	25.000	Range 30 - 130	Recovery	= 89.200%		
43) trans-1,3-Dichloroprop...	10.575	79	2875	22.245	ug/L	0.00
Spiked Amount	25.000	Range 30 - 135	Recovery	= 89.000%		
47) 2-Hexanone-d5	0.000	63	0d	0.000	ug/L	
Spiked Amount	50.000	Range 20 - 135	Recovery	= 0.000%#		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	7040	27.932	ug/L	0.00
Spiked Amount	25.000	Range 45 - 120	Recovery	= 111.720%		
66) 1,2-Dichlorobenzene-d4	13.848	152	4621	26.102	ug/L	0.00
Spiked Amount	25.000	Range 75 - 120	Recovery	= 104.400%		
Target Compounds						Qvalue
16) Methylene chloride	4.935	84	1778m	4.402	ug/L	
34) Trichloroethene	9.093	95	23882	72.088	ug/L	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100523\
Data File : VW027238.D
Acq On : 05 Oct 2023 16:06
Operator : SY/MD
Sample : 04747-20
Misc : 3.42g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EX849

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 10/07/2023
Supervised By :Mahesh Dadoda 10/09/2023

10/07/2023
Supervised By :Mahesh
Dadoda

10/09/2023

Quant Time: Oct 06 01:25:59 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092723SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Oct 04 22:49:04 2023
Response via : Initial Calibration

