




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100523\
Data File : VW027243.D
Acq On : 05 Oct 2023 18:06
Operator : SY/MD
Sample : 04747-16
Misc : 1.63g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EX845

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 10/07/2023
Supervised By :Mahesh Dadoda 10/09/2023

Quant Time: Oct 06 01:26:46 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092723SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Oct 04 22:49:04 2023
Response via : Initial Calibration

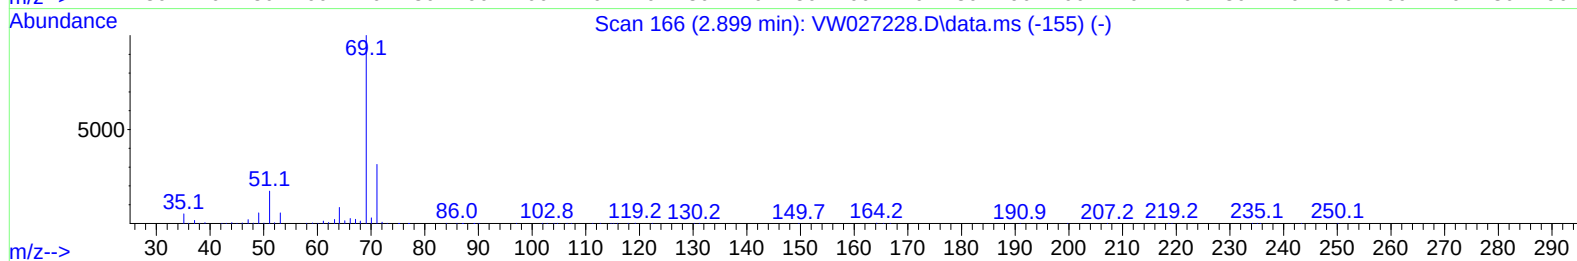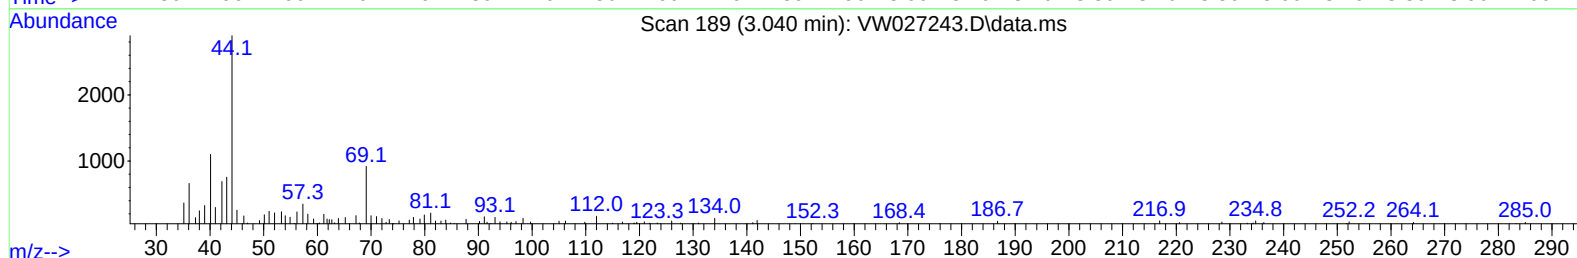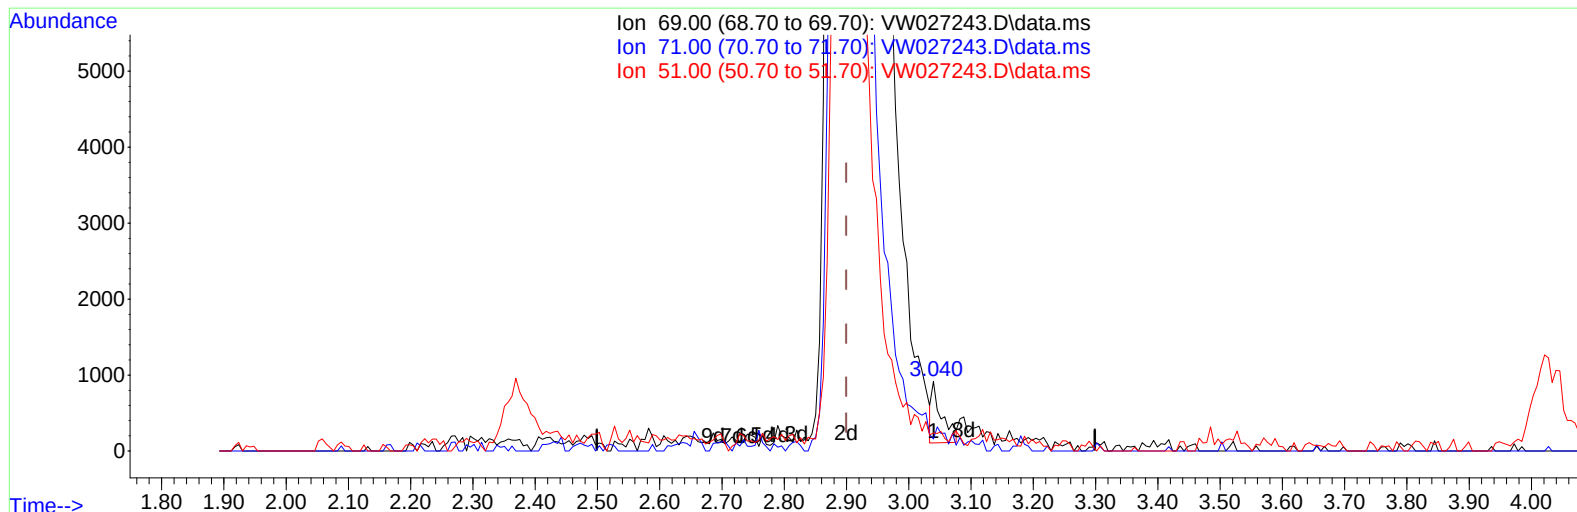

TIC: VW027243.D\data.ms

(7) Chloroethane-d5 (S)

3.040min (+ 0.140) 0.07 ug/L

response 903

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	31.60	35.55
51.00	25.20	25.91
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100523\
 Data File : VW027243.D
 Acq On : 05 Oct 2023 18:06
 Operator : SY/MD
 Sample : 04747-16
 Misc : 1.63g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EX845

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 10/07/2023
 Supervised By :Mahesh Dadoda 10/09/2023

Quant Time: Oct 06 01:26:46 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092723SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Oct 04 22:49:04 2023
 Response via : Initial Calibration

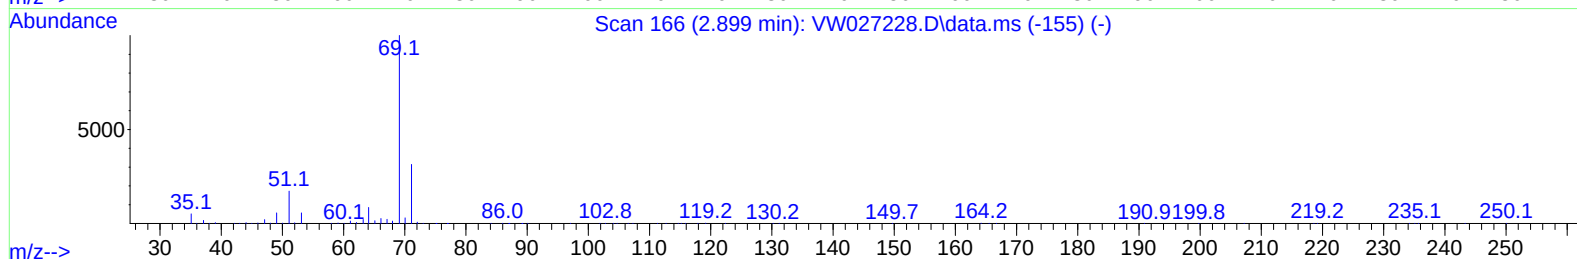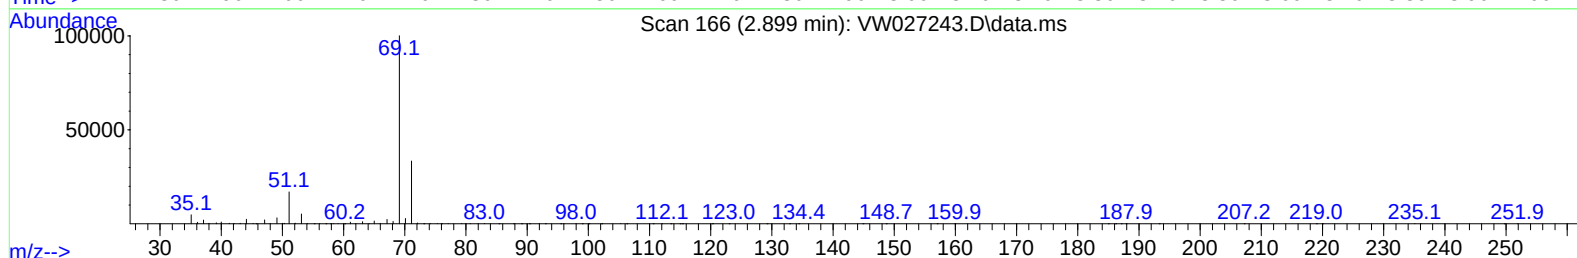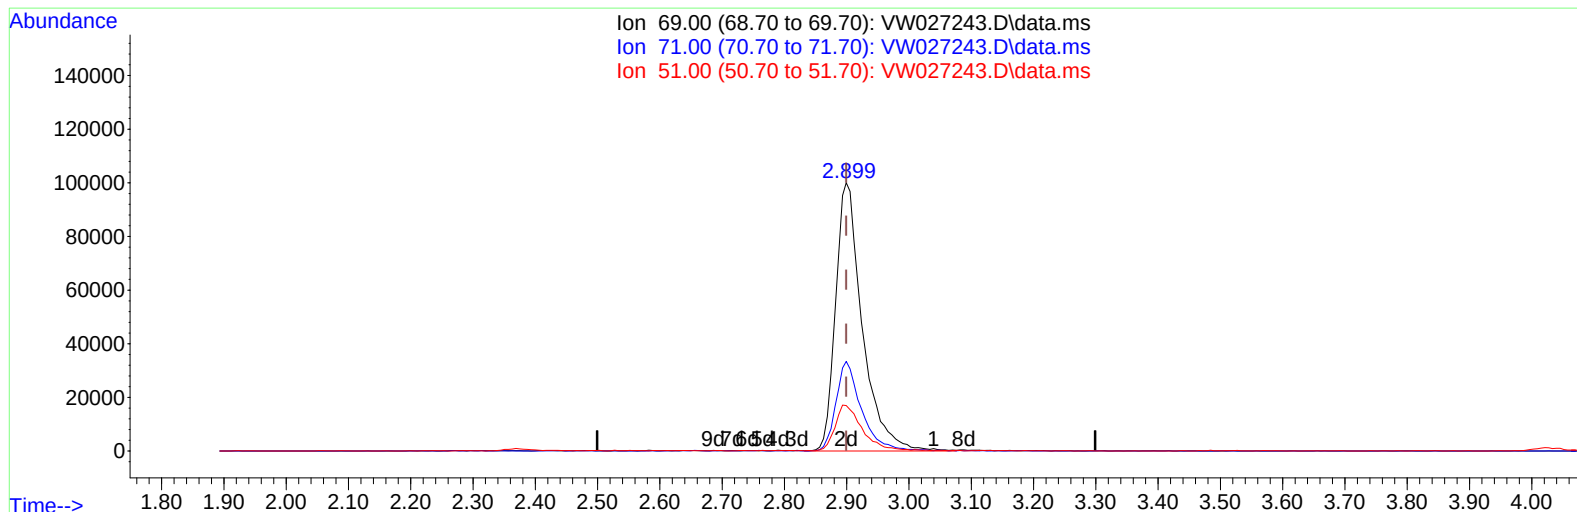

TIC: VW027243.D\data.ms

(7) Chloroethane-d5 (S)

2.899min (+ 0.000) 23.23 ug/L m

response 298168

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	31.60	0.11#
51.00	25.20	0.08#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100523\
 Data File : VW027243.D
 Acq On : 05 Oct 2023 18:06
 Operator : SY/MD
 Sample : 04747-16
 Misc : 1.63g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EX845

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 10/07/2023
 Supervised By :Mahesh Dadoda 10/09/2023

Quant Time: Oct 06 01:26:46 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092723SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Oct 04 22:49:04 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	1033526	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	969169	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	431867	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.369	65	345342	21.267	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	85.080%		
7) Chloroethane-d5	2.899	69	298168m	23.233	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	92.920%		
11) 1,1-Dichloroethene-d2	4.021	65	132272	19.606	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	78.440%		
21) 2-Butanone-d5	7.075	46	166452	49.585	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	99.160%		
24) Chloroform-d	7.648	84	656731	21.711	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	86.840%		
26) 1,2-Dichloroethane-d4	8.307	65	327544	22.595	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	90.400%		
32) Benzene-d6	8.276	84	1317420	22.180	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	88.720%		
36) 1,2-Dichloropropane-d6	9.276	67	435075	24.467	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	97.880%		
41) Toluene-d8	10.325	98	1123522	21.436	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	85.760%		
43) trans-1,3-Dichloroprop...	10.575	79	154848	22.189	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	88.760%		
47) 2-Hexanone-d5	10.922	63	114958	42.261	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	84.520%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	349249	25.663	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	102.640%		
66) 1,2-Dichlorobenzene-d4	13.855	152	340372	23.506	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	94.040%		
Target Compounds						
16) Methylene chloride	4.923	84	54919	2.714	ug/L	95
34) Trichloroethene	9.093	95	20927	1.170	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100523\
Data File : VW027243.D
Acq On : 05 Oct 2023 18:06
Operator : SY/MD
Sample : 04747-16
Misc : 1.63g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EX845

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 10/07/2023
Supervised By :Mahesh Dadoda 10/09/2023

Quant Time: Oct 06 01:26:46 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092723SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Oct 04 22:49:04 2023
Response via : Initial Calibration

