

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW100618\
 Data File : VW005878.D
 Acq On : 05 Oct 2018 04:23
 Operator : SY/AP
 Sample : J5204-01RE
 Misc : 7.06G/5ML/MSVOA W/SOIL
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 SU-04-100318-ARE

Quant Time: Oct 05 05:15:42 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W100418S.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 04 07:08:57 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	0.00	168	0	0.00	ug/l	-7.95
34) 1,4-Difluorobenzene	0.00	114	0	0.00	ug/l	-8.85
63) Chlorobenzene-d5	11.64	117	23	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	0.00	152	0	0.00	ug/l	-13.57

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	0.00	65	0	0.00	ug/l	
Spiked Amount						
			Recovery	=	0.00%	
35) Dibromofluoromethane	0.00	113	0	0.00	ug/l	
Spiked Amount						
			Recovery	=	0.00%	
50) Toluene-d8	0.00	98	0	0.00	ug/l	
Spiked Amount						
			Recovery	=	0.00%	
62) 4-Bromofluorobenzene	0.00	95	0	0.00	ug/l	
Spiked Amount						
			Recovery	=	0.00%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW100618\
Data File : VW005878.D
Acq On : 05 Oct 2018 04:23
Operator : SY/AP
Sample : J5204-01RE
Misc : 7.06G/5ML/MSVOA W/SOIL
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
SU-04-100318-ARE

Quant Time: Oct 05 05:15:42 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\82W100418S.M
Quant Title : SW846 8260
QLast Update : Thu Oct 04 07:08:57 2018
Response via : Initial Calibration

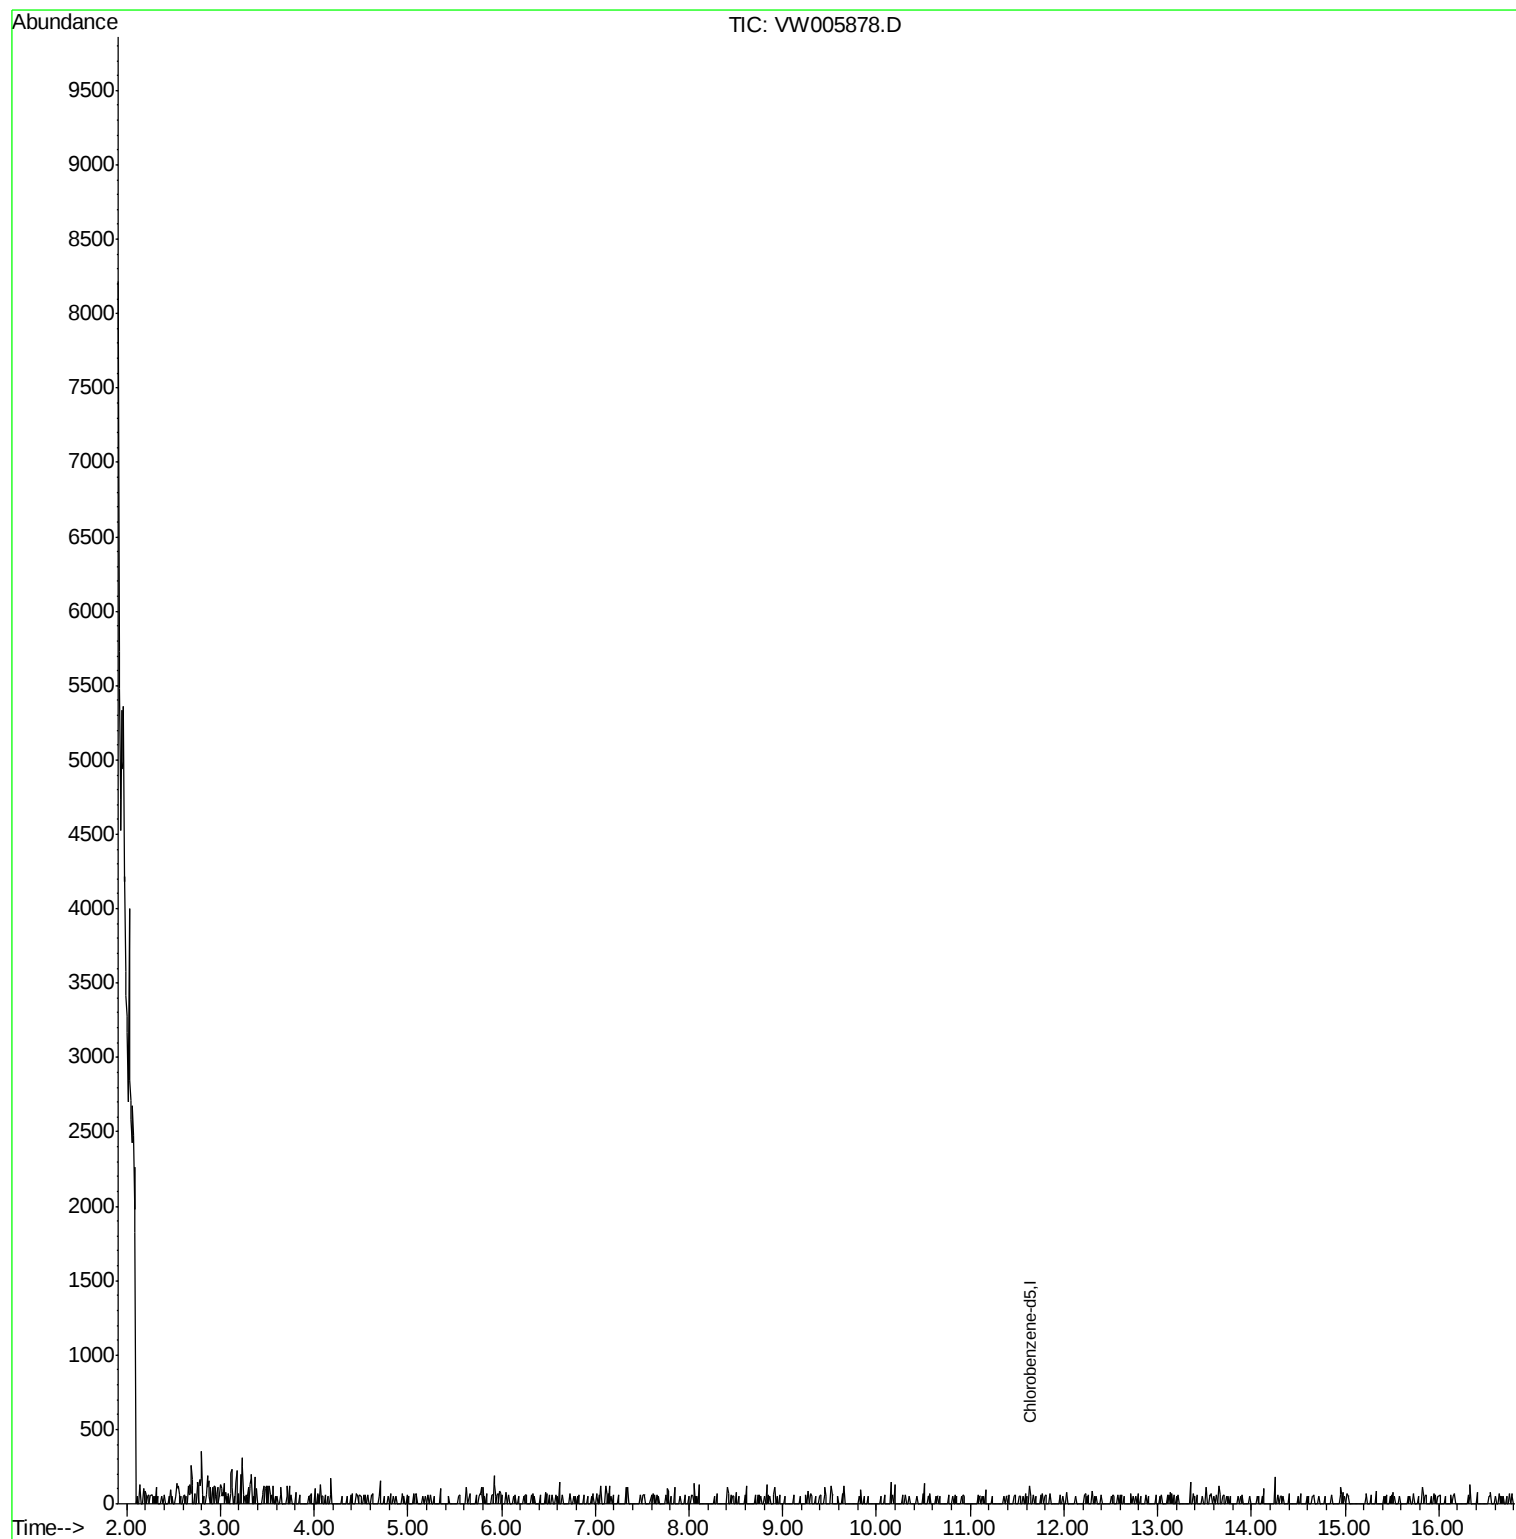

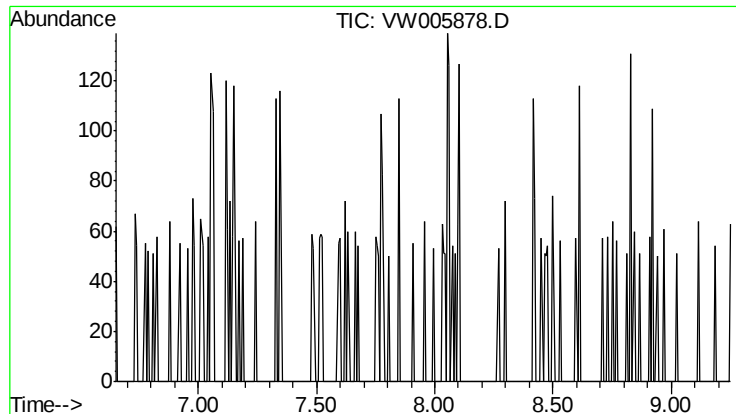

#1

Pentafluorobenzene

Concen: 0.000 ug/l

Expected RT: 7.95 min

Lab File: VW005878.D

Acq: 05 Oct 2018 04:23

Tot Ion: 168

Sig Exp Ratio

168 100



99 56.8

Instrument :

MSVOA_W

ClientSampleId :

SU-04-100318-ARE

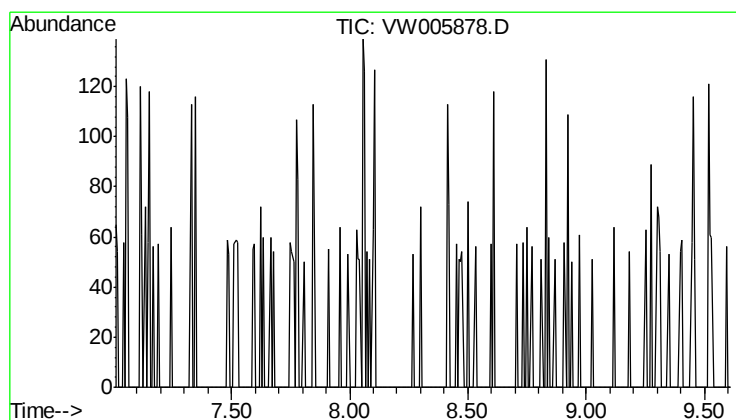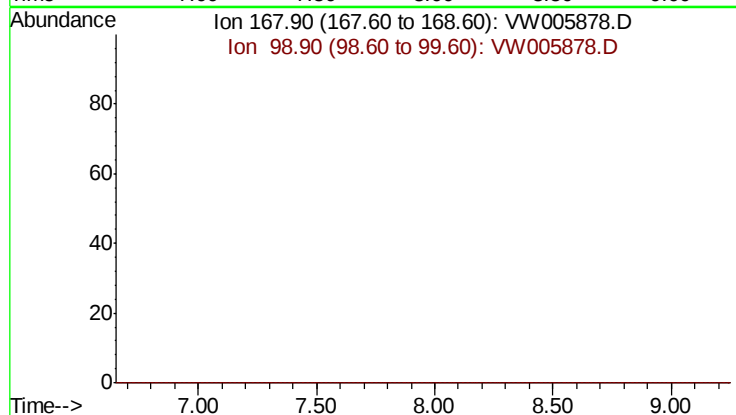

#33

1,2-Dichloroethane-d4

Concen: 0.000 ug/l

Expected RT: 8.31 min

Lab File: VW005878.D


Acq: 05 Oct 2018 04:23


Tgt Ion: 65

Sig Exp Ratio

65 100

67 49.0


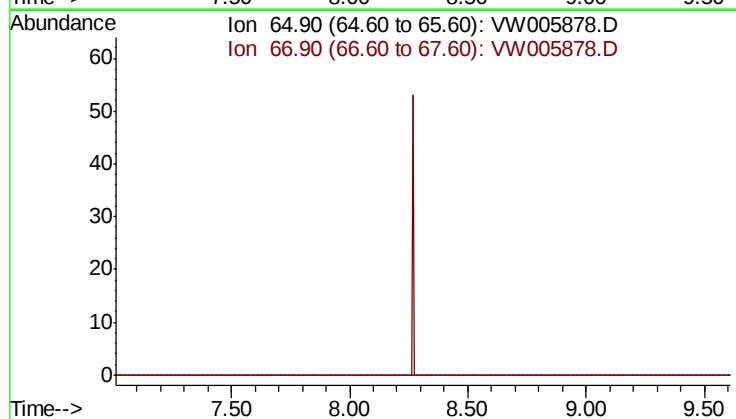


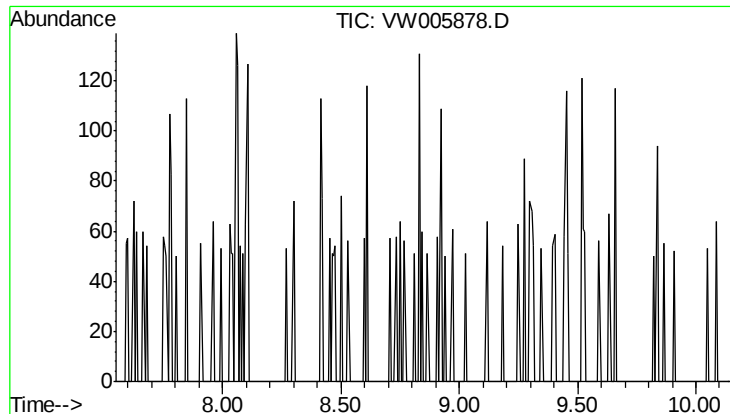

#34
 1,4-Difluorobenzene
 Concen: 0.000 ug/l
 Expected RT: 8.85 min
 Lab File: VW005878.D
 Acq: 05 Oct 2018 04:23


Instrument :
 MSVOA_W
 ClientSampleId :
 SU-04-100318-ARE


Tot Ion	114
Sig	Exp Ratio
114	100
63	21.0
88	15.6

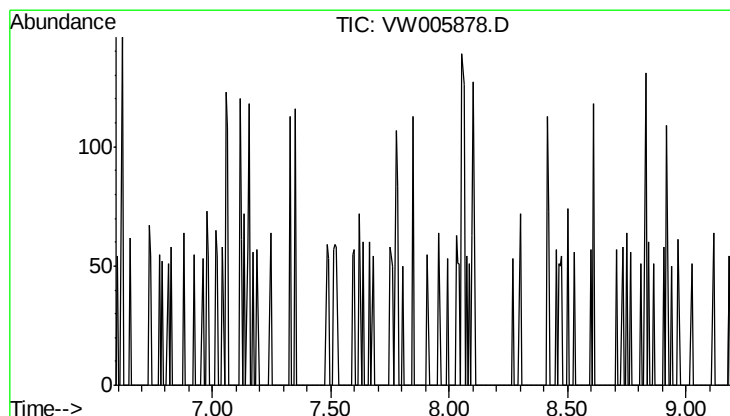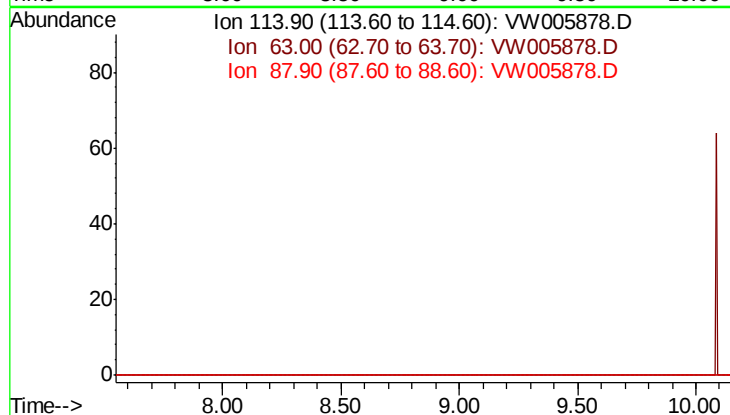

#35
 Dibromofluoromethane
 Concen: 0.000 ug/l
 Expected RT: 7.89 min
 Lab File: VW005878.D
 Acq: 05 Oct 2018 04:23

Tgt Ion	113
Sig	Exp Ratio
113	100
111	101.8
192	21.6


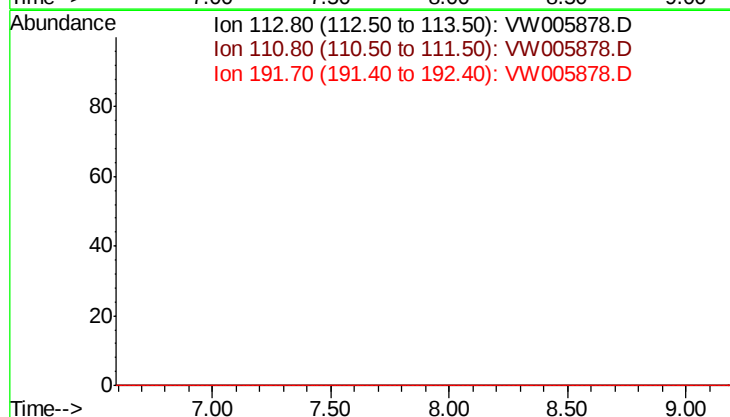


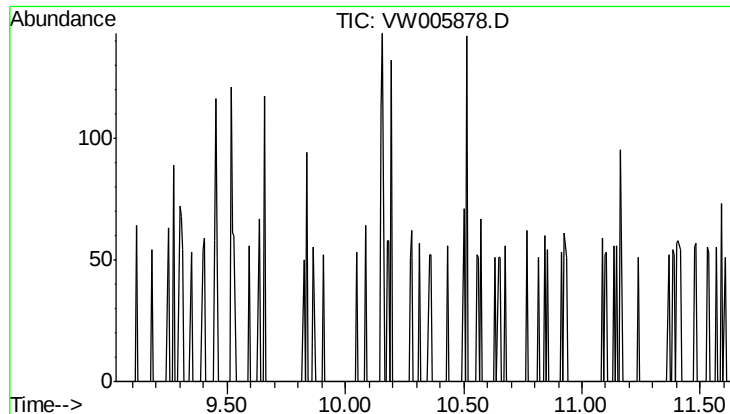

#50
Toluene-d8
Concen: 0.000 ug/l
Expected RT: 10.33 min
Lab File: VW005878.D
Acq: 05 Oct 2018 04:23


Instrument :
MSVOA_W
ClientSampleId :
SU-04-100318-ARE


Tot Ion	98
Sig	Exp Ratio
98	100
100	64.6

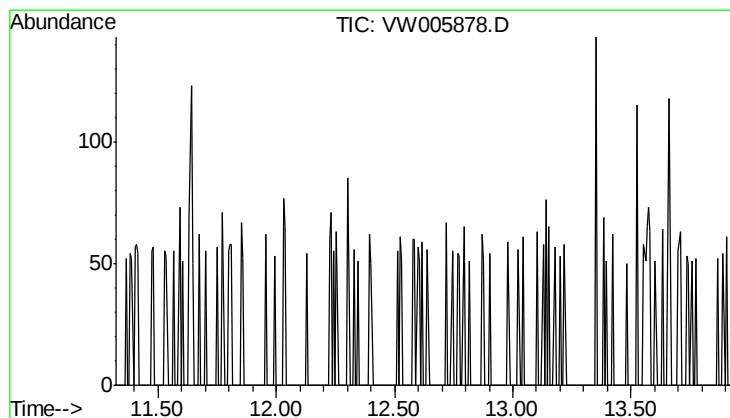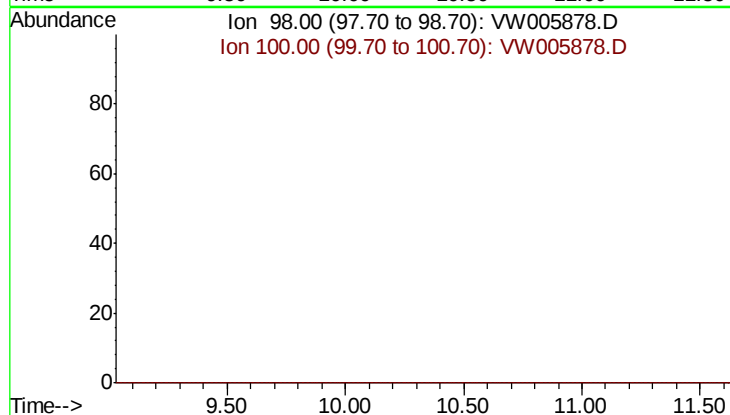

#62
4-Bromofluorobenzene
Concen: 0.000 ug/l
Expected RT: 12.62 min
Lab File: VW005878.D
Acq: 05 Oct 2018 04:23

Tgt Ion	95
Sig	Exp Ratio
95	100
174	84.5
176	82.1




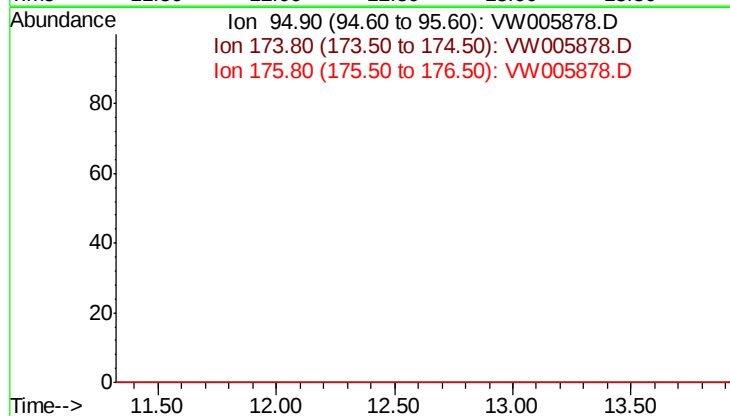


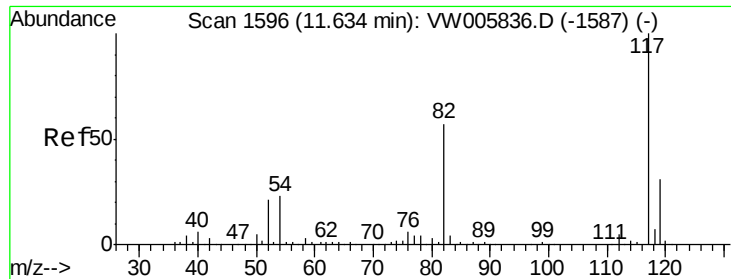

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.64 min Scan# 1597
Delta R.T. 0.01 min
Lab File: VW005878.D
Acq: 05 Oct 2018 04:23

Instrument :
MSVOA_W
ClientSampleId :
SU-04-100318-ARE

Tot Ion	Ratio	Lower	Upper
117	100		
82	0.0	45.6	68.4#
119	0.0	25.0	37.6#

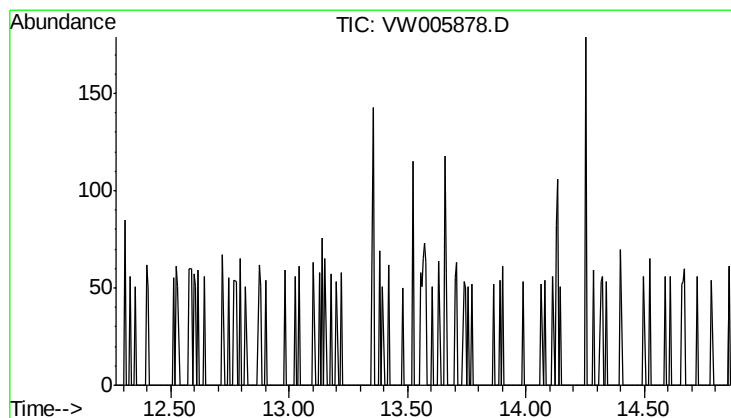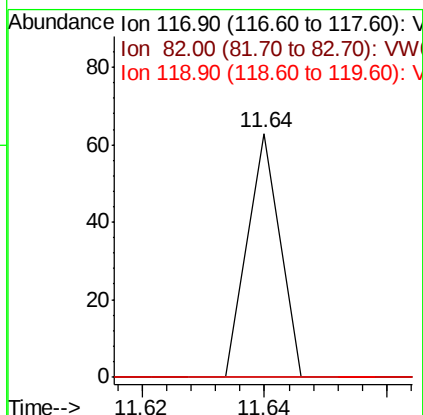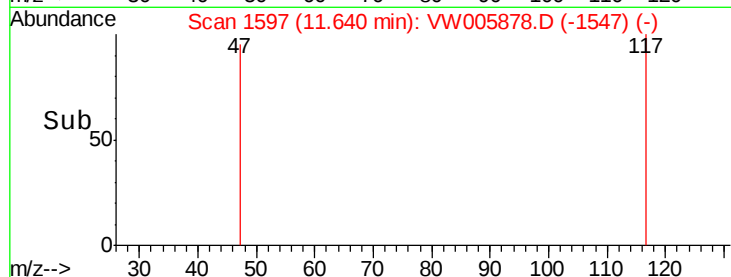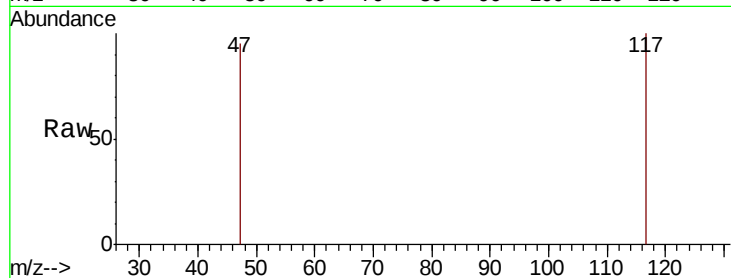

#72
1,4-Dichlorobenzene-d4
Concen: 0.000 ug/l
Expected RT: 13.57 min

Lab File: VW005878.D
Acq: 05 Oct 2018 04:23

Tgt Ion	Exp Ratio
152	100
115	59.6
150	174.7

