


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW100618\
Data File : VW005866.D
Acq On : 04 Oct 2018 21:29
Operator : SY/AP
Sample : BFB
Misc : 5.00G/5ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W100418S.M
Title : SW846 8260
Last Update : Thu Oct 04 07:08:57 2018

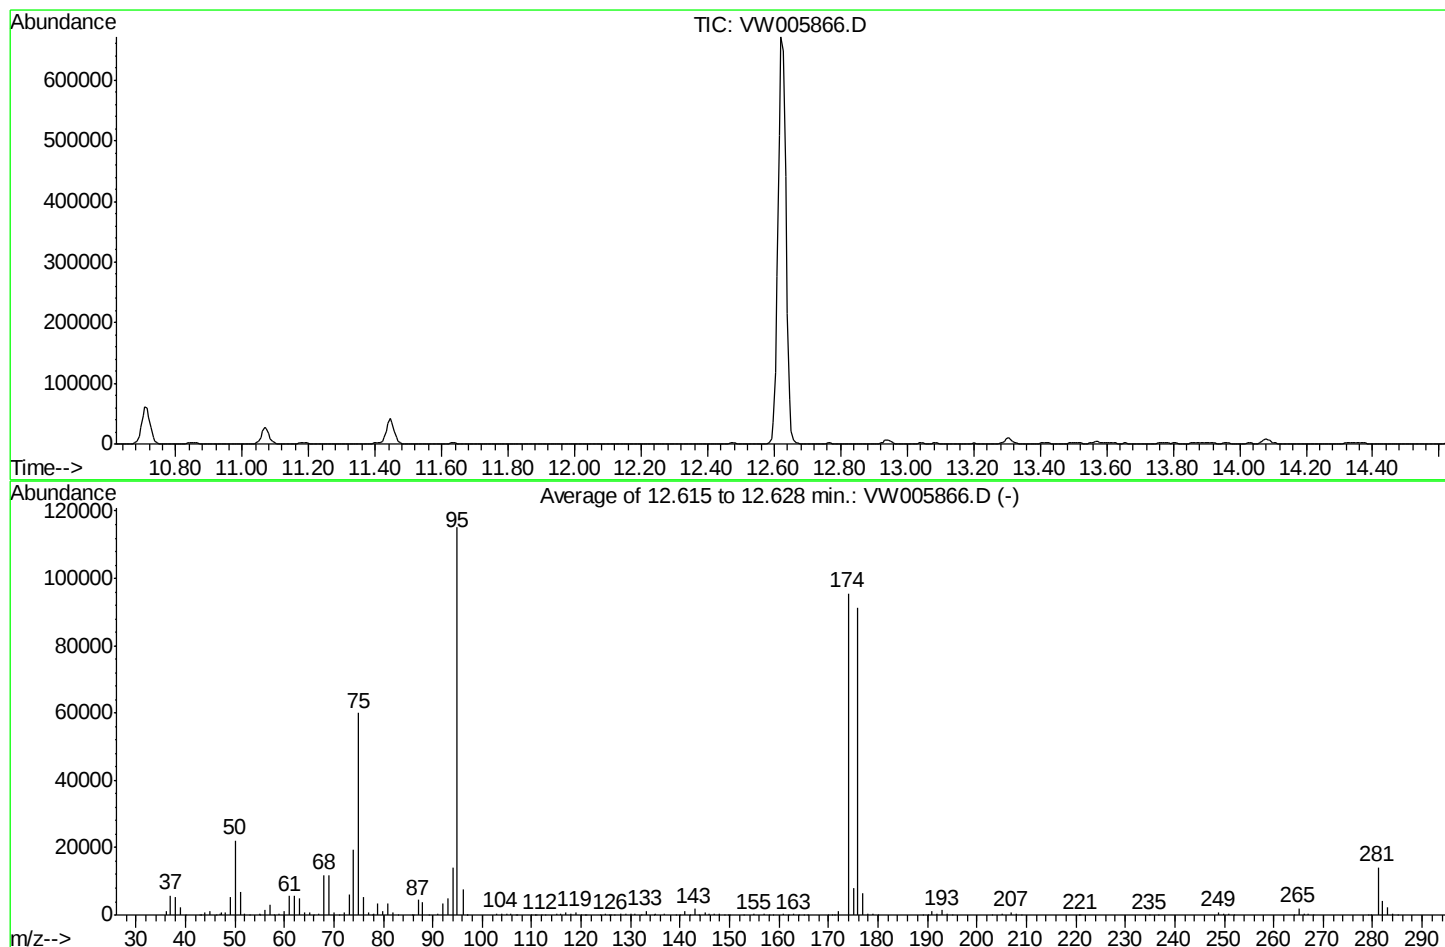

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.2	22130	PASS
75	95	30	60	52.2	60077	PASS
95	95	100	100	100.0	115178	PASS
96	95	5	9	6.7	7772	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	82.9	95461	PASS
175	174	5	9	8.4	8021	PASS
176	174	95	101	95.7	91373	PASS
177	176	5	9	7.1	6506	PASS