

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100621\
 Data File : VW020326.D
 Acq On : 06 Oct 2021 20:35
 Operator : SY/VA
 Sample : M4001-10
 Misc : 6.75g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW923

Manual Integrations
 APPROVED

MMDadoda
 10/11/2021 2:06:36 PM

Quant Time: Oct 07 01:55:22 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100621SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Oct 07 01:49:38 2021
 Response via : Initial Calibration

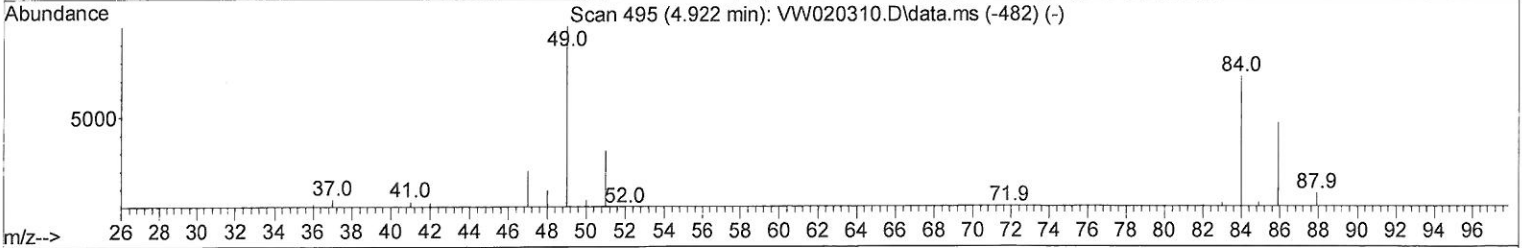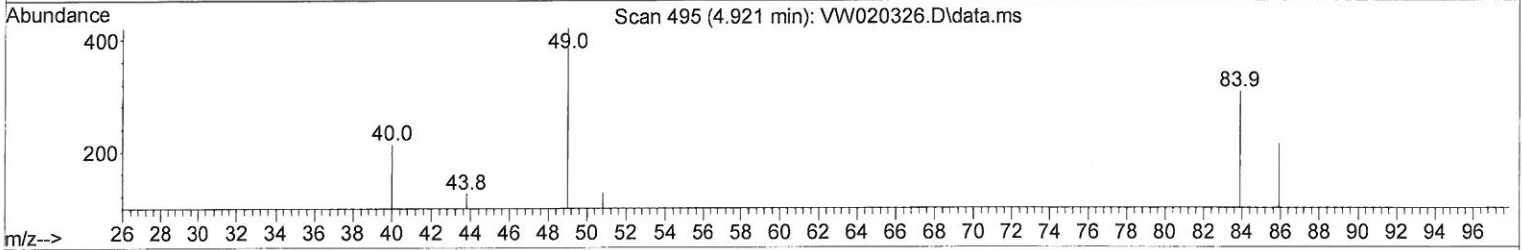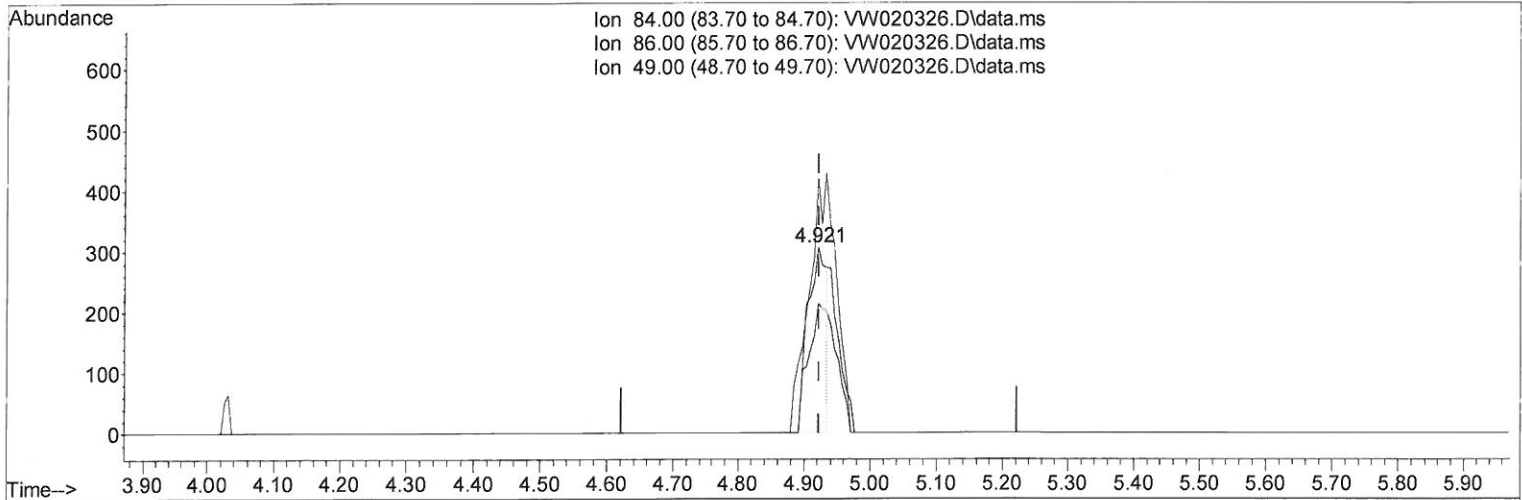

TIC: VW020326.D\data.ms

(16) Methylene chloride (T)

4.921min (-0.000) 3.86 ug/L

response 603

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	63.90	69.61
49.00	145.30	137.25
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100621\
 Data File : VW020326.D
 Acq On : 06 Oct 2021 20:35
 Operator : SY/VA
 Sample : M4001-10
 Misc : 6.75g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW923

Manual Integrations
 APPROVED

MMDadoda
 10/11/2021 2:06:36 PM

Quant Time: Oct 07 01:55:22 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100621SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Oct 07 01:49:38 2021
 Response via : Initial Calibration

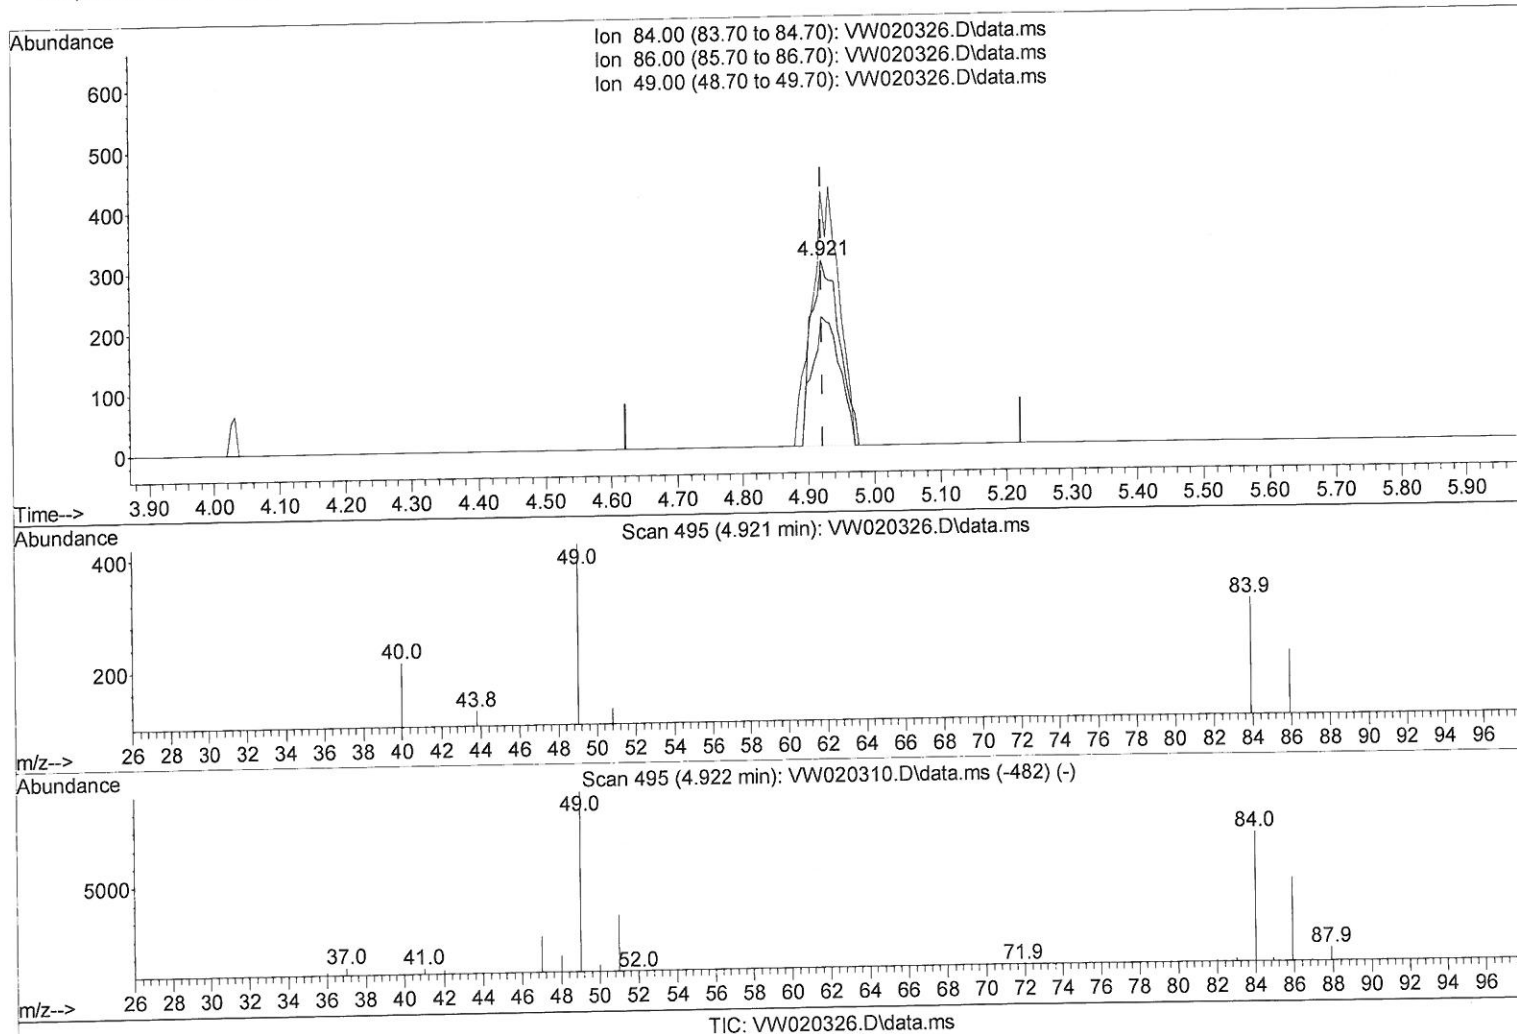

(16) Methylene chloride (T)

4.921min (-0.000) 5.85 ug/L m

response 913

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	63.90	69.61
49.00	145.30	137.25
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100621\
 Data File : VW020326.D
 Acq On : 06 Oct 2021 20:35
 Operator : SY/VA
 Sample : M4001-10
 Misc : 6.75g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW923

Manual Integrations
 APPROVED

MMDadoda
 10/11/2021 2:06:36 PM

Quant Time: Oct 07 01:55:22 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100621SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Oct 07 01:49:38 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	8.848	114	8742	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	5941	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	1598	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	3257	27.033	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	= 108.120%		
7) Chloroethane-d5	2.891	69	3979	76.217	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	= 304.880%#		
11) 1,1-Dichloroethene-d2	4.031	63	5043	20.325	ug/L	0.01
Spiked Amount	25.000	Range 45 - 110	Recovery	= 81.320%		
21) 2-Butanone-d5	7.092	46	1503	49.107	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	= 98.220%		
24) Chloroform-d	7.659	84	10230	40.755	ug/L	0.00
Spiked Amount	25.000	Range 40 - 150	Recovery	= 163.000%#		
26) 1,2-Dichloroethane-d4	8.311	65	7186	52.310	ug/L	0.00
Spiked Amount	25.000	Range 70 - 130	Recovery	= 209.240%#		
32) Benzene-d6	8.281	84	15789	43.894	ug/L	0.00
Spiked Amount	25.000	Range 20 - 135	Recovery	= 175.560%#		
36) 1,2-Dichloropropane-d6	9.280	67	6495	56.926	ug/L	0.00
Spiked Amount	25.000	Range 70 - 120	Recovery	= 227.720%#		
41) Toluene-d8	10.329	98	9354	28.711	ug/L	0.00
Spiked Amount	25.000	Range 30 - 130	Recovery	= 114.840%		
43) trans-1,3-Dichloroprop...	10.579	79	1599	34.444	ug/L	0.00
Spiked Amount	25.000	Range 30 - 135	Recovery	= 137.760%#		
47) 2-Hexanone-d5	10.927	63	729	46.229	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	= 92.460%		
56) 1,1,2,2-Tetrachloroeth...	12.694	84	5078	63.769	ug/L	0.00
Spiked Amount	25.000	Range 45 - 120	Recovery	= 255.080%#		
66) 1,2-Dichlorobenzene-d4	13.859	152	1873	33.472	ug/L	0.00
Spiked Amount	25.000	Range 75 - 120	Recovery	= 133.880%#		
Target Compounds						
16) Methylene chloride	4.921	84	913m	5.849	ug/L	Qvalue 10
30) 1,1,1-Trichloroethane	7.878	97	638	4.477	ug/L #	41
34) Trichloroethene	9.098	95	2397	23.584	ug/L	87
42) Toluene	10.396	91	479	1.153	ug/L #	75

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100621\
Data File : VW020326.D
Acq On : 06 Oct 2021 20:35
Operator : SY/VA
Sample : M4001-10
Misc : 6.75g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW923

Manual Integrations
APPROVED

MMDadoda
10/11/2021 2:06:36 PM

Quant Time: Oct 07 01:55:22 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100621SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Oct 07 01:49:38 2021
Response via : Initial Calibration

