

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100621\
 Data File : VW020369.D
 Acq On : 07 Oct 2021 17:10
 Operator : SY/VA
 Sample : M4000-05
 Misc : 7.45g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW900

Quant Time: Oct 08 05:58:43 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100621SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Oct 08 05:56:34 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	316904	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	260224	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	86000	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	96160	22.017	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	88.080%		
7) Chloroethane-d5	2.891	69	59375	31.374	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	125.480%		
11) 1,1-Dichloroethene-d2	4.013	63	142463	15.839	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	63.360%		
21) 2-Butanone-d5	7.086	46	44567	40.168	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	80.340%		
24) Chloroform-d	7.647	84	183523	20.169	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	80.680%		
26) 1,2-Dichloroethane-d4	8.305	65	100351	20.151	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	80.600%		
32) Benzene-d6	8.274	84	363506	23.071	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	92.280%		
36) 1,2-Dichloropropane-d6	9.274	67	116331	23.278	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	93.120%		
41) Toluene-d8	10.323	98	309197	21.667	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	86.680%		
43) trans-1,3-Dichloroprop...	10.579	79	41064	20.195	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	80.760%		
47) 2-Hexanone-d5	10.926	63	30531	44.202	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	88.400%		
56) 1,1,2,2-Tetrachloroeth...	12.694	84	73101	20.958	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	83.840%		
66) 1,2-Dichlorobenzene-d4	13.853	152	68201	22.647	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	90.600%		
Target Compounds					Qvalue	
13) Acetone	4.135	43	5702	4.999	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100621\
Data File : VW020369.D
Acq On : 07 Oct 2021 17:10
Operator : SY/VA
Sample : M4000-05
Misc : 7.45g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW900

Quant Time: Oct 08 05:58:43 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100621SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Oct 08 05:56:34 2021
Response via : Initial Calibration

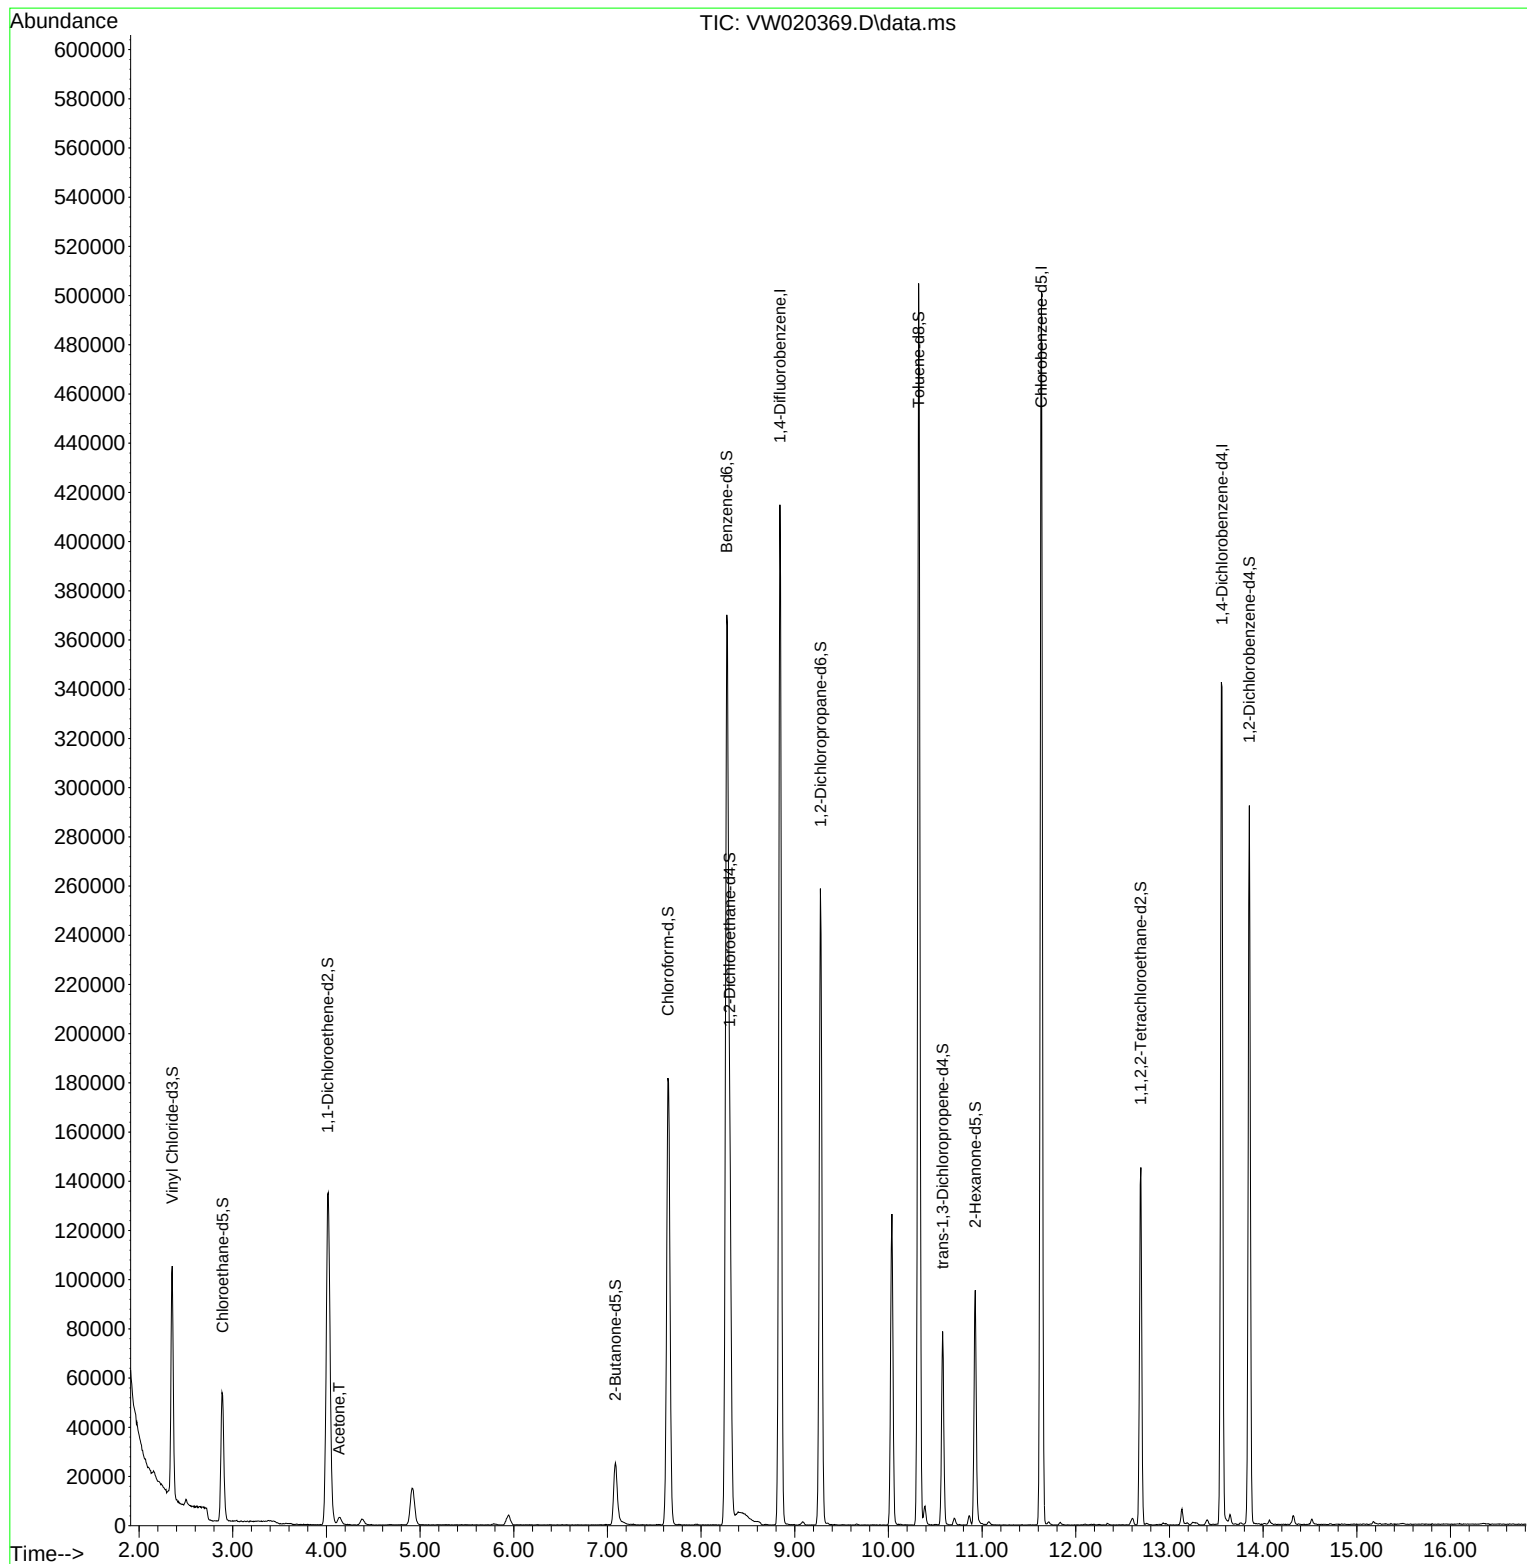

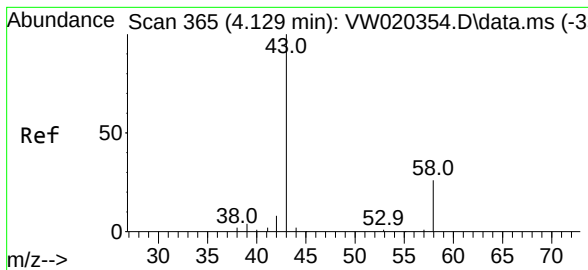

#13

Acetone

Concen: 4.999 ug/L

RT: 4.135 min Scan# 366

Delta R.T. 0.006 min

Lab File: VW020369.D

Acq: 07 Oct 2021 17:10

Tgt Ion: 43 Resp: 5702

Ion Ratio Lower Upper

43 100

58 28.5 0.0 58.4

Instrument :

MSVOA_W

ClientSampleId :

EW900

