
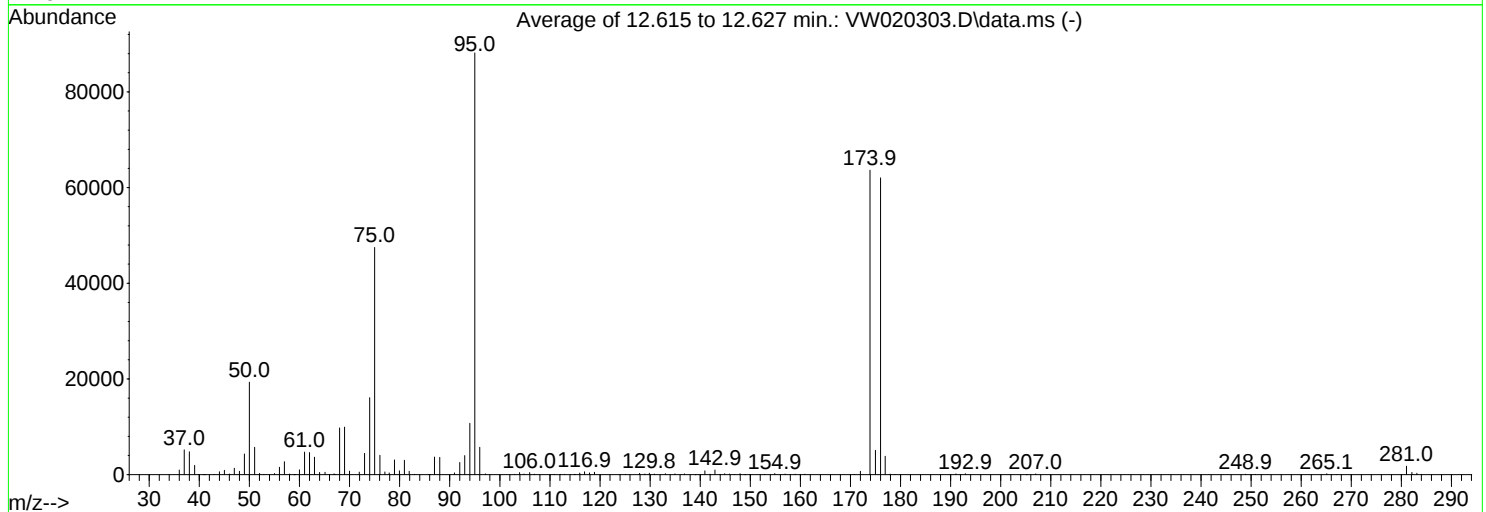


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100621\
Data File : VW020303.D
Acq On : 06 Oct 2021 08:31
Operator : SY/VA
Sample : BFB446
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB446

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100621SMA.M
Title : SFAM01.0
Last Update : Fri Oct 08 07:38:51 2021

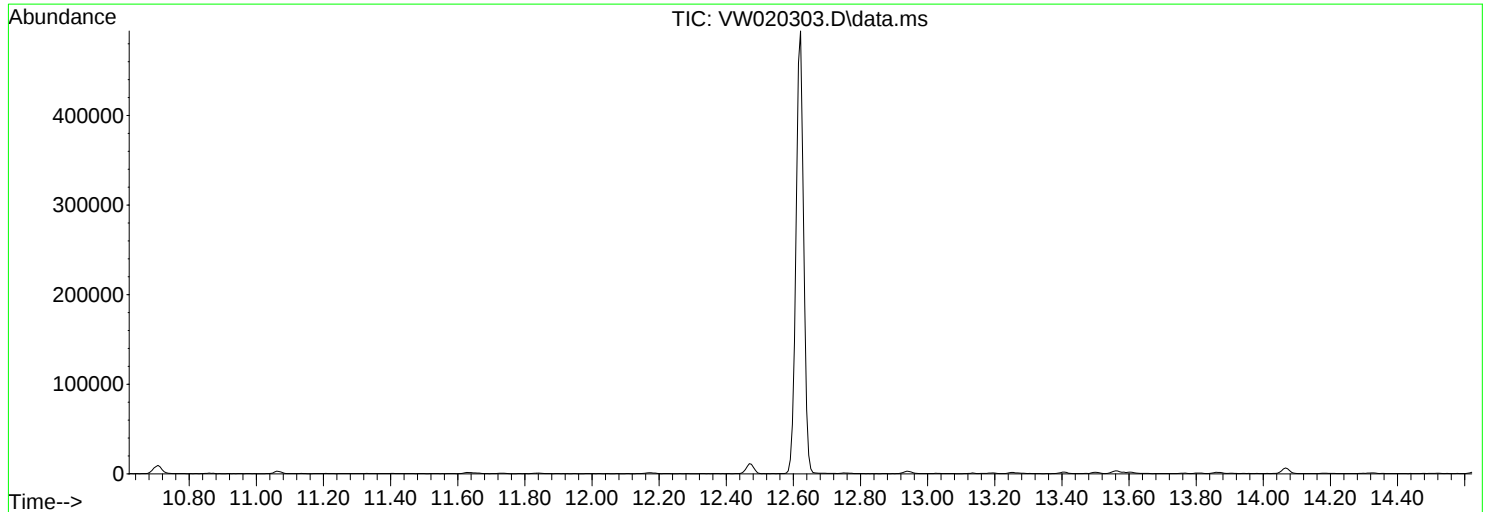

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.9	19334	PASS
75	95	30	80	53.9	47504	PASS
95	95	100	100	100.0	88163	PASS
96	95	5	9	6.5	5706	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	72.2	63648	PASS
175	174	5	9	8.0	5102	PASS
176	174	95	105	97.5	62037	PASS
177	176	5	10	6.2	3852	PASS

Scan 1749 (12.566 min): VW020303.D\data.ms
BFB446

m/z	Abundance
39.90	156.0
44.00	134.0

Instrument :
MSVOA_W
ClientSampleId :
BFB446

m/z	Abundance
36.00	1021.0
37.00	5889.0
38.00	5555.0
39.10	2123.0
40.00	235.0
40.80	68.0
43.00	67.0
44.10	821.0
45.00	1100.0
46.10	189.0
47.00	1476.0
48.00	820.0
49.00	4608.0
50.00	21576.0
51.00	6473.0
52.00	309.0
52.90	93.0
55.00	297.0
56.00	1709.0
57.00	2895.0
58.10	132.0
59.20	90.0
60.00	1074.0
61.00	5413.0
62.00	5192.0
63.00	4046.0
64.00	584.0
65.10	665.0
65.90	107.0
66.90	289.0
68.00	10735.0
69.00	10839.0
70.00	821.0
72.00	628.0
73.00	4936.0
74.00	18168.0
75.00	52208.0
76.10	4387.0
77.00	551.0
77.90	391.0
78.90	3322.0
80.00	921.0
81.00	3118.0
81.90	819.0
83.00	70.0
86.10	136.0
87.00	3814.0
88.00	4013.0
91.00	413.0
92.00	2674.0
93.00	4307.0
94.00	11701.0
95.00	94424.0
96.00	6355.0
97.10	191.0
103.00	104.0
104.00	459.0
104.90	139.0
105.90	456.0
106.90	88.0
110.10	50.0
110.80	125.0
112.00	90.0
113.00	92.0
114.90	136.0
115.90	332.0
116.90	687.0
117.90	347.0
118.90	582.0
125.10	113.0
127.80	269.0
129.10	89.0
129.90	268.0
130.90	97.0
133.00	342.0
134.90	176.0
136.90	207.0
139.00	57.0
139.70	53.0
141.00	803.0
142.00	115.0
142.90	950.0
143.90	96.0
144.90	226.0
145.90	125.0
146.90	115.0
147.90	225.0
148.90	58.0
149.90	114.0
152.90	59.0
154.80	259.0
157.00	129.0

Instrument :
MSVOA_W
ClientSampleId :
BFB446

158.90	78.0
161.00	91.0
170.90	127.0
172.00	791.0
173.90	60104.0
175.00	5135.0
176.00	59376.0
176.90	3800.0
178.00	120.0
178.90	59.0
191.00	270.0
191.90	62.0
192.90	287.0
205.10	55.0
207.10	186.0
248.90	133.0
250.10	59.0
250.90	86.0
265.10	289.0
266.00	83.0
267.00	65.0
281.00	2608.0
282.10	709.0
283.10	446.0
284.00	138.0

Instrument :
MSVOA_W
ClientSampleId :
BFB446

m/z	Abundance
36.00	1125.0
37.00	5812.0
38.00	5410.0
39.00	2227.0
40.00	189.0
41.00	51.0
42.90	79.0
43.90	783.0
45.00	930.0
46.00	105.0
47.00	1501.0
48.00	799.0
49.00	5007.0
50.00	21736.0
51.10	6114.0
52.10	333.0
52.90	76.0
55.00	261.0
56.00	1761.0
57.00	3098.0
58.00	123.0
58.90	53.0
60.00	1259.0
61.00	5325.0
62.00	5004.0
63.00	4206.0
64.00	488.0
65.10	577.0
66.00	63.0
67.10	255.0
68.00	10683.0
69.00	11142.0
70.00	884.0
71.90	551.0
73.00	4978.0
74.00	17376.0
75.00	52648.0
76.00	4481.0
77.10	678.0
77.90	456.0
78.90	3522.0
79.90	898.0
80.90	3492.0
81.90	800.0
82.90	81.0
85.80	146.0
86.90	4300.0
88.00	4109.0
91.00	387.0
92.00	2832.0
93.00	4567.0
94.00	11913.0
95.00	100152.0
96.00	6191.0
97.10	197.0
103.00	89.0
103.90	578.0
104.90	151.0
105.90	409.0
106.90	109.0
110.90	101.0
112.10	85.0
112.90	104.0
115.10	118.0
116.00	327.0
116.90	707.0
117.90	465.0
118.90	521.0
123.80	76.0
125.10	72.0
127.90	309.0
128.90	171.0
129.80	341.0
130.90	167.0
133.10	180.0
135.00	203.0
136.90	167.0
139.80	85.0
140.90	973.0
142.00	130.0
143.00	1189.0
144.00	76.0
144.90	212.0
145.90	151.0
146.90	95.0
148.00	223.0
149.90	76.0
152.90	69.0
154.90	254.0
157.00	144.0
159.00	156.0
160.90	127.0

Instrument :
MSVOA_W
ClientSampleId :
BFB446

m/z	Abundance
36.00	794.0
37.10	3895.0
38.00	3432.0
39.00	1431.0
39.90	196.0
43.00	58.0
44.00	588.0
45.00	731.0
46.00	107.0
47.00	1034.0
47.90	475.0
49.00	3370.0
50.00	14690.0
51.00	4553.0
52.00	205.0
52.90	60.0
55.10	185.0
56.00	1111.0
57.00	2125.0
58.00	122.0
60.00	667.0
61.10	3455.0
62.00	3683.0
63.00	2723.0
64.00	372.0
65.10	299.0
66.90	197.0
68.00	7865.0
69.00	7815.0
70.00	512.0
71.90	397.0
73.00	3479.0
74.00	12684.0
75.00	37656.0
76.00	3242.0
77.00	461.0
77.90	275.0
79.00	2390.0
80.00	623.0
80.90	2443.0
81.90	534.0
83.00	73.0
87.00	2892.0
88.00	2760.0
90.80	281.0
92.00	2081.0
93.00	3048.0
94.00	8566.0
95.00	69912.0
96.00	4572.0
97.10	144.0
103.90	318.0
104.80	135.0
106.00	405.0
106.90	76.0
110.10	62.0
112.00	80.0
114.90	63.0
116.00	313.0
116.90	461.0
117.90	339.0
118.90	417.0
125.00	60.0
128.00	224.0
128.90	126.0
129.90	262.0
130.80	112.0
133.00	69.0
135.00	151.0
136.80	139.0
140.90	685.0
141.90	82.0
143.00	741.0
144.90	134.0
145.90	109.0
147.90	195.0
152.90	93.0
155.00	173.0
156.80	116.0
158.90	89.0
160.80	89.0
170.80	81.0
172.00	538.0
173.90	55520.0
175.00	4346.0
176.00	54768.0
177.00	2849.0
177.90	95.0
191.00	80.0
192.90	66.0
207.10	101.0
265.10	120.0

Instrument :
MSVOA_W
ClientSampleId :
BFB446

281.10

282.00

283.00

838.0

239.0

141.0

Instrument :

MSVOA_W

ClientSampleId :

BFB446

172.00	755.0
173.90	75320.0
175.00	5824.0
176.00	71968.0
177.00	4906.0
177.80	115.0
191.10	129.0
193.00	233.0
206.90	169.0
248.90	139.0
250.80	76.0
265.10	217.0
266.10	58.0
281.00	1902.0
282.10	463.0
283.10	353.0
284.10	61.0

Instrument :
MSVOA_W
ClientSampleId :
BFB446