


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW100719\
Data File : VW013451.D
Acq On : 07 Oct 2019 09:29
Operator : SY/VA
Sample : BFB
Misc : 5.00G/5ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W100119S.M
Title : SW846 8260
Last Update : Wed Oct 02 11:49:57 2019

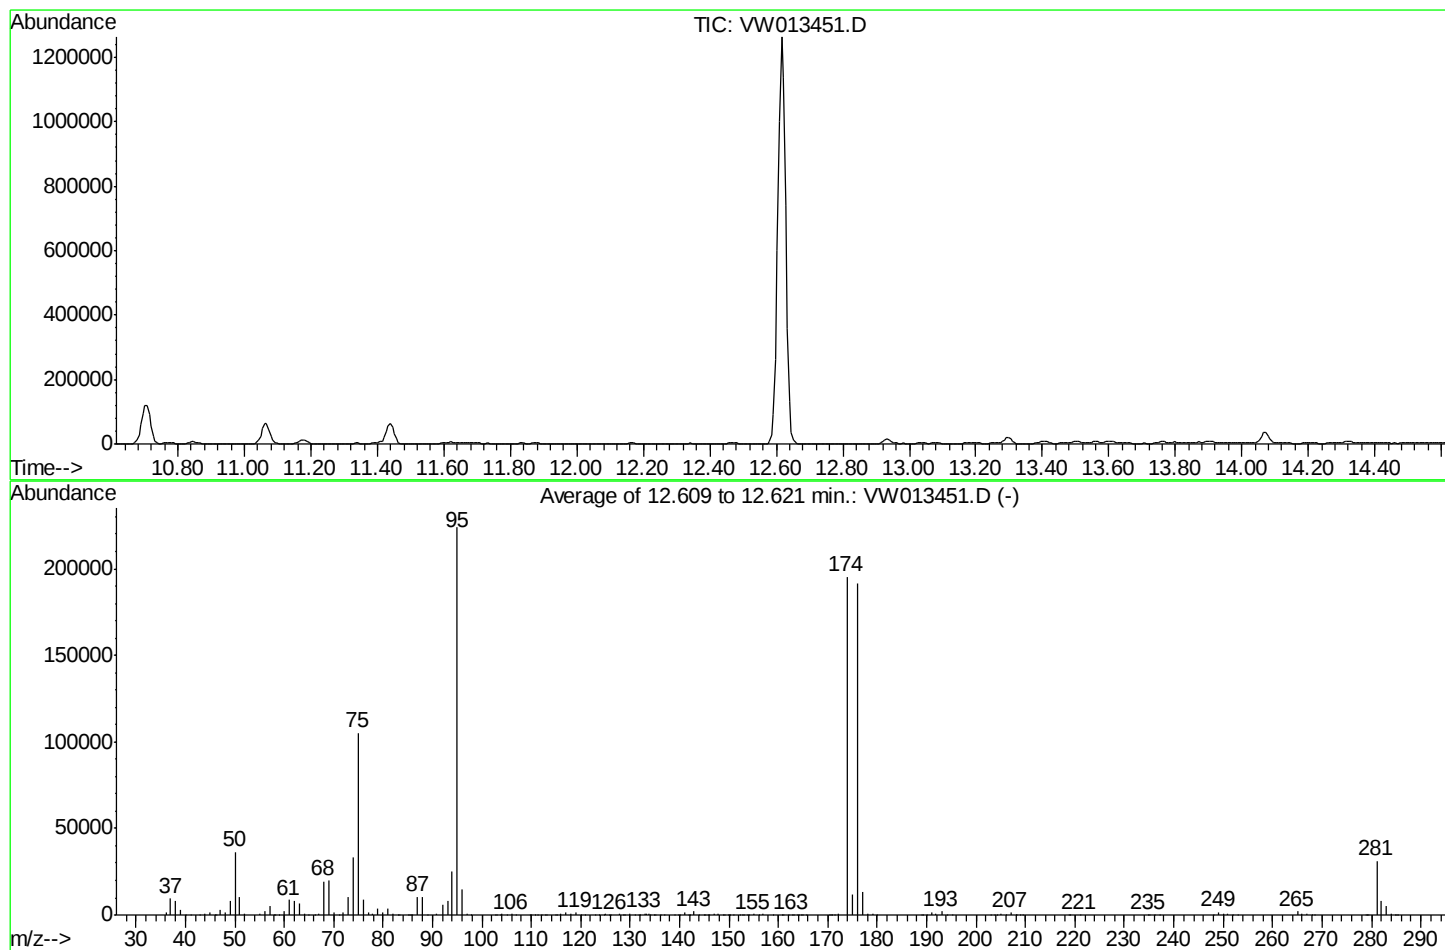

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1747

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.3	36589	PASS
75	95	30	60	46.9	104992	PASS
95	95	100	100	100.0	223914	PASS
96	95	5	9	6.5	14613	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	87.3	195370	PASS
175	174	5	9	6.0	11634	PASS
176	174	95	101	97.9	191253	PASS
177	176	5	9	6.8	13041	PASS