
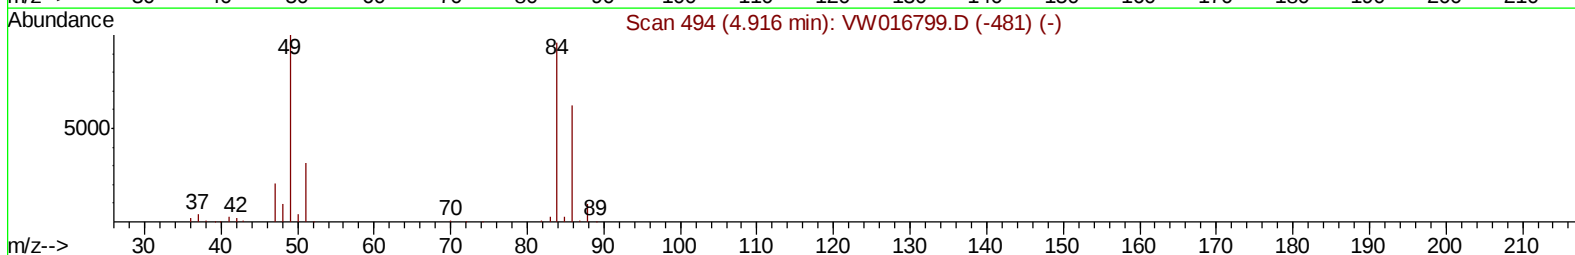
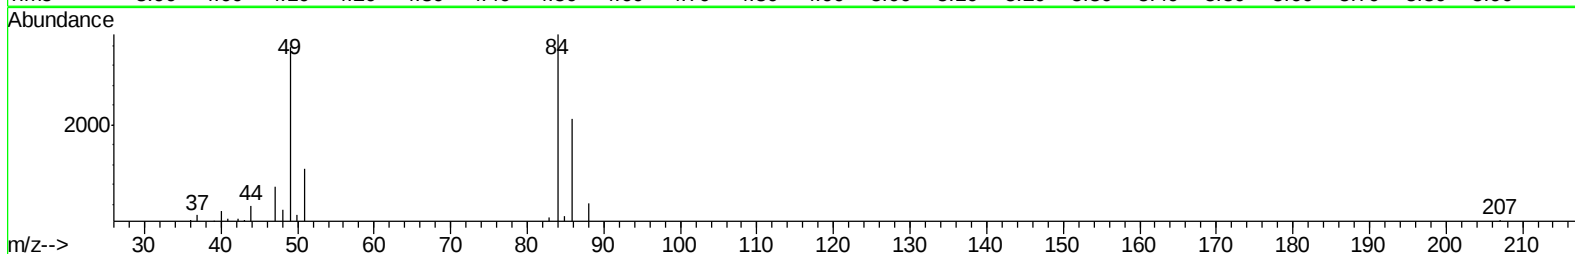


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW100720\
Data File : VW016821.D
Acq On : 07 Oct 2020 02:38
Operator : SY/VA
Sample : L4254-16
Misc : 6.24G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 07 03:16:23 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100720S.M
Quant Title : VOC Analysis
QLast Update : Wed Oct 07 03:05:19 2020
Response via : Initial Calibration

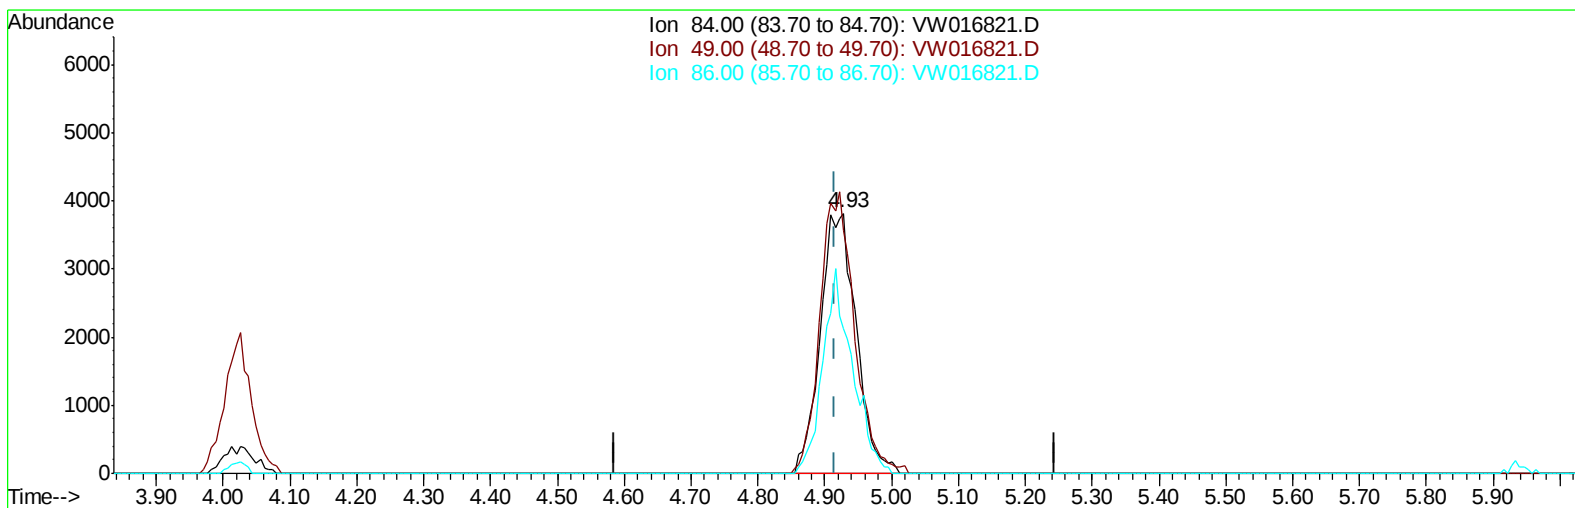

TIC: VW016821.D

(16) Methylene chloride (T)

4.928min (+0.012) 1.59ug/L m

response 14247

Ion	Exp%	Act%
84.00	100	100
49.00	104.50	93.56
86.00	65.70	55.83
0.00	0.00	0.00