

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100720\
Quantitation Report (LSC Reviewed)


Data File : VW016800.D
Acq On : 06 Oct 2020 18:11
Operator : SY/VA
Sample : VW1007SBL01
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK26

Manual Integrations
APPROVED

MMDadoda
10/8/2020 5:38:23 PM

Quant Time: Oct 07 15:27:07 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100720S.M
Quant Title : VOC Analysis
QLast Update : Wed Oct 07 03:05:19 2020
Response via : Initial Calibration

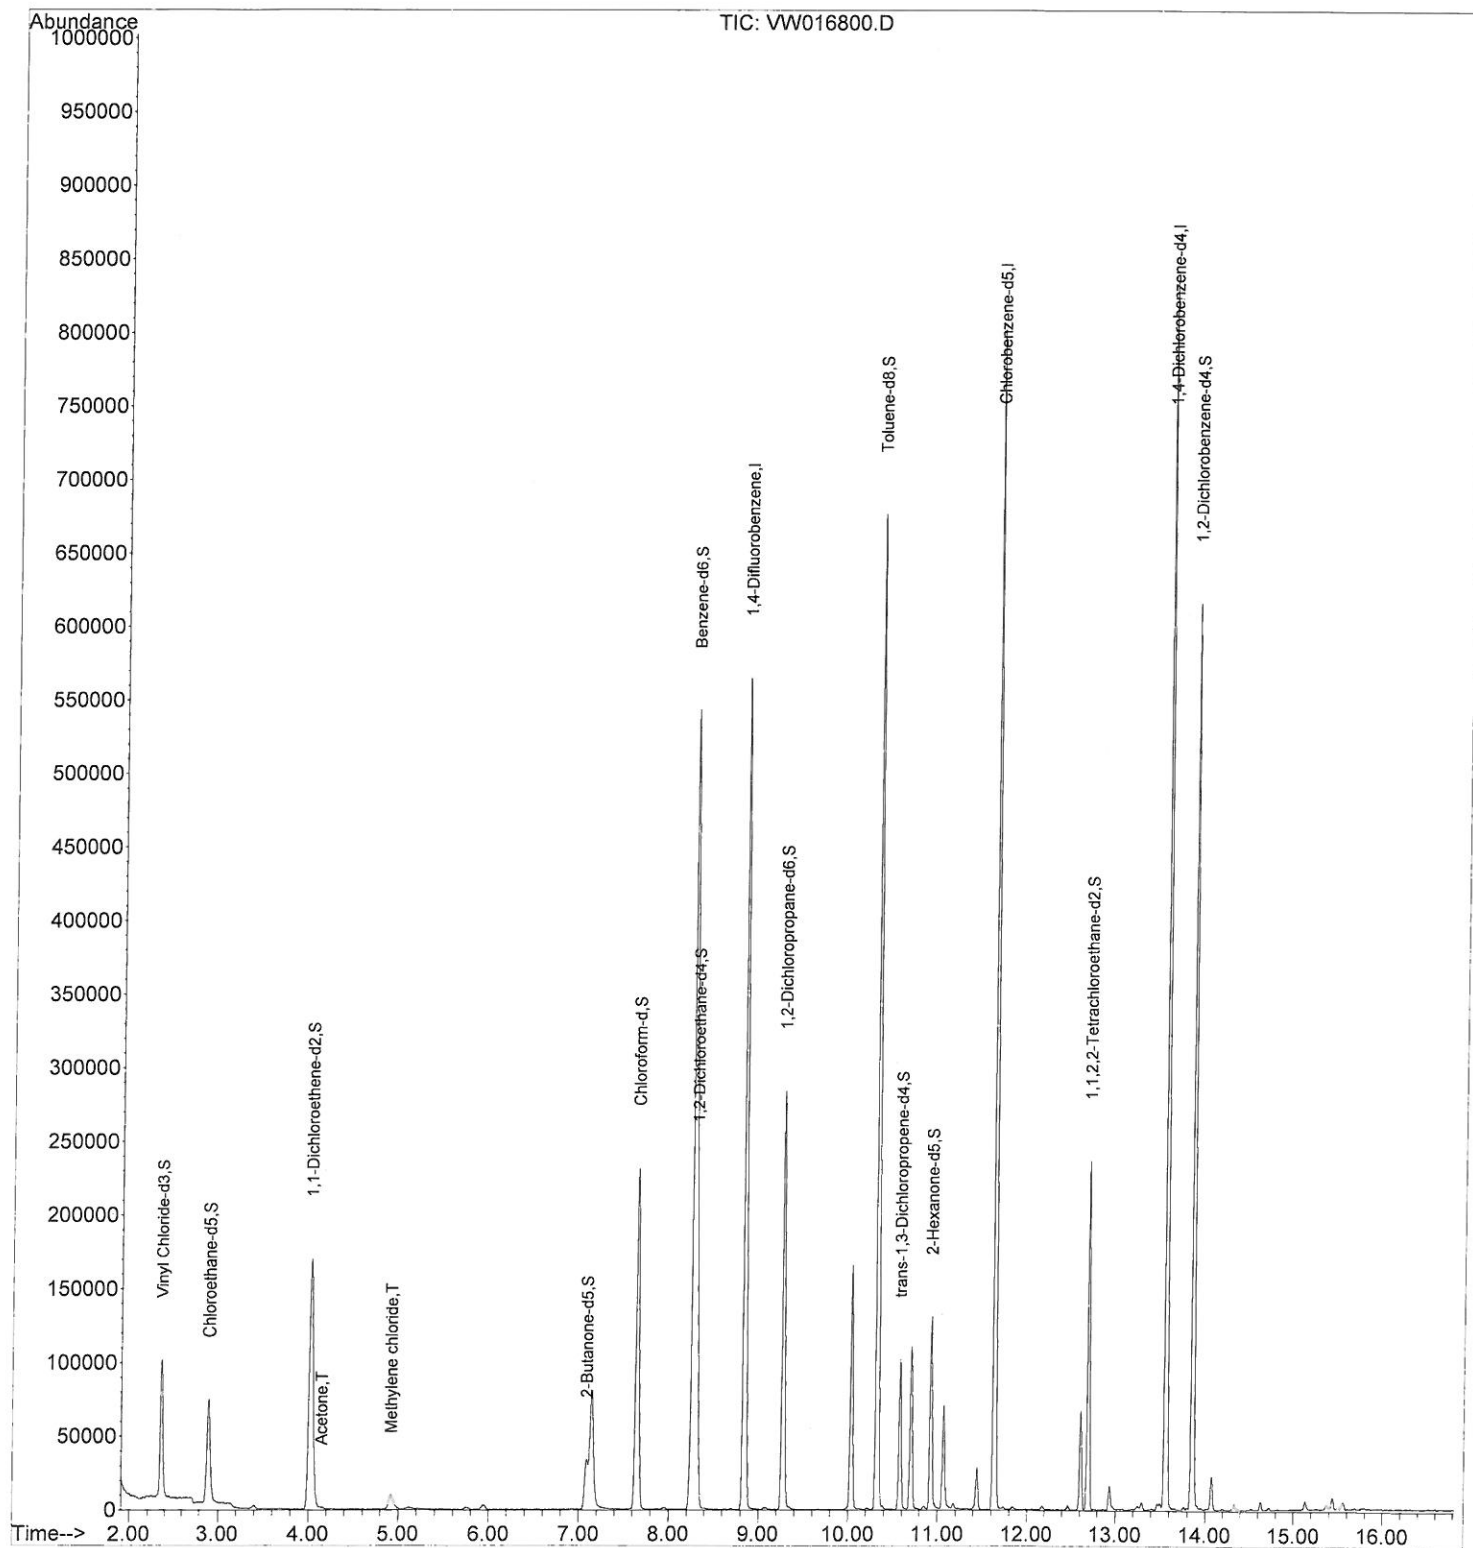

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW100720\
 Data File : VW016803.D
 Acq On : 06 Oct 2020 19:34
 Operator : SY/VA
 Sample : L4144-05
 Misc : 5.02G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK26

Manual Integrations
 APPROVED

MMDadoda
 10/8/2020 5:38:23 PM

Quant Time: Oct 07 03:14:09 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100720S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Oct 07 03:05:19 2020
 Response via : Initial Calibration

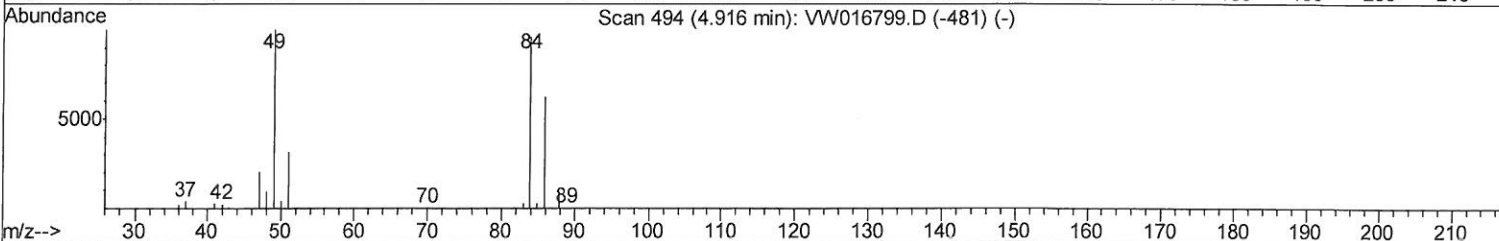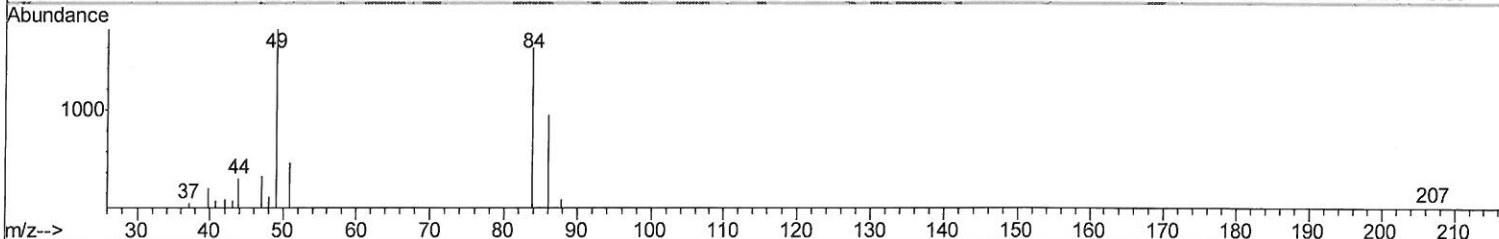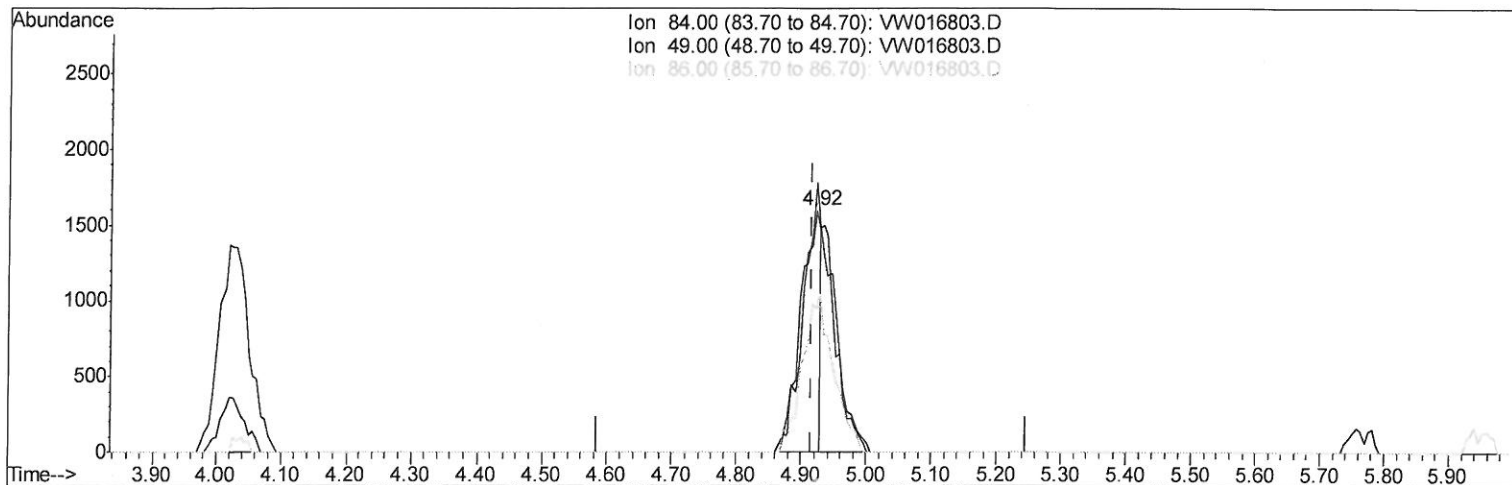

TIC: VW016803.D

(16) Methylene chloride (T)
 4.921min (+0.006) 0.44ug/L
 response 3202

Ion	Exp%	Act%
84.00	100	100
49.00	104.50	111.45
86.00	65.70	59.51
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW100720\
 Data File : VW016803.D
 Acq On : 06 Oct 2020 19:34
 Operator : SY/VA
 Sample : L4144-05
 Misc : 5.02G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK26

Manual Integrations
 APPROVED

MMDadoda
 10/8/2020 5:38:23 PM

Quant Time: Oct 07 03:14:09 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100720S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Oct 07 03:05:19 2020
 Response via : Initial Calibration

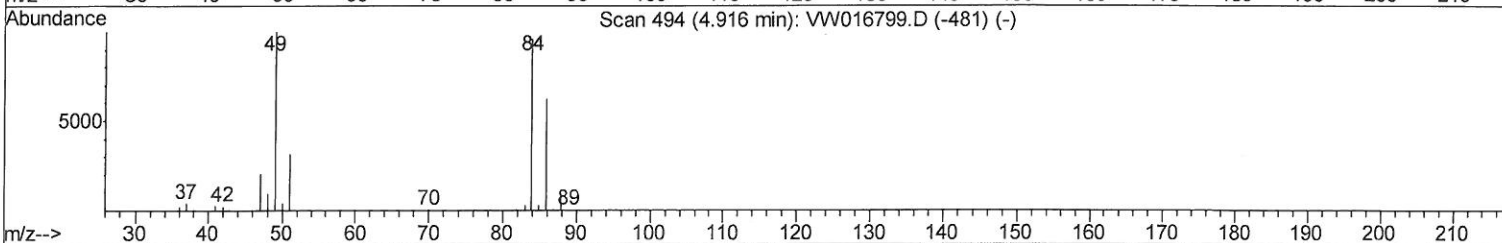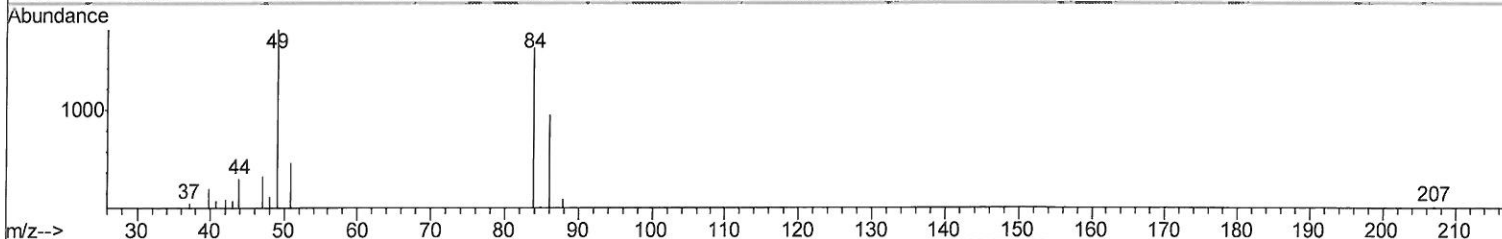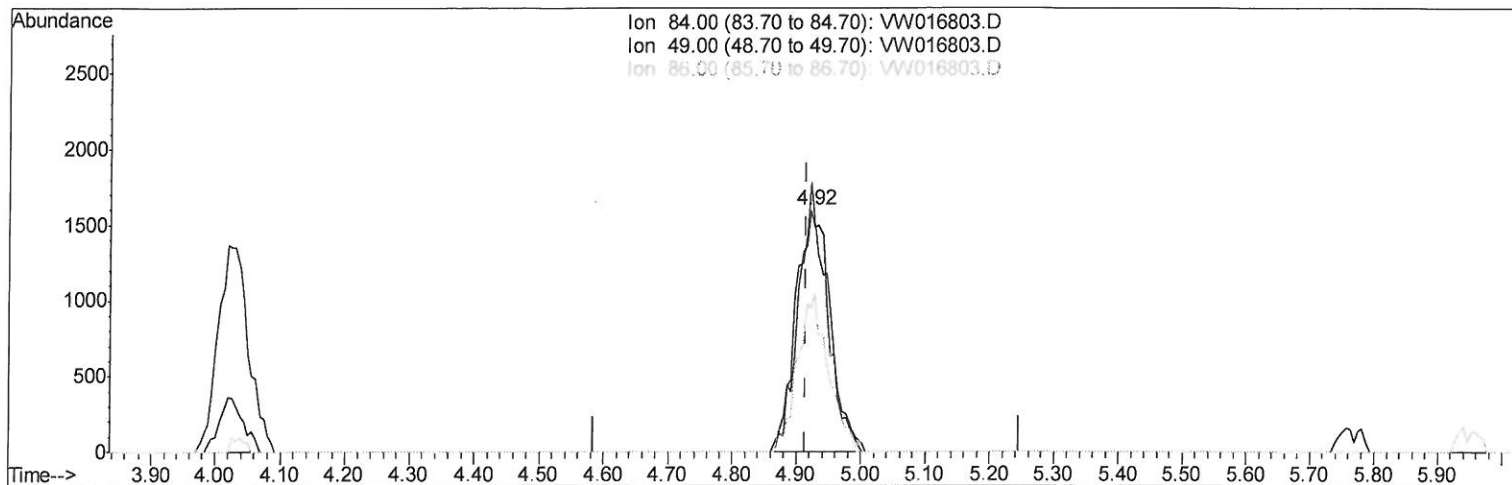

TIC: VW016803.D

(16) Methylene chloride (T)

4.921min (+0.006) 0.76ug/L m

> 10/cg/2e sy

response 5552

Ion	Exp%	Act%
84.00	100	100
49.00	104.50	111.45
86.00	65.70	59.51
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW100720\
 Data File : VW016803.D
 Acq On : 06 Oct 2020 19:34
 Operator : SY/VA
 Sample : L4144-05
 Misc : 5.02G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleID :
 VBLK26

Manual Integrations
 APPROVED

MMDadoda
 10/8/2020 5:38:23 PM

Quant Time: Oct 07 03:37:29 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100720S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Oct 07 03:05:19 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	529692	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	484215	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	229551	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	115850	22.17	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	88.68%
7) Chloroethane-d5	2.90	69	97782	22.31	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	89.24%
10) 1,1-Dichloroethene-d2	4.03	63	175117	15.78	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	63.12%
20) 2-Butanone-d5	7.09	46	53018	44.79	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	89.58%
24) Chloroform-d	7.65	84	244447	21.87	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	87.48%
26) 1,2-Dichloroethane-d4	8.31	65	123207	22.82	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	91.28%
29) Benzene-d6	8.28	84	502040	22.83	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	91.32%
33) 1,2-Dichloropropane-d6	9.27	67	134542	22.76	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	91.04%
37) Toluene-d8	10.33	98	474110	22.85	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	91.40%
38) trans-1,3-Dichloropropene-	10.58	79	55478	21.28	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	85.12%
39) 2-Hexanone-d5	10.93	63	41475	45.38	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	90.76%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	104971	21.99	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	87.96%
61) 1,2-Dichlorobenzene-d4	13.85	152	165409	22.72	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	90.88%

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
13) Acetone	4.14	43	1846	2.061	ug/L	67
16) Methylene chloride	4.92	84	5552m	0.759	ug/L	10/09/20 Sy

(#) = qualifier out of range (m) = manual integration (+) = signals summed