

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW100720\
 Data File : VW016811.D
 Acq On : 06 Oct 2020 22:42
 Operator : SY/VA
 Sample : L4235-17
 Misc : 3.91G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
ClientSampleId :
 C0AQ3

Manual Integrations
APPROVED

MMDadoda
 10/8/2020 5:38:33 PM

Quant Time: Oct 07 03:15:04 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100720S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Oct 07 03:05:19 2020
 Response via : Initial Calibration

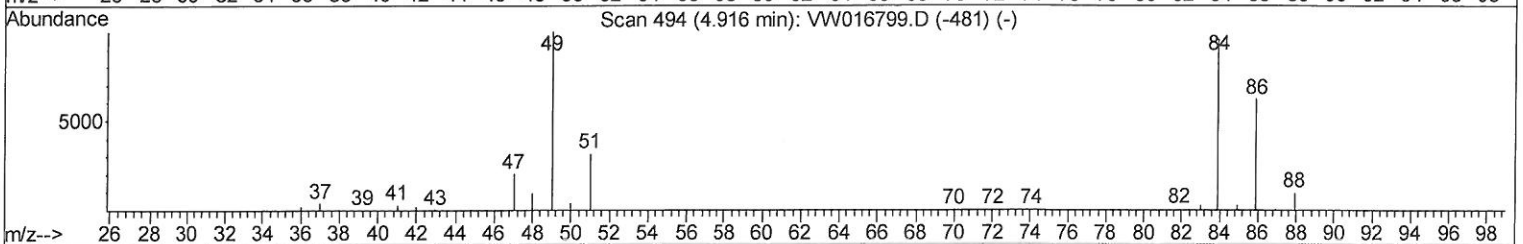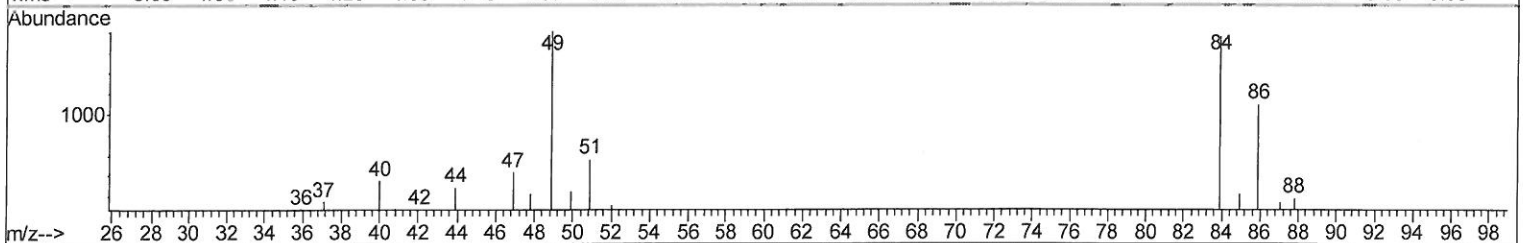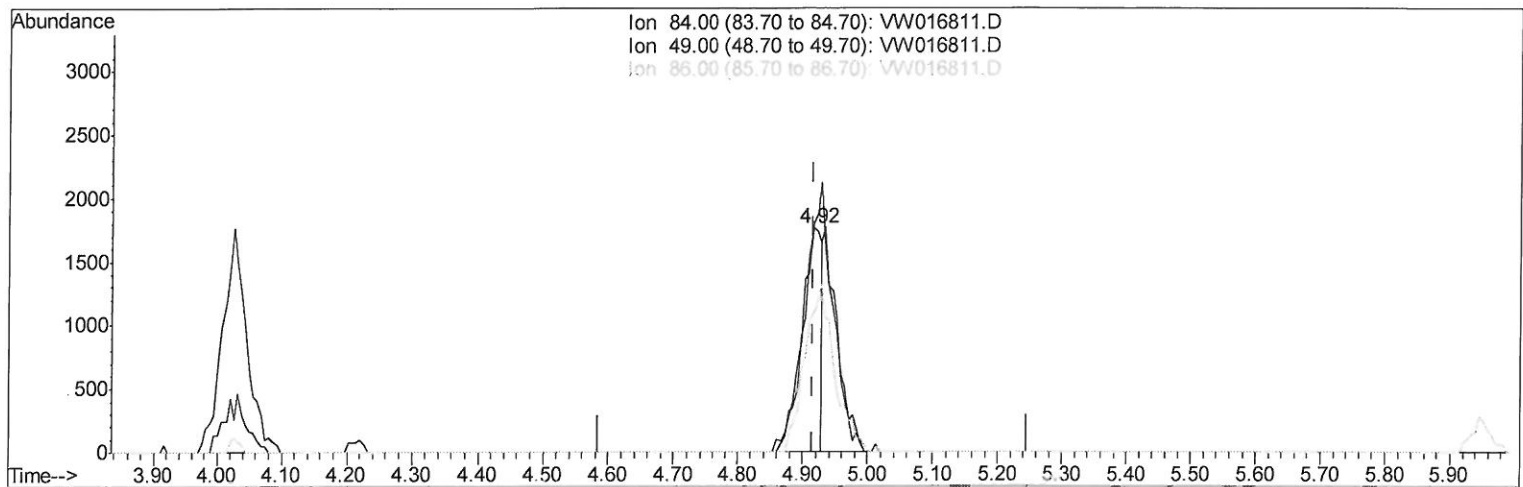

TIC: VW016811.D

(16) Methylene chloride (T)

4.915min (-0.000) 0.52ug/L

response 3663

Ion	Exp%	Act%
84.00	100	100
49.00	104.50	102.49
86.00	65.70	62.24
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW100720\
 Data File : VW016811.D
 Acq On : 06 Oct 2020 22:42
 Operator : SY/VA
 Sample : L4235-17
 Misc : 3.91G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AQ3

Manual Integrations
 APPROVED

MMDadoda
 10/8/2020 5:38:33 PM

Quant Time: Oct 07 03:15:04 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100720S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Oct 07 03:05:19 2020
 Response via : Initial Calibration

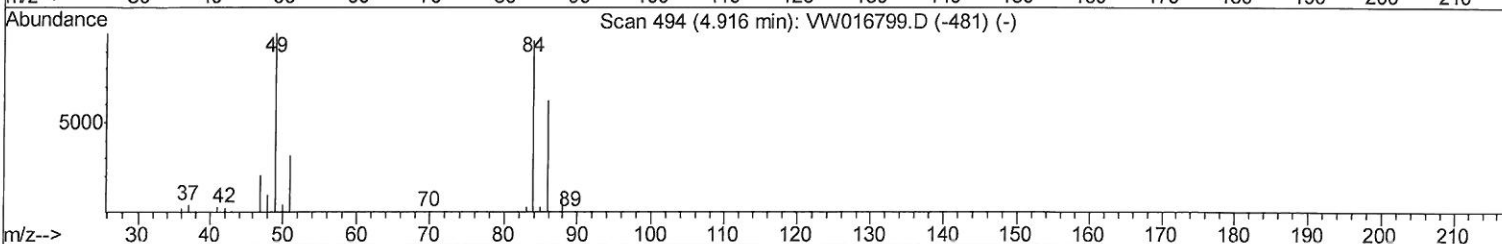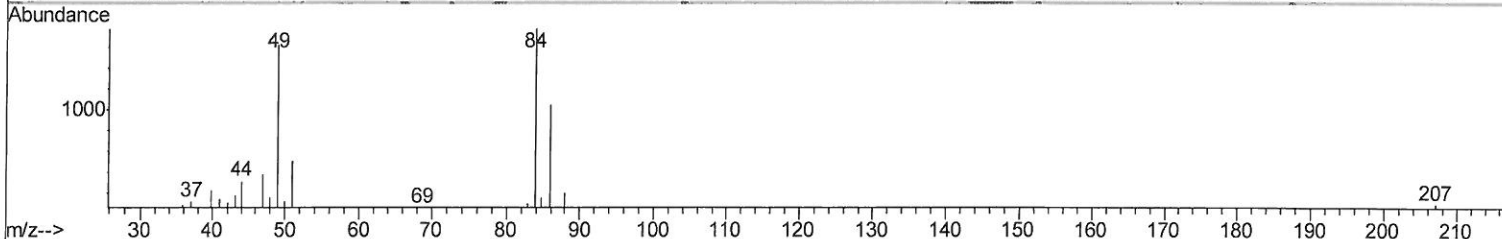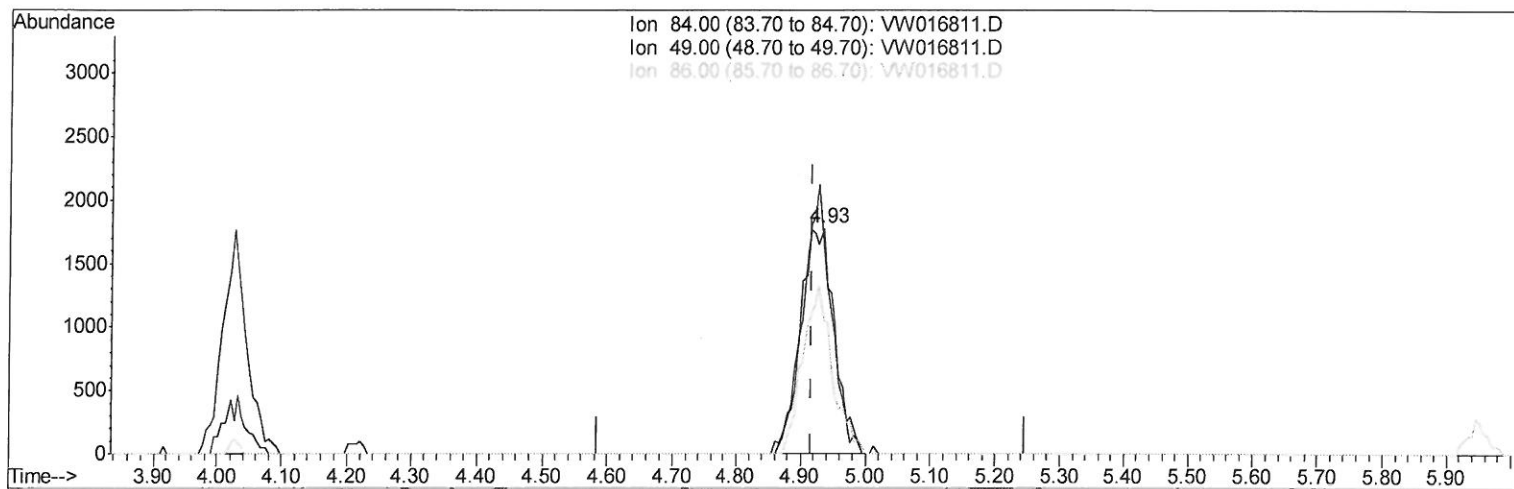

TIC: VW016811.D

(16) Methylene chloride (T)

4.934min (+0.018) 0.90ug/L m

response 6263

Ion	Exp%	Act%
84.00	100	100
49.00	104.50	91.45
86.00	65.70	59.11
0.00	0.00	0.00

Handwritten note: 10/09/20 sy

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW100720\
 Data File : VW016811.D
 Acq On : 06 Oct 2020 22:42
 Operator : SY/VA
 Sample : L4235-17
 Misc : 3.91G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
ClientSampleId :
 C0AQ3

Manual Integrations
APPROVED

MMDadoda
 10/8/2020 5:38:33 PM

Quant Time: Oct 07 03:15:04 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100720S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Oct 07 03:05:19 2020
 Response via : Initial Calibration

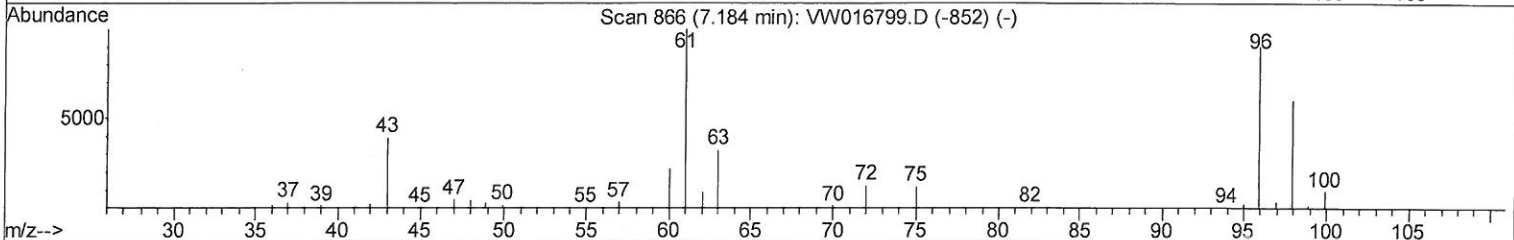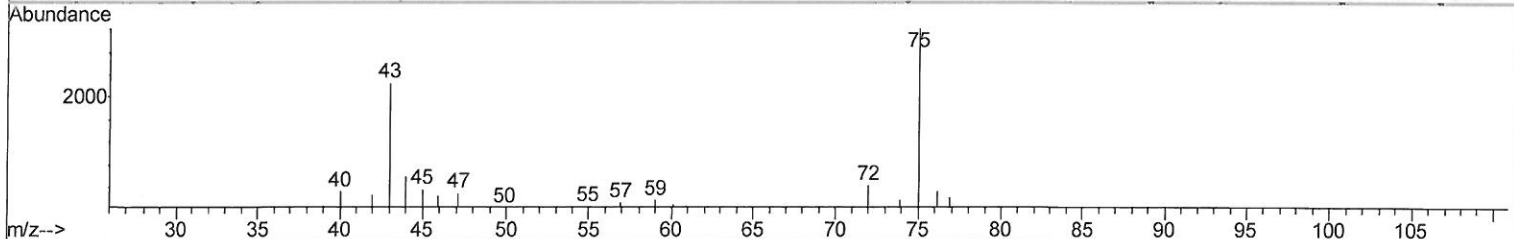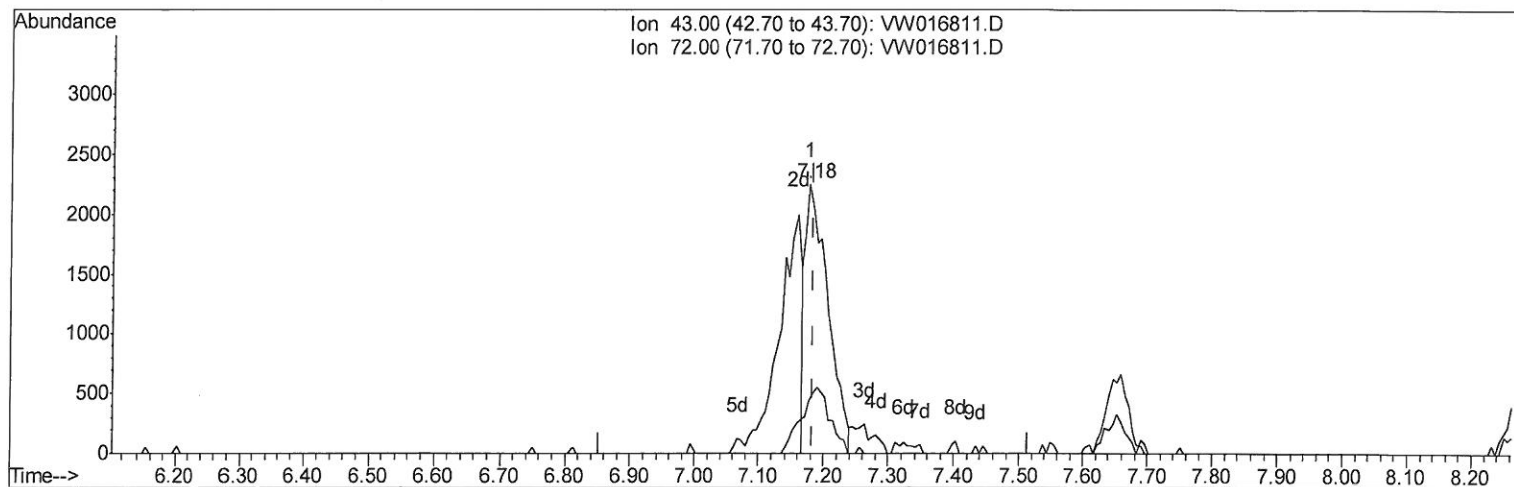

TIC: VW016811.D

(21) 2-Butanone

7.177min (-0.006) 3.82ug/L

response 5497

Ion	Exp%	Act%
43.00	100	100
72.00	32.30	31.09
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW100720\
 Data File : VW016811.D
 Acq On : 06 Oct 2020 22:42
 Operator : SY/VA
 Sample : L4235-17
 Misc : 3.91G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AQ3

Manual Integrations
 APPROVED

MMDadoda
 10/8/2020 5:38:33 PM

Quant Time: Oct 07 03:15:04 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100720S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Oct 07 03:05:19 2020
 Response via : Initial Calibration

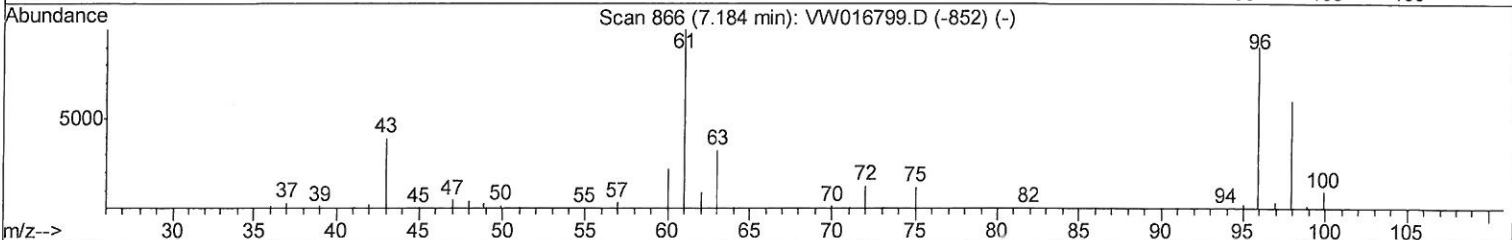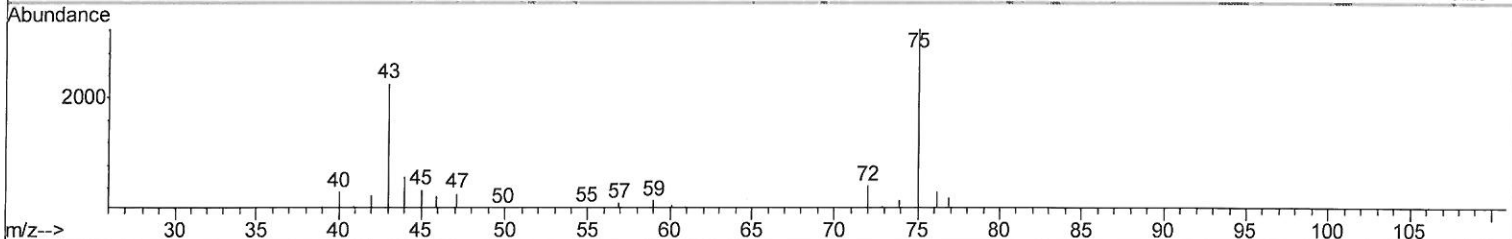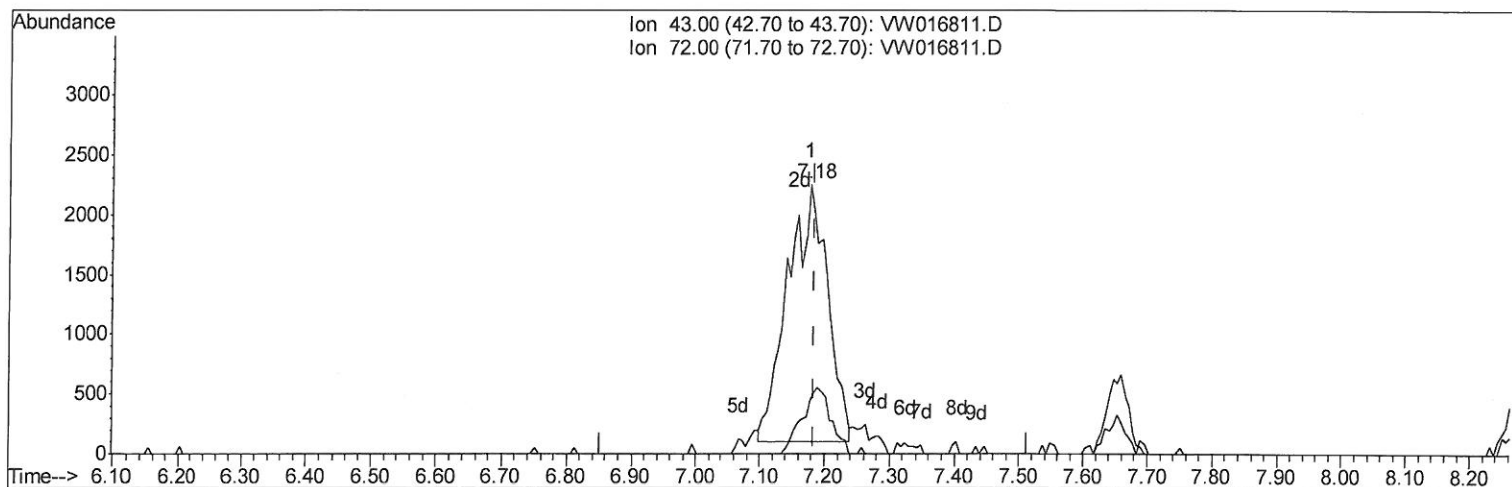

TIC: VW016811.D

(21) 2-Butanone

7.177min (-0.006) 6.36ug/L m

response 9152

Ion	Exp%	Act%
43.00	100	100
72.00	32.30	18.67
0.00	0.00	0.00
0.00	0.00	0.00

10/09/2020

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW100720\
 Data File : VW016811.D
 Acq On : 06 Oct 2020 22:42
 Operator : SY/VA
 Sample : L4235-17
 Misc : 3.91G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampled :
 C0AQ3

Manual Integrations
 APPROVED

MMDadoda
 10/8/2020 5:38:33 PM

Quant Time: Oct 07 04:48:19 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100720S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Oct 07 03:05:19 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	506888	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	336359	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	84686	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	124568	24.91	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	99.64%
7) Chloroethane-d5	2.90	69	109282	26.05	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	104.20%
10) 1,1-Dichloroethene-d2	4.03	63	179299	16.89	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	67.56%
20) 2-Butanone-d5	7.09	46	35476	31.32	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	62.64%
24) Chloroform-d	7.65	84	238710	22.32	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	89.28%
26) 1,2-Dichloroethane-d4	8.31	65	124873	24.17	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	96.68%
29) Benzene-d6	8.28	84	488538	31.98	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	127.92%
33) 1,2-Dichloropropane-d6	9.28	67	132473	32.27	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	129.08%#
37) Toluene-d8	10.33	98	391871	27.19	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	108.76%
38) trans-1,3-Dichloropropene-	10.59	79	35690	19.71	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	78.84%
39) 2-Hexanone-d5	10.93	63	29660	46.72	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	93.44%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	75827	22.86	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	91.44%
61) 1,2-Dichlorobenzene-d4	13.85	152	60240	22.43	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	89.72%

Target Compounds

					Ovalue
13) Acetone	4.15	43	12093	14.109 ug/L	83
16) Methylene chloride	4.93	84	6263m	0.895 ug/L	
21) 2-Butanone	7.18	43	9152m	6.361 ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW100720\
Data File : VW016811.D
Acq On : 06 Oct 2020 22:42
Operator : SY/VA
Sample : L4235-17
Misc : 3.91G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0AQ3

Manual Integrations
APPROVED

MMDadoda
10/8/2020 5:38:33 PM

Quant Time: Oct 07 04:48:19 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100720S.M
Quant Title : VOC Analysis
QLast Update : Wed Oct 07 03:05:19 2020
Response via : Initial Calibration

