

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100721\
 Data File : VW020383.D
 Acq On : 08 Oct 2021 01:00
 Operator : SY/VA
 Sample : M4070-10
 Misc : 5.25g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW7E7

Quant Time: Oct 08 07:40:33 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100621SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Oct 08 07:38:51 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.847	114	266397	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	236237	25.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	96019	25.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	83679	22.79	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	91.16%
7) Chloroethane-d5	2.885	69	42047	26.43	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	105.72%
11) 1,1-Dichloroethene-d2	4.013	63	123689	16.36	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	65.44%
21) 2-Butanone-d5	7.079	46	43241	46.36	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	92.72%
24) Chloroform-d	7.653	84	171203	22.38	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	89.52%
26) 1,2-Dichloroethane-d4	8.305	65	96766	23.12	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	92.48%
32) Benzene-d6	8.274	84	336120	23.50	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	94.00%
36) 1,2-Dichloropropane-d6	9.280	67	108974	24.02	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	96.08%
41) Toluene-d8	10.323	98	292171	22.55	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	90.20%
43) trans-1,3-Dichloroprop...	10.579	79	38394	20.80	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	83.20%
47) 2-Hexanone-d5	10.926	63	28639	45.67	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	91.34%
56) 1,1,2,2-Tetrachloroeth...	12.694	84	71518	22.59	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	90.36%
66) 1,2-Dichlorobenzene-d4	13.853	152	81931	24.37	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	97.48%
Target Compounds					Qvalue	
13) Acetone	4.135	43	7220	7.53	ug/L	78


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100721\
Data File : VW020383.D
Acq On : 08 Oct 2021 01:00
Operator : SY/VA
Sample : M4070-10
Misc : 5.25g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW7E7

Quant Time: Oct 08 07:40:33 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100621SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Oct 08 07:38:51 2021
Response via : Initial Calibration

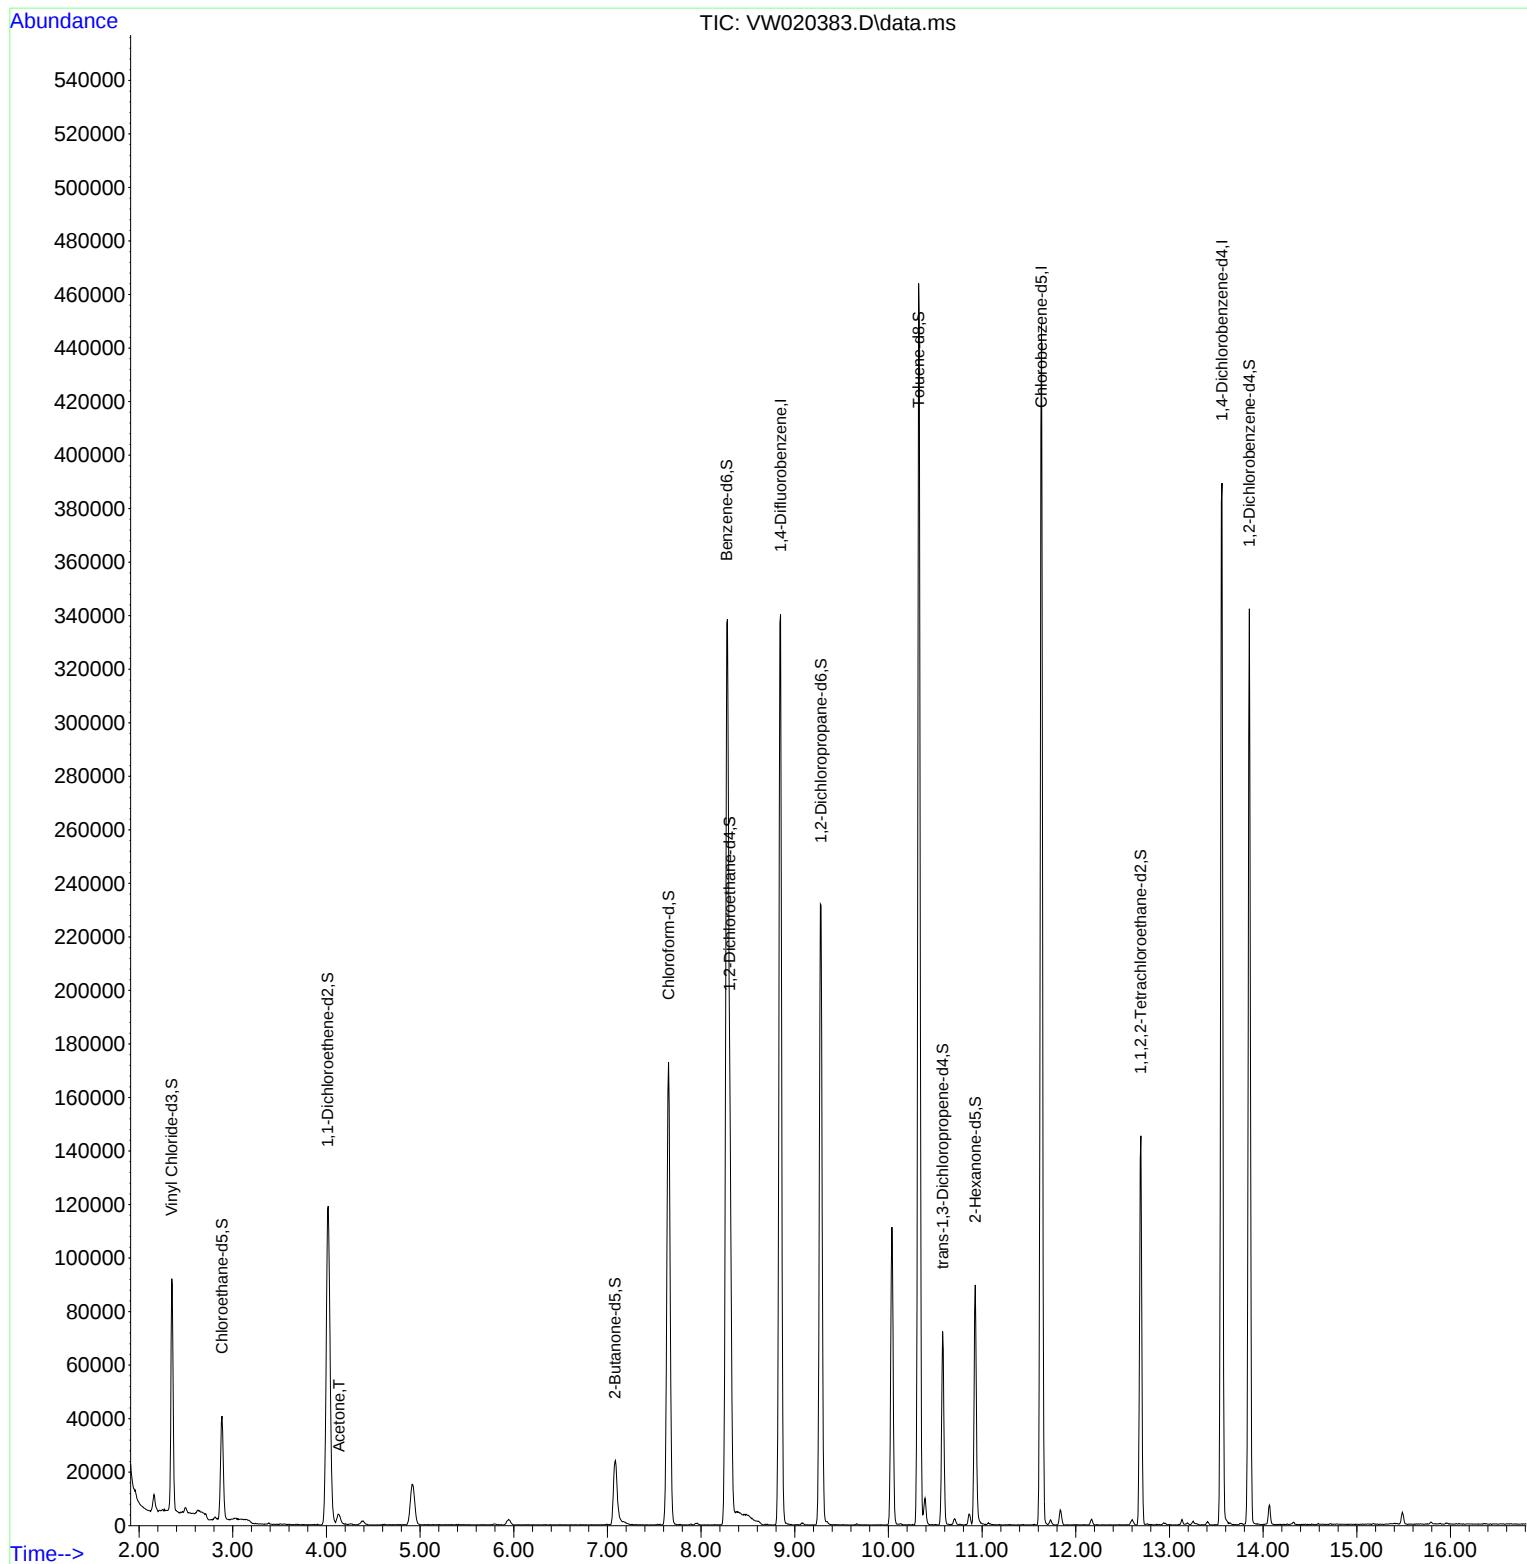

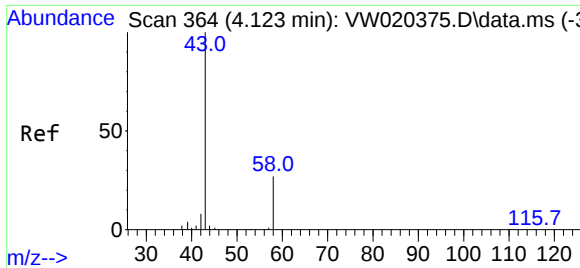

#13
 Acetone
 Concen: 7.53 ug/L
 RT: 4.135 min Scan# 366
 Delta R.T. 0.012 min
 Lab File: VW020383.D
 Acq: 08 Oct 2021 01:00

Instrument :
 MSVOA_W
 ClientSampleId :
 EW7E7

Tgt Ion: 43 Resp: 7220
 Ion Ratio Lower Upper
 43 100
 58 17.3 0.0 58.4

