

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100721\
 Data File : VW020386.D
 Acq On : 08 Oct 2021 02:12
 Operator : SY/VA
 Sample : M4070-13
 Misc : 5.24g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW7F0

Quant Time: Oct 08 07:40:51 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100621SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Oct 08 07:38:51 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.848	114	265533	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	224234	25.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	83633	25.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	82562	22.56	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	90.24%
7) Chloroethane-d5	2.879	69	36181	22.82	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	91.28%
11) 1,1-Dichloroethene-d2	4.013	63	121580	16.13	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	64.52%
21) 2-Butanone-d5	7.080	46	40877	43.97	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	87.94%
24) Chloroform-d	7.653	84	177199	23.24	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	92.96%
26) 1,2-Dichloroethane-d4	8.311	65	96930	23.23	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	92.92%
32) Benzene-d6	8.281	84	347795	25.62	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	102.48%
36) 1,2-Dichloropropane-d6	9.275	67	113778	26.42	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	105.68%
41) Toluene-d8	10.323	98	289787	23.57	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	94.28%
43) trans-1,3-Dichloroprop...	10.579	79	35958	20.52	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	82.08%
47) 2-Hexanone-d5	10.927	63	25987	43.66	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	87.32%
56) 1,1,2,2-Tetrachloroeth...	12.695	84	67323	22.40	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	89.60%
66) 1,2-Dichlorobenzene-d4	13.853	152	70943	24.22	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	96.88%
Target Compounds						
13) Acetone	4.135	43	3800	3.98	ug/L	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100721\
Data File : VW020386.D
Acq On : 08 Oct 2021 02:12
Operator : SY/VA
Sample : M4070-13
Misc : 5.24g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW7F0

Quant Time: Oct 08 07:40:51 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100621SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Oct 08 07:38:51 2021
Response via : Initial Calibration

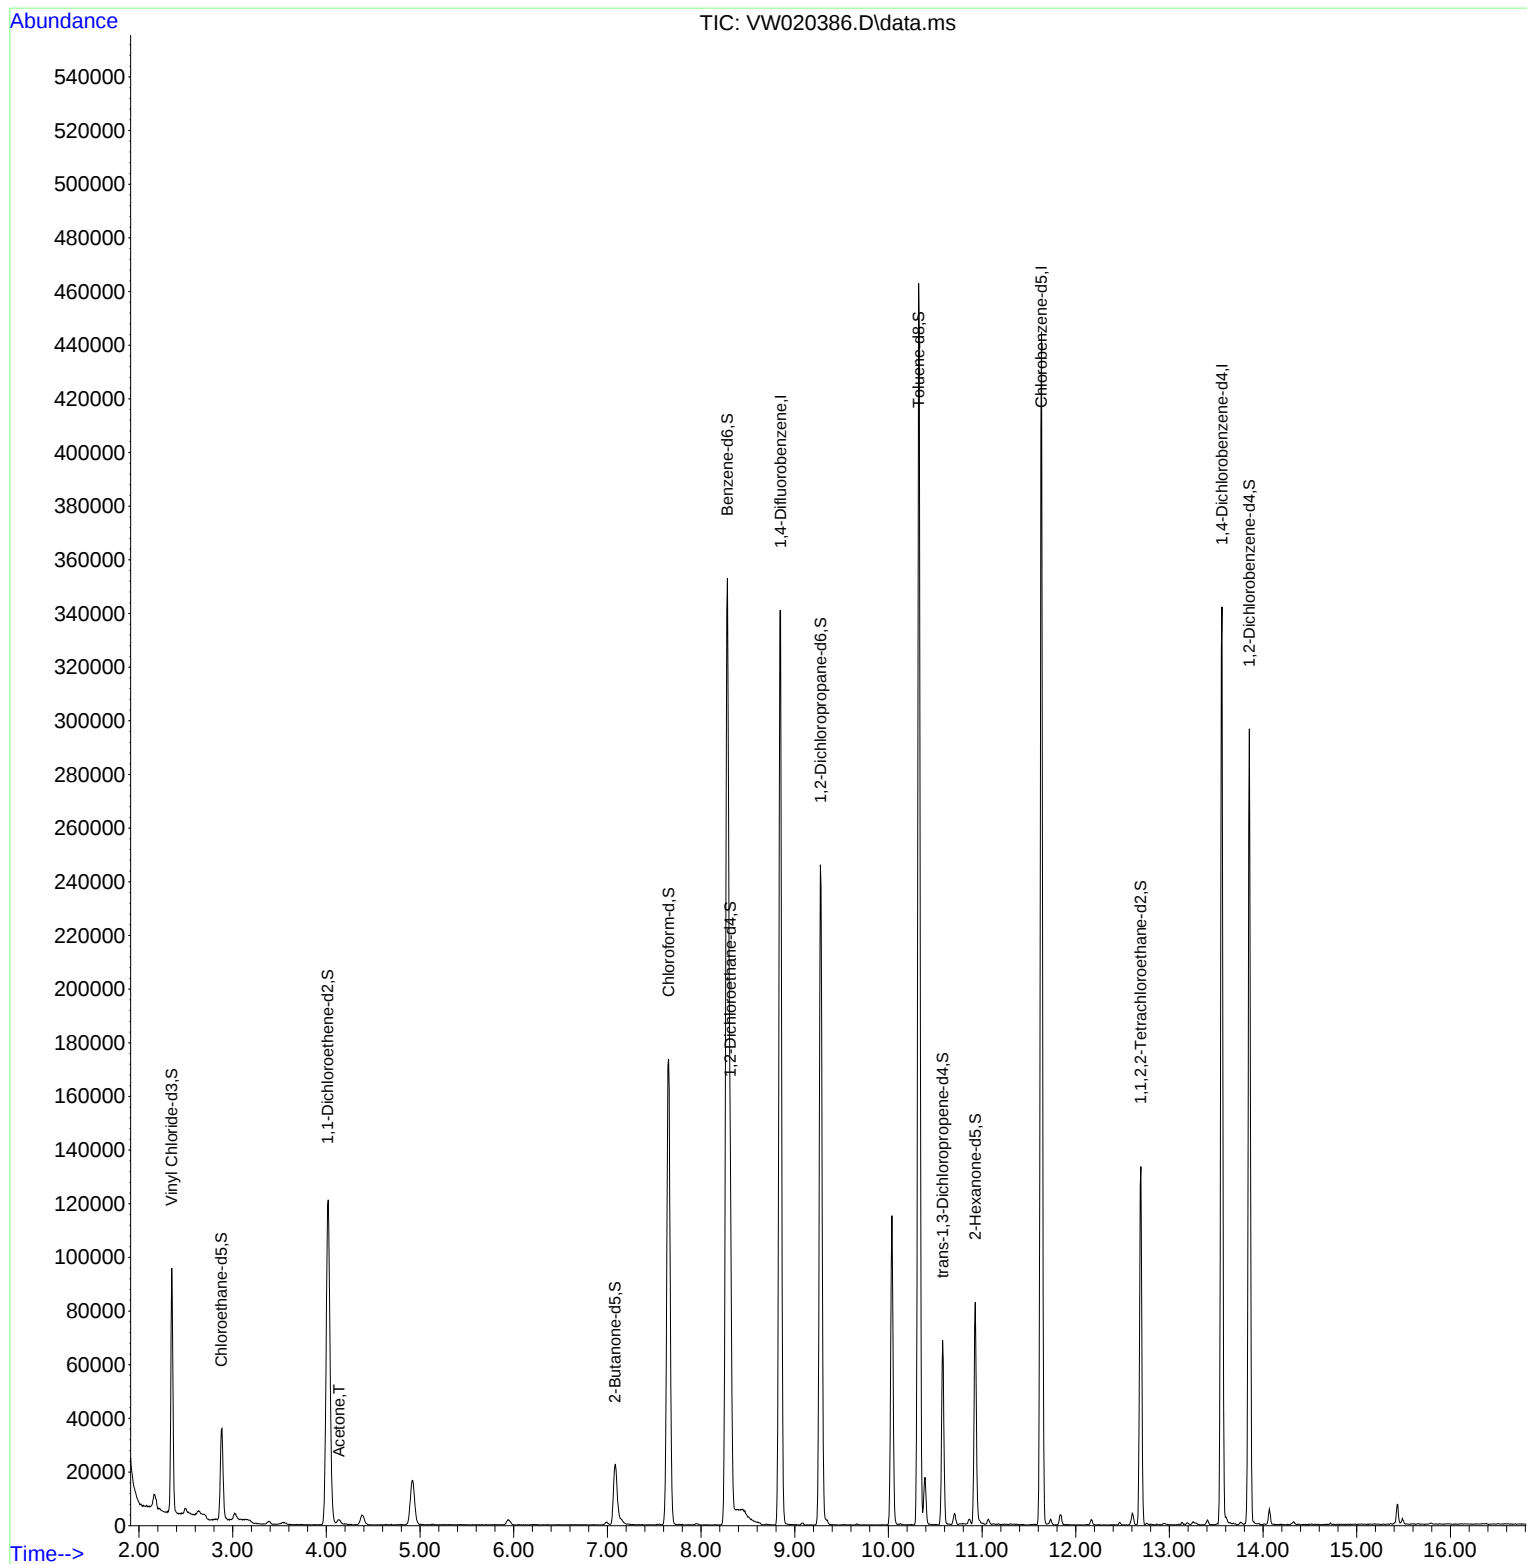

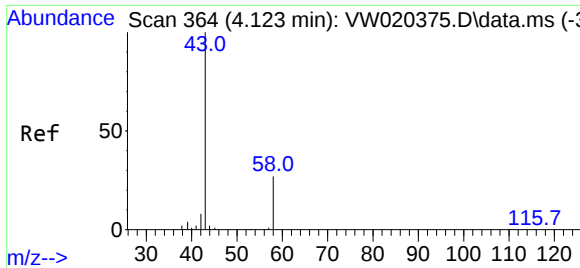

#13
 Acetone
 Concen: 3.98 ug/L
 RT: 4.135 min Scan# 366
 Delta R.T. 0.012 min
 Lab File: VW020386.D
 Acq: 08 Oct 2021 02:12

Instrument :
 MSVOA_W
 ClientSampleId :
 EW7F0

Tgt Ion: 43 Resp: 3800
 Ion Ratio Lower Upper
 43 100
 58 27.7 0.0 58.4

