

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100721\
 Data File : VW020392.D
 Acq On : 08 Oct 2021 04:36
 Operator : SY/VA
 Sample : M4103-07
 Misc : 4.05g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AC1

Quant Time: Oct 08 07:41:29 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100621SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Oct 08 07:38:51 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.848	114	90985	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	62127	25.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	12340	25.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	31671	25.26	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	101.04%
7) Chloroethane-d5	2.885	69	17045	31.37	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	125.48%
11) 1,1-Dichloroethene-d2	4.013	63	46014	17.82	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	71.28%
21) 2-Butanone-d5	7.086	46	16280	51.11	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	102.22%
24) Chloroform-d	7.653	84	70431	26.96	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	107.84%
26) 1,2-Dichloroethane-d4	8.311	65	36097	25.25	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	101.00%
32) Benzene-d6	8.281	84	127374	33.86	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	135.44%#
36) 1,2-Dichloropropane-d6	9.275	67	47189	39.55	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	158.20%#
41) Toluene-d8	10.329	98	85900	25.21	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	100.84%
43) trans-1,3-Dichloroprop...	10.579	79	7620	15.70	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	62.80%
47) 2-Hexanone-d5	10.927	63	8637	52.38	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	104.76%
56) 1,1,2,2-Tetrachloroeth...	12.695	84	29187	35.05	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	140.20%#
66) 1,2-Dichlorobenzene-d4	13.853	152	14918	34.52	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	138.08%#
Target Compounds					Qvalue	
13) Acetone	4.135	43	6193	18.91	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100721\
Data File : VW020392.D
Acq On : 08 Oct 2021 04:36
Operator : SY/VA
Sample : M4103-07
Misc : 4.05g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0AC1

Quant Time: Oct 08 07:41:29 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100621SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Oct 08 07:38:51 2021
Response via : Initial Calibration

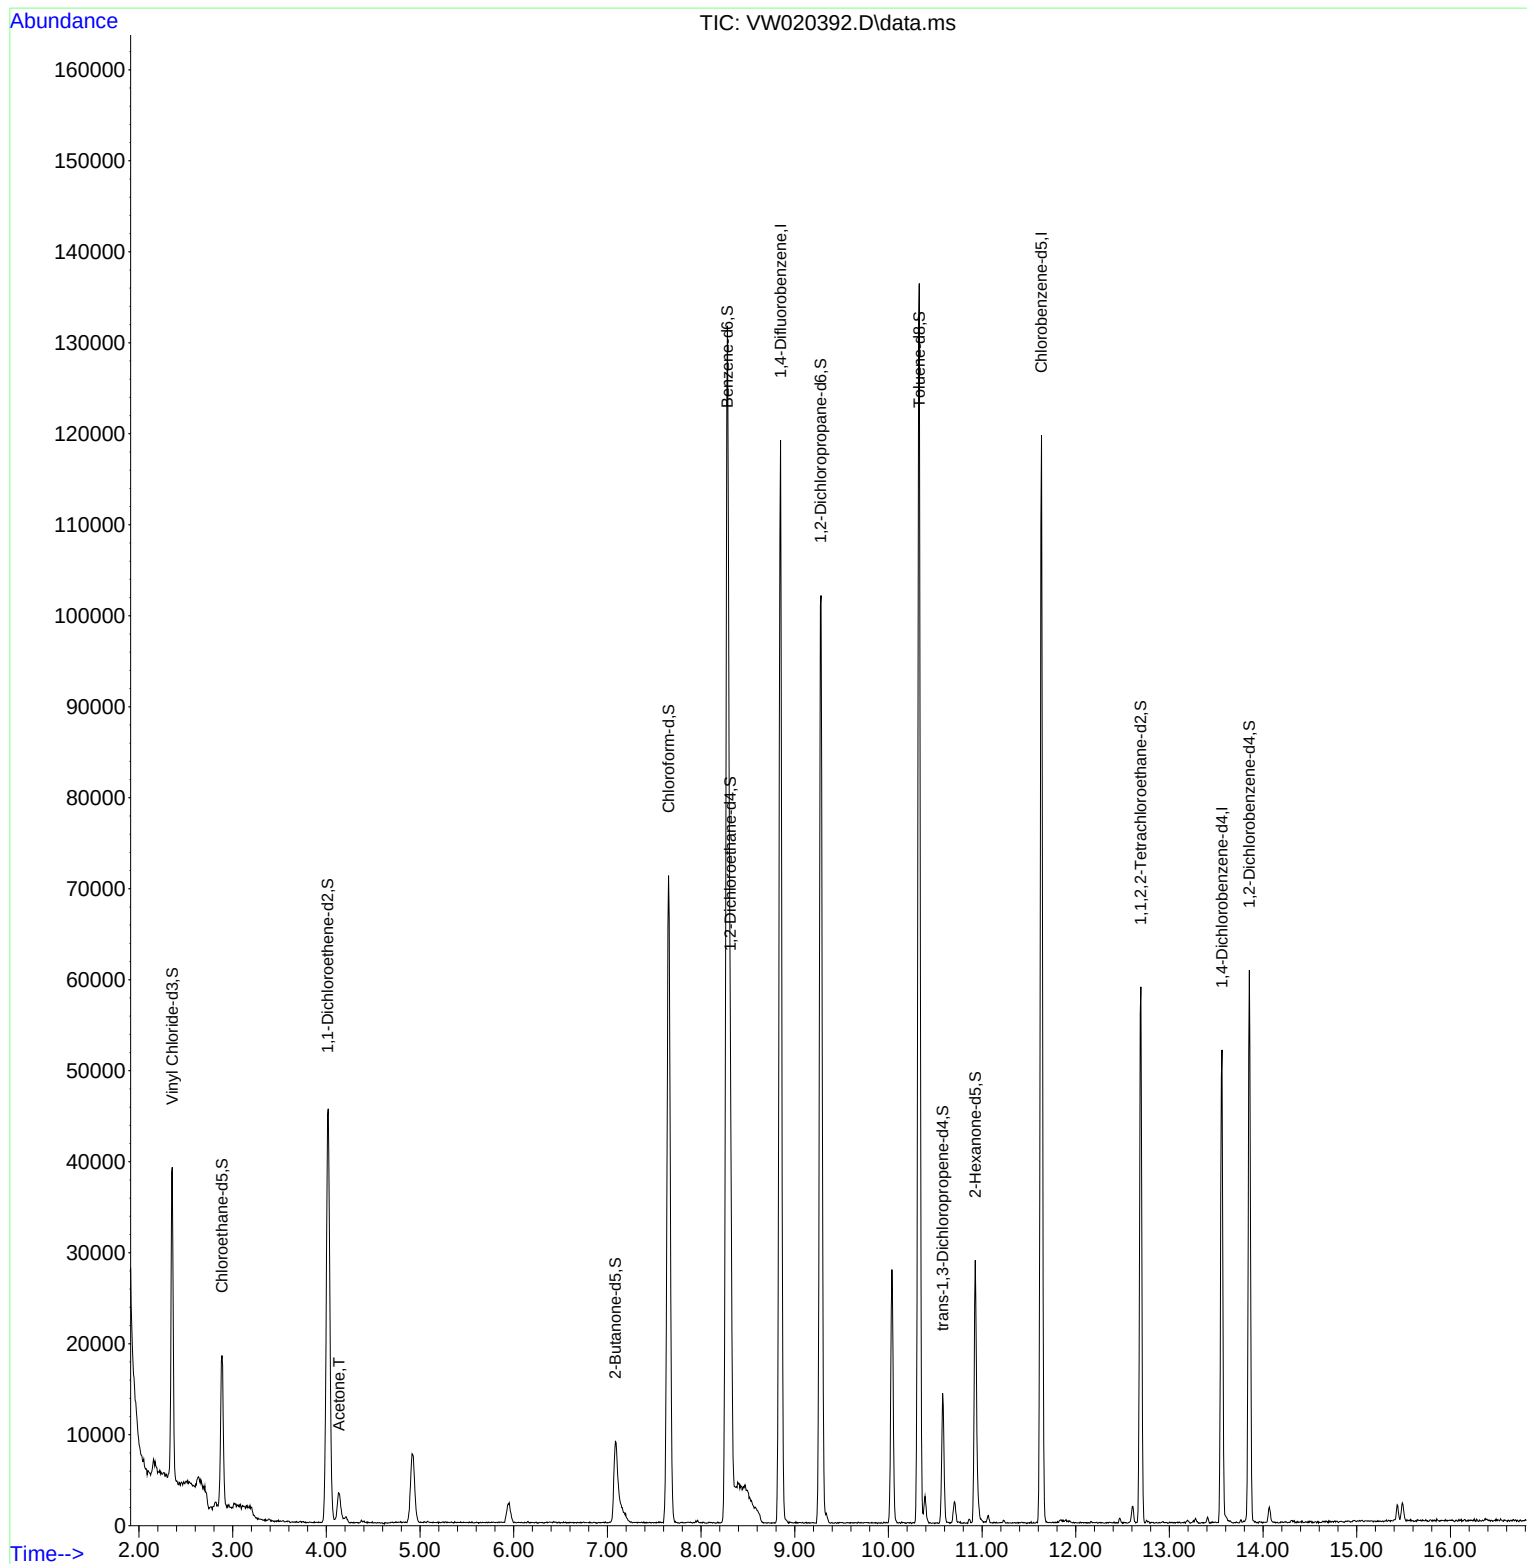

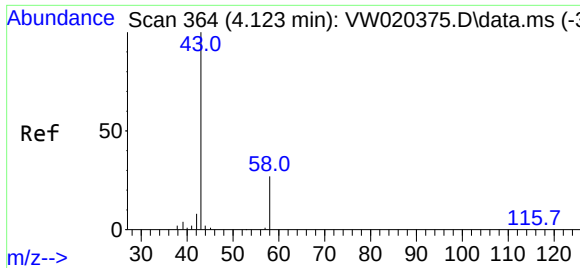

#13
 Acetone
 Concen: 18.91 ug/L
 RT: 4.135 min Scan# 366
 Delta R.T. 0.012 min
 Lab File: VW020392.D
 Acq: 08 Oct 2021 04:36

Instrument :
 MSVOA_W
 ClientSampled :
 C0AC1

Tgt Ion: 43 Resp: 6193
 Ion Ratio Lower Upper
 43 100
 58 26.6 0.0 58.4

