
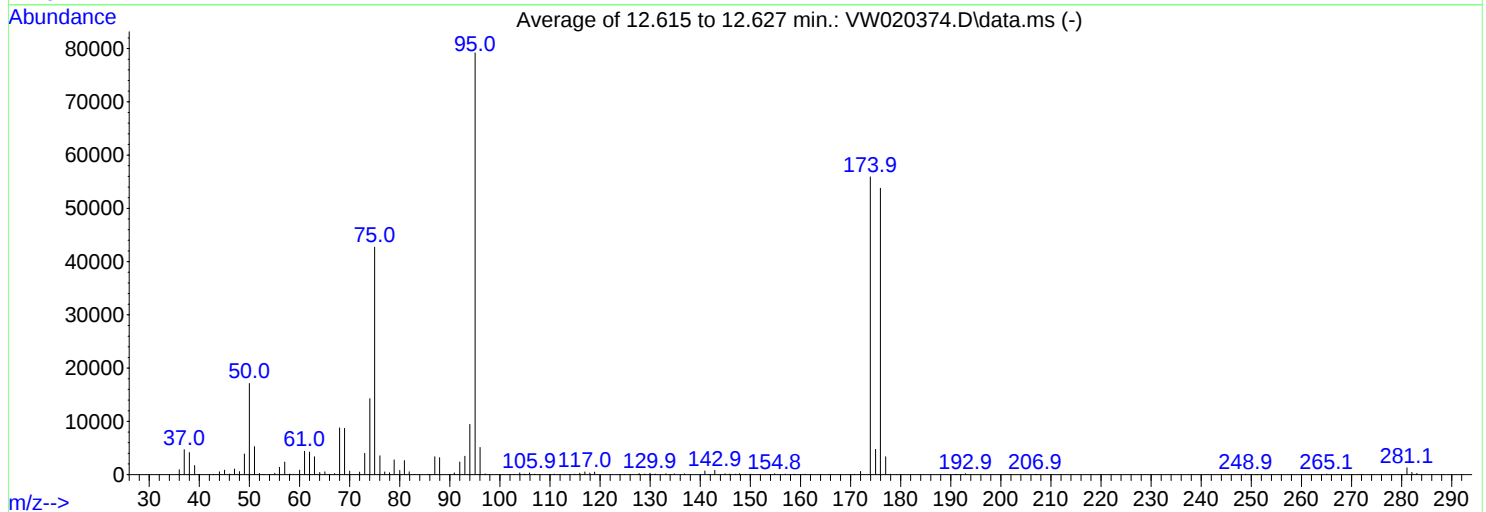


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100721\
 Data File : VW020374.D
 Acq On : 07 Oct 2021 20:29
 Operator : SY/VA
 Sample : BFB447
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB447

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100621SMA.M
 Title : SFAM01.0
 Last Update : Fri Oct 08 07:38:51 2021

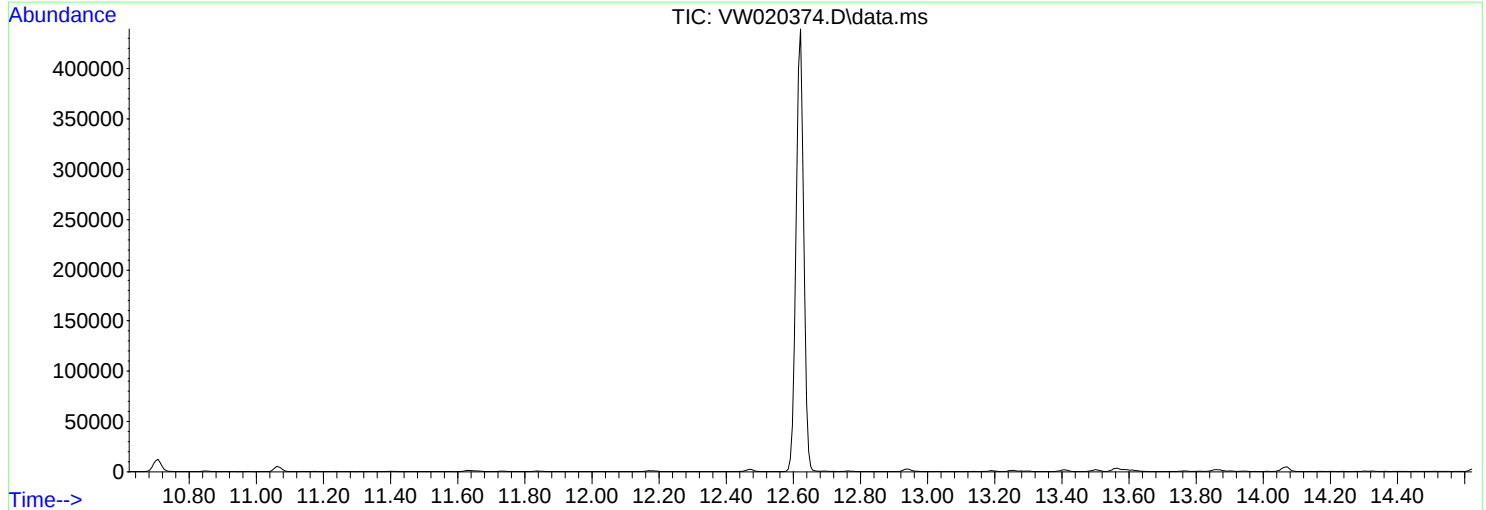

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.6	17136	PASS
75	95	30	80	54.0	42736	PASS
95	95	100	100	100.0	79203	PASS
96	95	5	9	6.5	5114	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	70.6	55912	PASS
175	174	5	9	8.5	4751	PASS
176	174	95	105	96.2	53789	PASS
177	176	5	10	6.3	3366	PASS

m/z	Abundance
40.00	121.0
44.00	232.0

Instrument :
MSVOA_W
ClientSampleId :
BFB447

m/z	Abundance
36.00	1158.0
37.00	5326.0
38.00	4650.0
39.00	1872.0
40.00	223.0
42.90	74.0
44.00	948.0
45.00	976.0
46.10	127.0
47.00	1308.0
48.00	590.0
49.00	4186.0
50.00	19104.0
51.00	5960.0
52.00	214.0
52.90	83.0
55.10	278.0
56.00	1643.0
57.10	2579.0
58.10	131.0
60.00	924.0
61.00	4801.0
62.00	4586.0
63.00	3597.0
64.10	582.0
65.10	702.0
66.10	73.0
67.00	252.0
68.00	9642.0
69.00	9395.0
70.00	684.0
72.00	547.0
73.00	4505.0
74.10	15163.0
75.00	45304.0
76.00	3945.0
77.00	532.0
77.90	400.0
78.90	3180.0
80.00	816.0
81.00	2900.0
81.90	610.0
82.90	69.0
87.00	3501.0
87.90	3243.0
90.90	368.0
92.00	2552.0
93.00	3531.0
94.00	9618.0
95.00	83008.0
96.10	5497.0
97.10	174.0
103.00	78.0
104.00	332.0
105.00	138.0
105.90	397.0
107.00	100.0
109.90	71.0
111.00	88.0
112.90	79.0
114.90	98.0
115.90	255.0
117.00	529.0
118.00	289.0
118.90	493.0
124.80	97.0
127.80	294.0
129.00	123.0
130.00	322.0
131.00	133.0
133.10	273.0
133.80	62.0
134.10	52.0
134.90	190.0
136.80	152.0
140.90	591.0
141.70	105.0
142.90	783.0
144.90	219.0
146.00	113.0
147.00	120.0
147.80	173.0
149.00	72.0
149.90	83.0
154.90	187.0
157.00	126.0
158.80	94.0
160.90	103.0
170.80	120.0
172.00	668.0
173.90	55064.0
175.00	4747.0

Instrument :
MSVOA_W
ClientSampleId :
BFB447

176.00	47664.0
177.00	3401.0
178.00	112.0
179.10	54.0
190.90	148.0
192.00	65.0
193.00	269.0
206.90	204.0
248.90	140.0
250.90	52.0
251.20	56.0
265.00	143.0
266.00	85.0
267.10	57.0
281.00	1836.0
282.00	570.0
283.00	344.0
284.00	79.0

Instrument :
MSVOA_W
ClientSampleId :
BFB447

m/z	Abundance
36.00	1022.0
37.00	5185.0
38.00	4671.0
39.10	1915.0
40.00	128.0
42.90	85.0
44.00	729.0
45.00	891.0
46.00	131.0
47.00	1068.0
48.00	669.0
49.00	4284.0
50.00	18752.0
51.00	5661.0
52.00	262.0
52.90	63.0
55.00	295.0
56.00	1448.0
57.00	2669.0
58.00	124.0
60.00	911.0
61.00	4873.0
62.00	4639.0
63.00	3857.0
64.00	381.0
65.00	518.0
65.90	113.0
67.00	218.0
68.00	9797.0
69.00	9733.0
70.00	673.0
72.00	473.0
73.00	4318.0
74.00	16069.0
75.00	48192.0
76.00	3881.0
77.00	616.0
78.00	414.0
78.90	2873.0
80.00	908.0
80.90	2952.0
81.90	618.0
83.00	80.0
85.80	188.0
87.00	3934.0
88.00	3703.0
90.90	340.0
92.00	2523.0
93.00	3990.0
94.00	11010.0
95.00	88448.0
96.00	5775.0
97.00	174.0
102.80	58.0
104.00	397.0
104.80	103.0
105.90	343.0
107.00	80.0
110.00	81.0
110.90	99.0
113.00	84.0
115.00	117.0
116.00	340.0
116.90	557.0
118.00	336.0
118.90	553.0
124.00	58.0
124.90	55.0
127.80	344.0
128.90	148.0
130.00	272.0
131.00	105.0
133.20	175.0
134.20	58.0
134.90	141.0
136.90	169.0
140.00	75.0
140.90	793.0
142.00	64.0
142.90	925.0
145.00	190.0
145.80	148.0
147.00	79.0
147.90	210.0
149.00	72.0
150.00	95.0
154.00	74.0
154.90	178.0
156.90	131.0
158.80	106.0
160.90	84.0
170.80	106.0

Instrument :
MSVOA_W
ClientSampleId :
BFB447

172.00	680.0
174.00	67096.0
175.00	5349.0
175.90	64416.0
177.00	3498.0
177.90	102.0
191.10	116.0
192.90	200.0
207.10	117.0
248.90	96.0
265.10	162.0
281.10	1357.0
282.10	516.0
283.10	235.0

Instrument :
MSVOA_W
ClientSampleId :
BFB447

m/z	Abundance
36.00	655.0
37.00	3530.0
38.00	3155.0
39.00	1371.0
40.00	173.0
42.90	54.0
44.00	624.0
45.10	661.0
46.00	88.0
47.00	821.0
48.00	497.0
49.00	3126.0
50.00	13551.0
51.00	4155.0
52.00	171.0
55.00	211.0
56.00	1030.0
57.00	1886.0
58.00	74.0
60.00	724.0
61.00	3503.0
62.00	3472.0
63.00	2659.0
64.00	270.0
65.00	420.0
66.10	52.0
67.00	199.0
68.00	6903.0
69.00	6954.0
70.00	640.0
72.00	383.0
73.00	3149.0
74.00	11629.0
75.00	34712.0
76.10	2820.0
77.00	382.0
78.00	306.0
78.90	2215.0
80.00	582.0
81.00	2114.0
81.90	441.0
83.00	74.0
86.00	95.0
87.00	2681.0
87.90	2586.0
90.90	285.0
92.00	2019.0
93.00	2854.0
94.00	7693.0
95.10	66152.0
96.00	4071.0
97.10	120.0
103.90	272.0
105.10	107.0
105.80	232.0
106.90	71.0
110.00	52.0
110.80	79.0
112.90	70.0
114.90	75.0
116.00	220.0
117.00	456.0
117.90	332.0
118.90	450.0
124.00	69.0
128.00	235.0
128.90	89.0
129.90	227.0
131.00	96.0
133.10	88.0
134.80	138.0
136.80	89.0
136.90	88.0
140.00	76.0
140.90	689.0
141.80	63.0
142.90	713.0
144.90	130.0
146.00	71.0
147.00	75.0
147.90	124.0
149.90	73.0
154.80	154.0
156.90	85.0
158.90	82.0
160.90	82.0
172.00	489.0
174.00	45576.0
175.00	4157.0
176.00	49288.0
177.00	3198.0
177.90	97.0

Instrument :
MSVOA_W
ClientSampleId :
BFB447

193.00	104.0
248.90	60.0
265.00	76.0
281.10	661.0
282.00	175.0
283.10	183.0

Instrument :
MSVOA_W
ClientSampleId :
BFB447