


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW100819\  
Data File : VW013477.D  
Acq On : 08 Oct 2019 09:25  
Operator : SY/VA  
Sample : BFB  
Misc : 5.00G/5ML/MSVOA W/SOIL  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_W  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_W\METHOD\82W100819S.M  
Title : SW846 8260  
Last Update : Wed Oct 09 05:54:09 2019

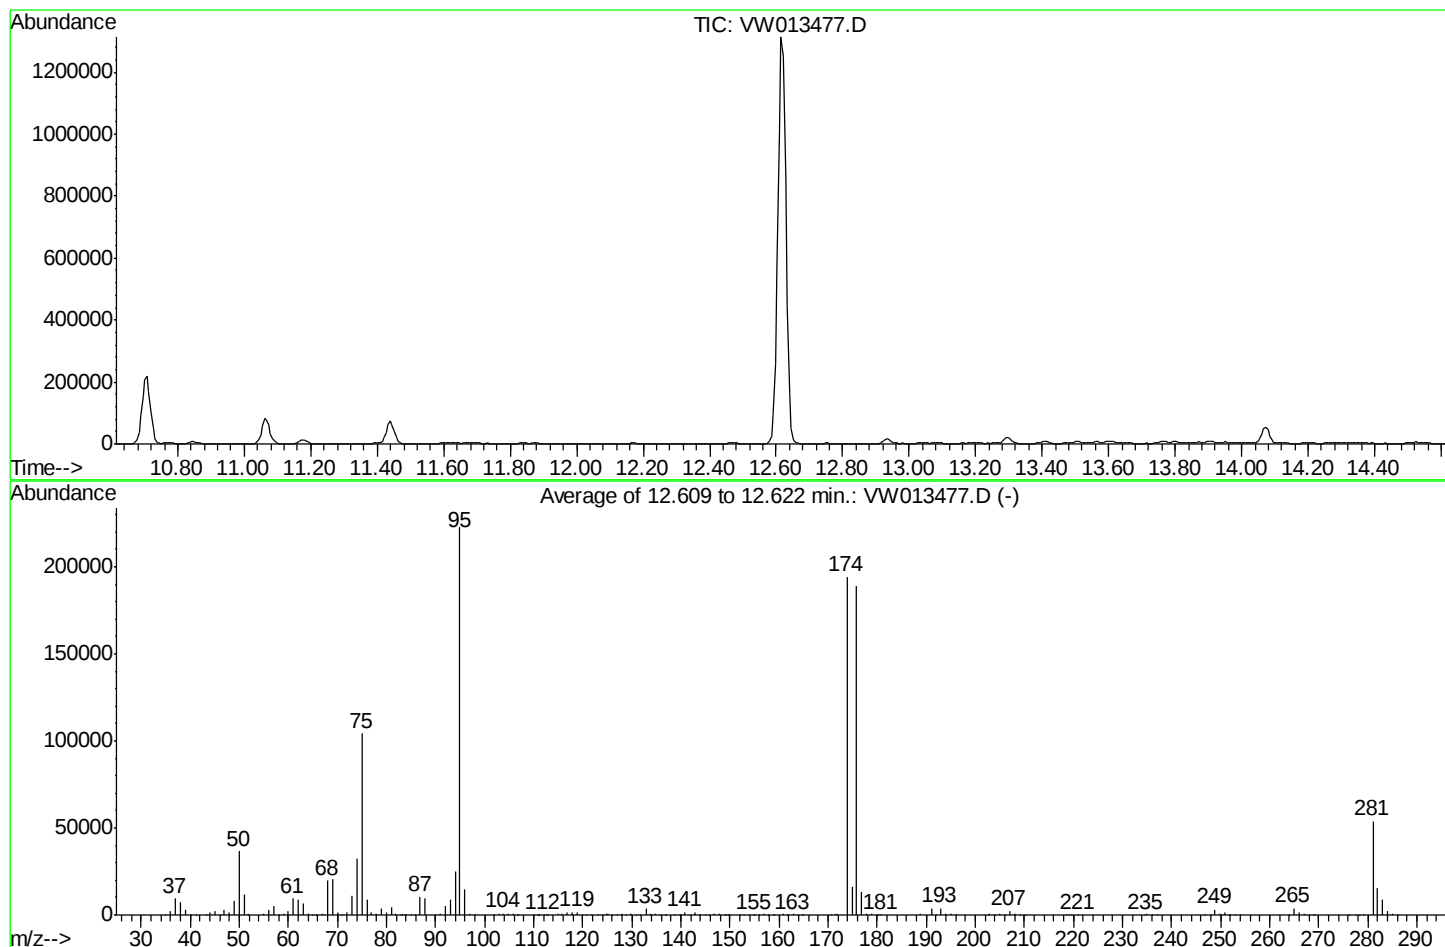

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1748

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 16.5      | 36733   | PASS             |
| 75          | 95           | 30           | 60           | 46.7      | 104104  | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 222698  | PASS             |
| 96          | 95           | 5            | 9            | 6.7       | 14882   | PASS             |
| 173         | 174          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 174         | 95           | 50           | 100          | 87.3      | 194325  | PASS             |
| 175         | 174          | 5            | 9            | 8.3       | 16119   | PASS             |
| 176         | 174          | 95           | 101          | 97.1      | 188736  | PASS             |
| 177         | 176          | 5            | 9            | 6.9       | 13092   | PASS             |