

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW100820\
 Data File : VW016835.D
 Acq On : 07 Oct 2020 16:01
 Operator : SY/VA
 Sample : VIBLK11
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK11

Manual Integrations
 APPROVED

MMDadoda
 10/12/2020 1:55:27 PM

Quant Time: Oct 08 08:40:56 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100720S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Oct 08 08:32:41 2020
 Response via : Initial Calibration

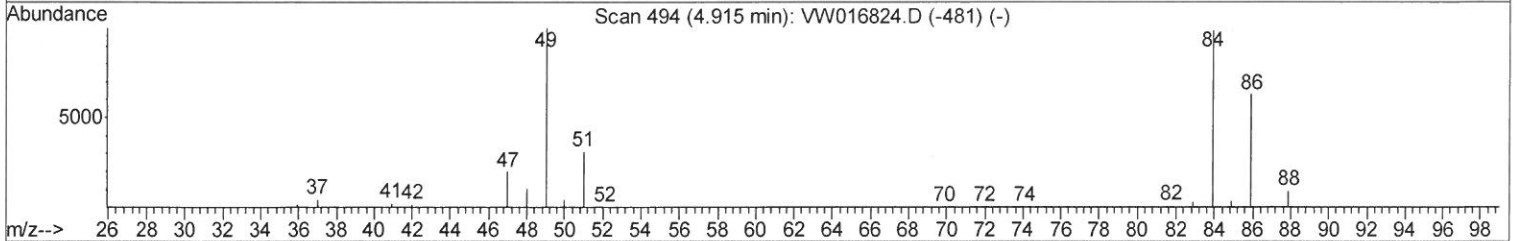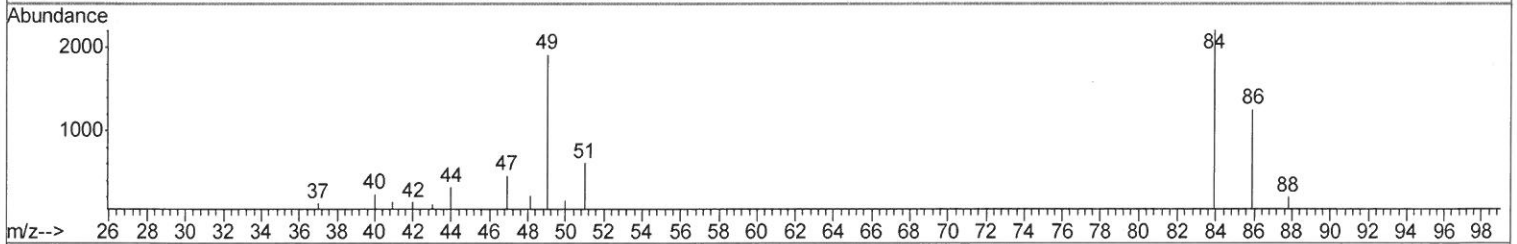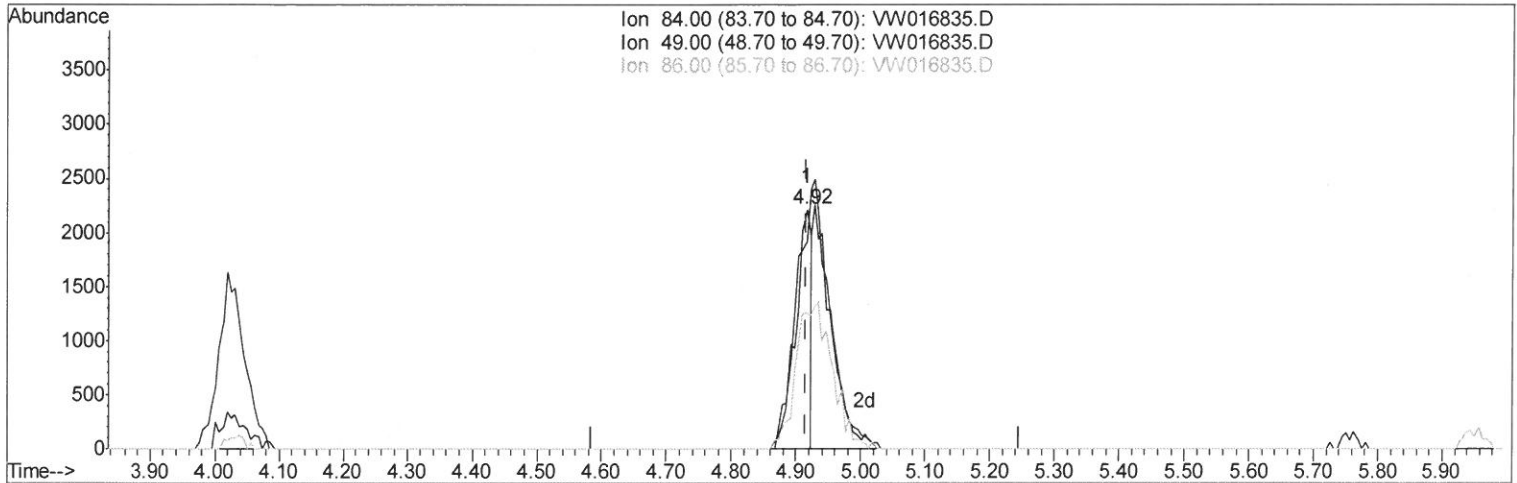

TIC: VW016835.D

(16) Methylene chloride (T)

4.915min (-0.000) 0.52ug/L

response 3723

Ion	Exp%	Act%
84.00	100	100
49.00	104.50	86.88
86.00	65.70	56.90
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW100820\
 Data File : VW016835.D
 Acq On : 07 Oct 2020 16:01
 Operator : SY/VA
 Sample : VIBLK11
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK11

Manual Integrations
 APPROVED

MMDadoda
 10/12/2020 1:55:27 PM

Quant Time: Oct 08 08:40:56 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100720S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Oct 08 08:32:41 2020
 Response via : Initial Calibration

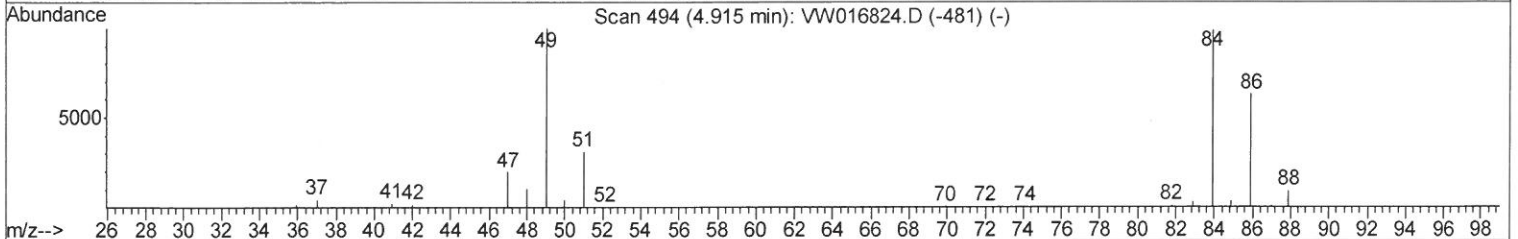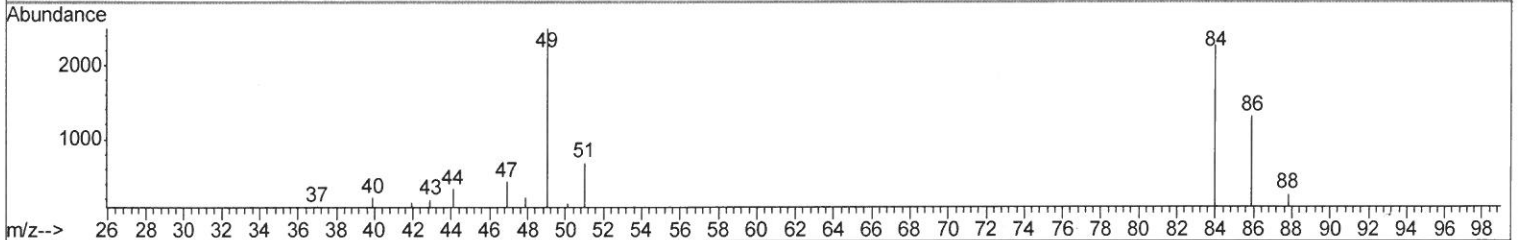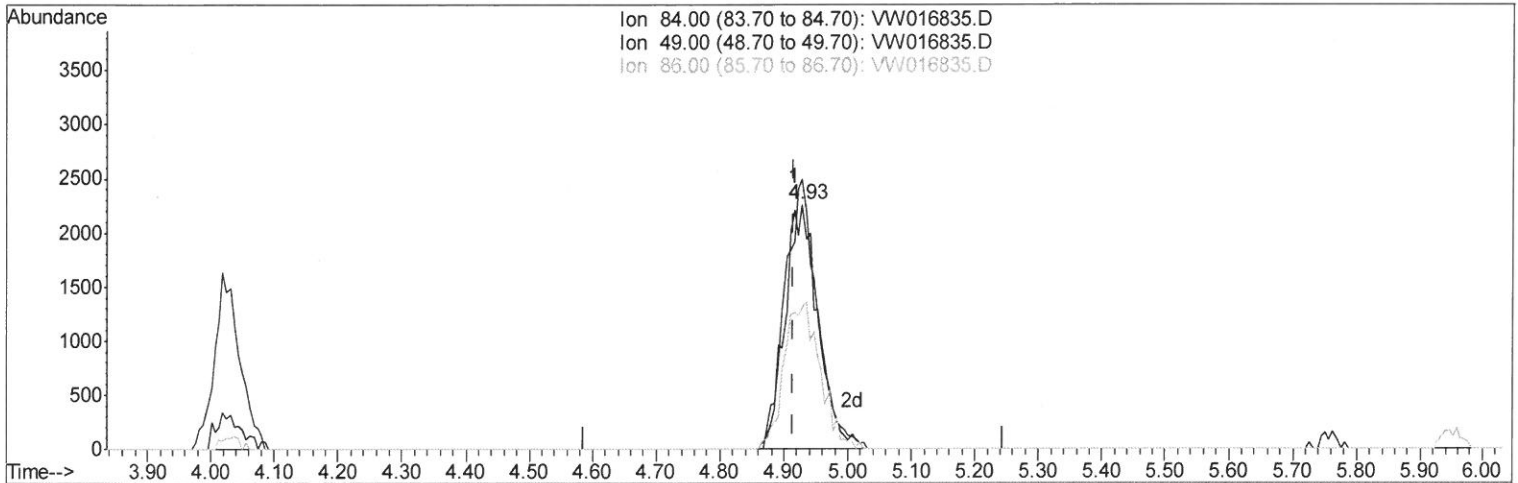

TIC: VW016835.D

(16) Methylene chloride (T)

4.928min (+0.012) 1.15ug/L m

response 8240

Ion	Exp%	Act%
84.00	100	100
49.00	104.50	110.50
86.00	65.70	57.82
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW100820\
 Data File : VW016835.D
 Acq On : 07 Oct 2020 16:01
 Operator : SY/VA
 Sample : VIBLK11
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK11

Manual Integrations
 APPROVED

MMDadoda
 10/12/2020 1:55:27 PM

Quant Time: Oct 08 09:21:21 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100720S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Oct 08 08:32:41 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	518173	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	472168	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	219435	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	121564	23.78	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	95.12%
7) Chloroethane-d5	2.90	69	99366	23.17	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	92.68%
10) 1,1-Dichloroethene-d2	4.03	63	173961	16.03	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	64.12%
20) 2-Butanone-d5	7.09	46	51621	44.58	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	89.16%
24) Chloroform-d	7.65	84	250297	22.89	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	91.56%
26) 1,2-Dichloroethane-d4	8.31	65	128104	24.26	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	97.04%
29) Benzene-d6	8.27	84	502401	23.43	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	93.72%
33) 1,2-Dichloropropane-d6	9.27	67	138433	24.02	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	96.08%
37) Toluene-d8	10.33	98	464073	22.93	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	91.72%
38) trans-1,3-Dichloropropene-	10.58	79	55460	21.82	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	87.28%
39) 2-Hexanone-d5	10.93	63	43552	48.87	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	97.74%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	112695	24.21	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	96.84%
61) 1,2-Dichlorobenzene-d4	13.85	152	170308	24.47	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	97.88%

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
16) Methylene chloride	4.93	84	8240m	1.152	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW100820\
Data File : VW016835.D
Acq On : 07 Oct 2020 16:01
Operator : SY/VA
Sample : VIBLK11
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK11

Manual Integrations
APPROVED

MMDadoda
10/12/2020 1:55:27 PM

Quant Time: Oct 08 09:21:21 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100720S.M
Quant Title : VOC Analysis
QLast Update : Thu Oct 08 08:32:41 2020
Response via : Initial Calibration

