

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW100820\
 Data File : VW016830.D
 Acq On : 07 Oct 2020 12:54
 Operator : SY/VA
 Sample : L4235-19
 Misc : 4.93G/10ML/MSVOA W/SOIL
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AT5

Quant Time: Oct 08 09:06:59 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100720S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Oct 08 08:32:41 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	563969	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	477084	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	189720	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	148094	26.62	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	106.48%
7) Chloroethane-d5	2.89	69	123987	26.57	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	106.28%
10) 1,1-Dichloroethene-d2	4.02	63	216972	18.37	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	73.48%
20) 2-Butanone-d5	7.09	46	54971	43.62	ug/L	0.01
Spiked Amount	50.000	Range	20 - 135	Recovery	=	87.24%
24) Chloroform-d	7.65	84	303180	25.48	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	101.92%
26) 1,2-Dichloroethane-d4	8.31	65	151462	26.35	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	105.40%
29) Benzene-d6	8.28	84	621845	28.70	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	114.80%
33) 1,2-Dichloropropane-d6	9.27	67	167394	28.75	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	115.00%
37) Toluene-d8	10.33	98	565237	27.65	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	110.60%
38) trans-1,3-Dichloropropene-	10.58	79	65080	25.34	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	101.36%
39) 2-Hexanone-d5	10.93	63	45673	50.72	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	101.44%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	121178	25.76	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	103.04%
61) 1,2-Dichlorobenzene-d4	13.85	152	157794	26.22	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	104.88%


Target Compounds					Ovalue
13) Acetone	4.15	43	5045	5.290 ug/L	96
16) Methylene chloride	4.92	84	7640	0.982 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW100820\
Data File : VW016830.D
Acq On : 07 Oct 2020 12:54
Operator : SY/VA
Sample : L4235-19
Misc : 4.93G/10ML/MSVOA W/SOIL
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0AT5

Quant Time: Oct 08 09:06:59 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100720S.M
Quant Title : VOC Analysis
QLast Update : Thu Oct 08 08:32:41 2020
Response via : Initial Calibration

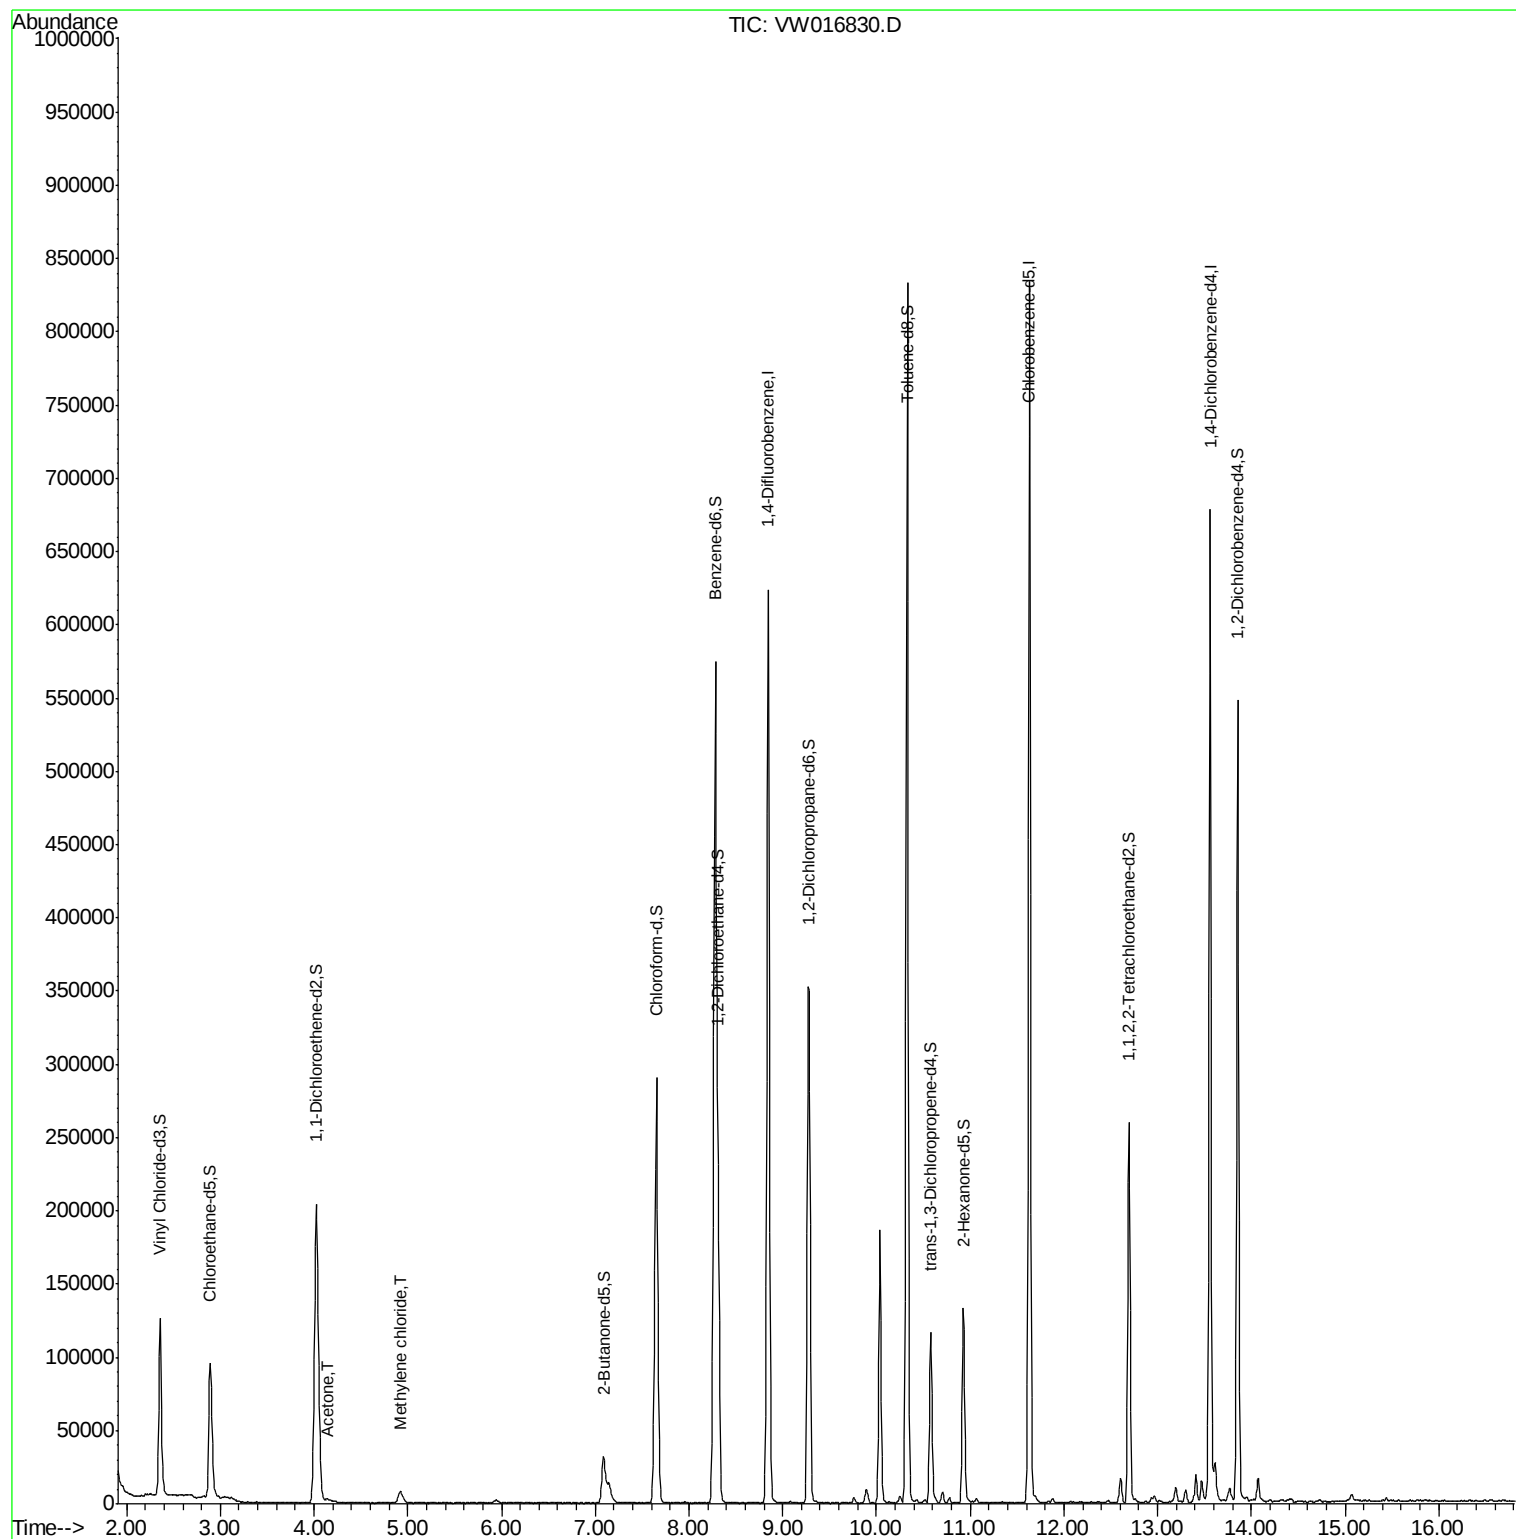

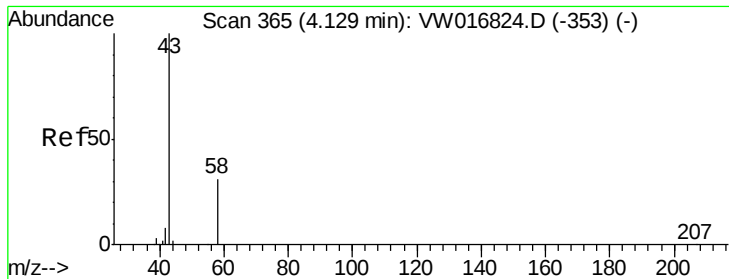

#13

Acetone

Concen: 5.290 ug/L

RT: 4.15 min Scan# 368

Delta R.T. 0.02 min

Lab File: VW016830.D

Acq: 07 Oct 2020 12:54

Instrument :

MSVOA_W

ClientSampleId :





C0AT5

Tot Ion: 43 Resp: 5045

Ion Ratio Lower Upper

43 100

58 31.4 0.0 67.6

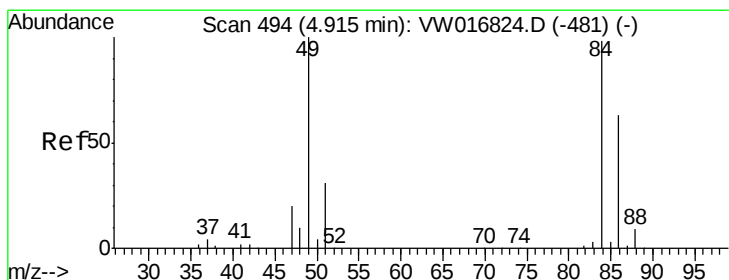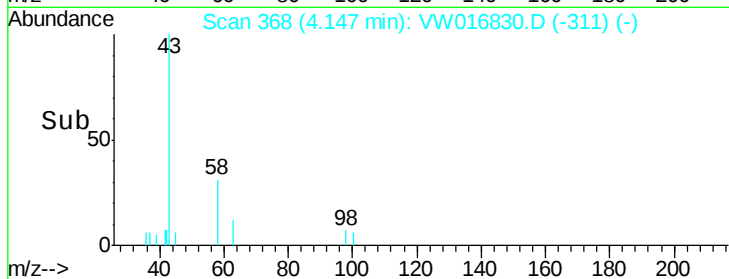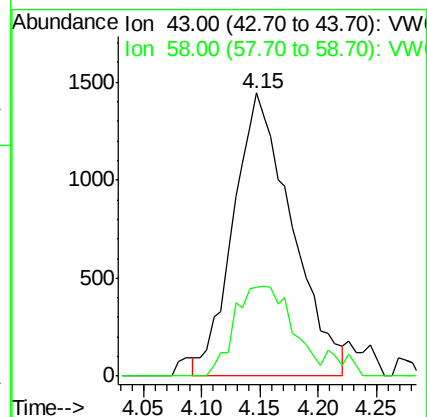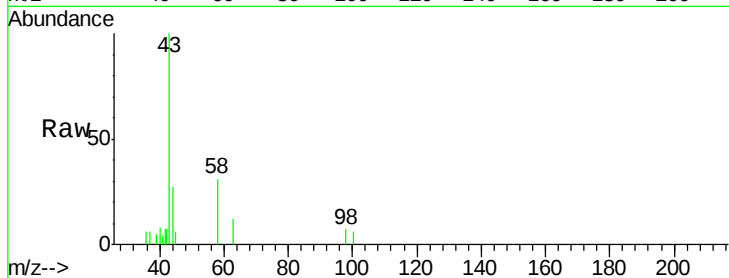

#16

Methylene chloride

Concen: 0.982 ug/L

RT: 4.92 min Scan# 495

Delta R.T. 0.01 min

Lab File: VW016830.D

Acq: 07 Oct 2020 12:54

Tgt Ion: 84 Resp: 7640

Ion Ratio Lower Upper

84 100

49 99.5 73.1 135.8

86 65.9 46.0 85.4

