

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100821\
 Data File : VW020422.D
 Acq On : 08 Oct 2021 20:51
 Operator : SY/VA
 Sample : M4070-15
 Misc : 5.89g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AC8

Quant Time: Oct 09 04:21:10 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100821SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Oct 09 04:18:42 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	133252	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	124982	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	48320	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	47361	24.426	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	97.720%
7) Chloroethane-d5	2.879	69	24664	24.081	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	96.320%
11) 1,1-Dichloroethene-d2	4.013	63	72688	18.295	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	73.200%
21) 2-Butanone-d5	7.086	46	26331	44.622	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	89.240%
24) Chloroform-d	7.653	84	105439	24.823	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	99.280%
26) 1,2-Dichloroethane-d4	8.305	65	61076	25.176	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	100.720%
32) Benzene-d6	8.274	84	194981	23.717	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	94.880%
36) 1,2-Dichloropropane-d6	9.274	67	66542	24.835	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	99.320%
41) Toluene-d8	10.323	98	162821	22.073	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	88.280%
43) trans-1,3-Dichloroprop...	10.579	79	22591	20.748	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	83.000%
47) 2-Hexanone-d5	10.926	63	15860	38.479	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	76.960%
56) 1,1,2,2-Tetrachloroeth...	12.694	84	46034	22.730	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	90.920%
66) 1,2-Dichlorobenzene-d4	13.853	152	45083	23.851	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	95.400%
Target Compounds						Qvalue
16) Methylene chloride	4.915	84	14003	5.406	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100821\
Data File : VW020422.D
Acq On : 08 Oct 2021 20:51
Operator : SY/VA
Sample : M4070-15
Misc : 5.89g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0AC8

Quant Time: Oct 09 04:21:10 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100821SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Oct 09 04:18:42 2021
Response via : Initial Calibration

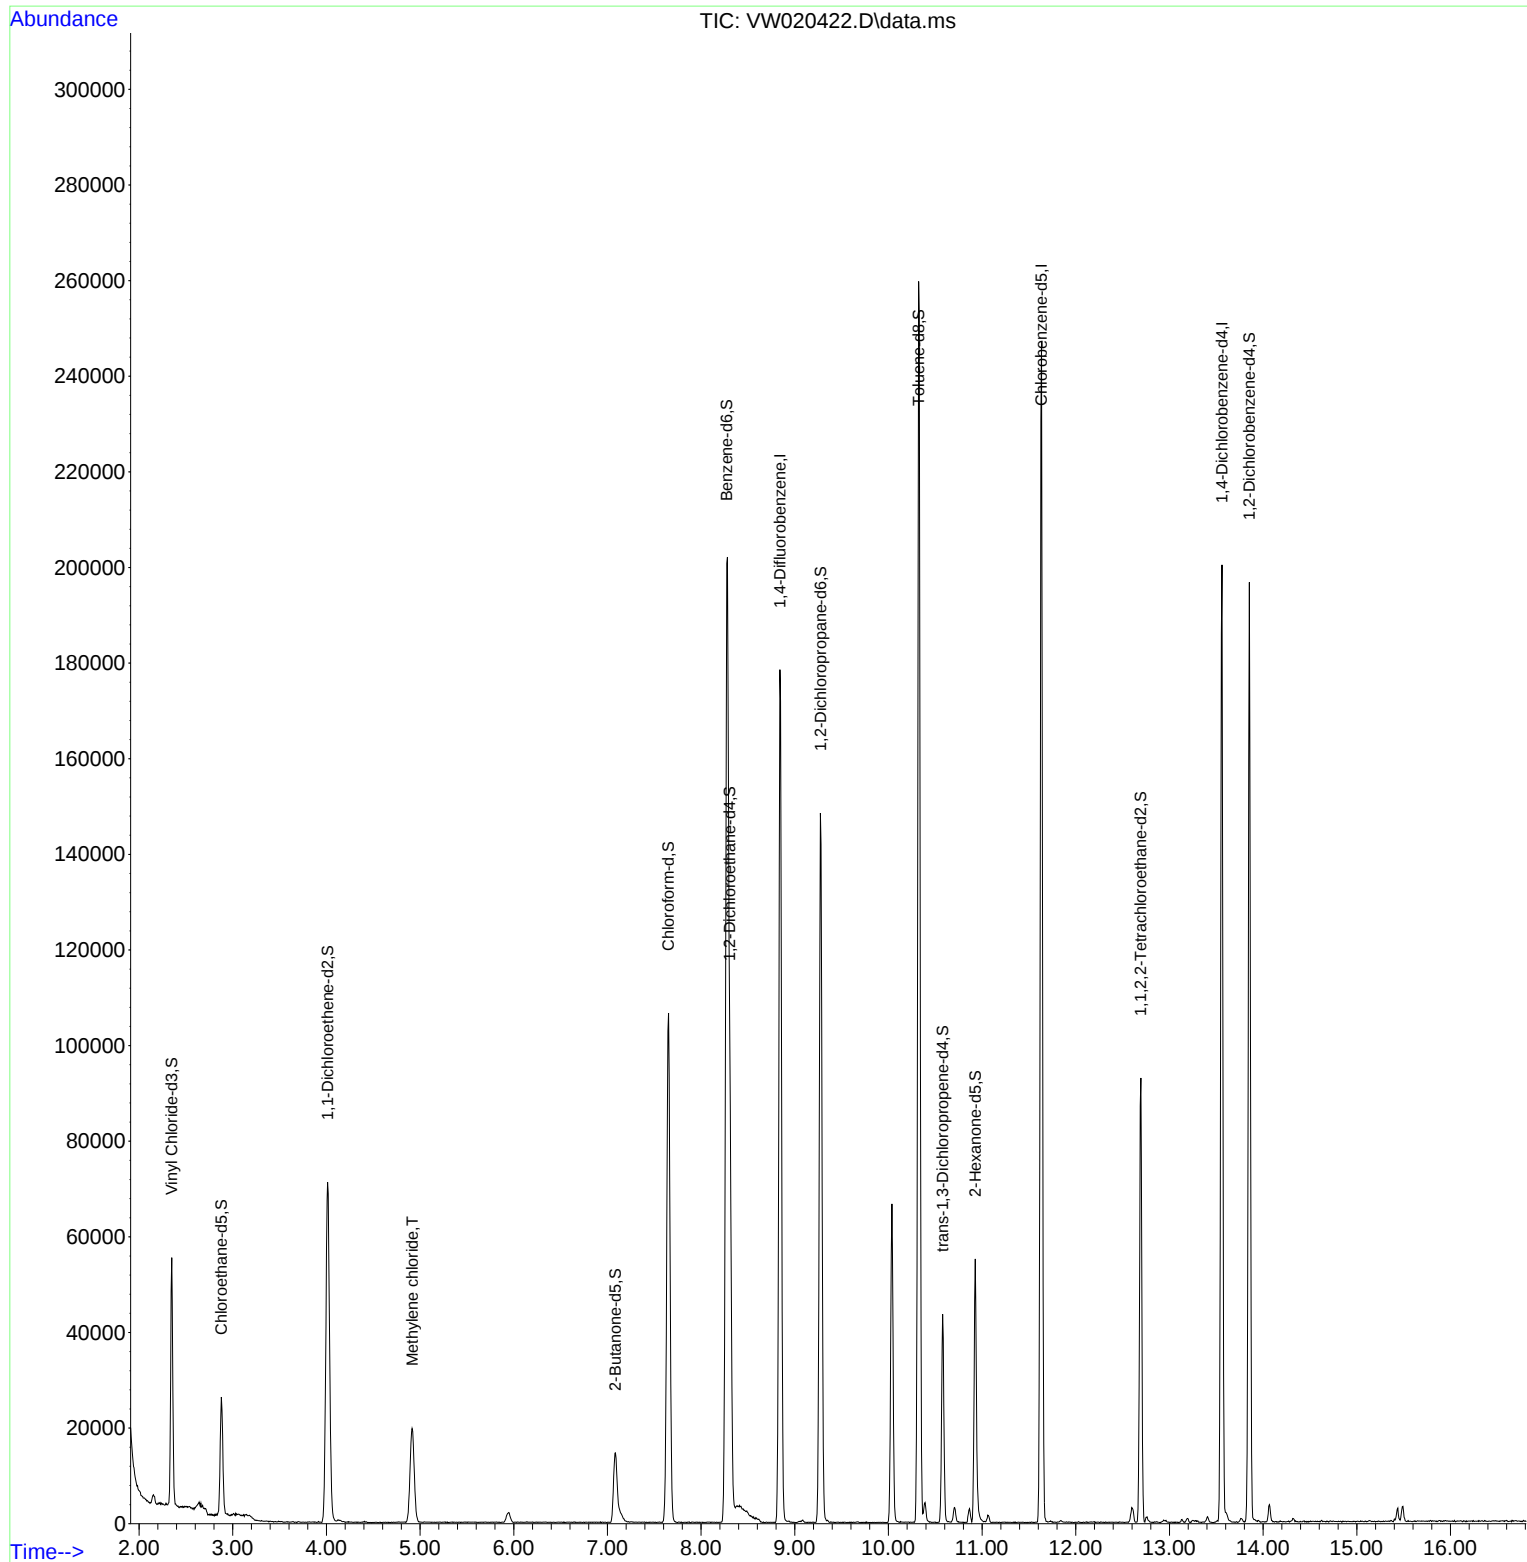

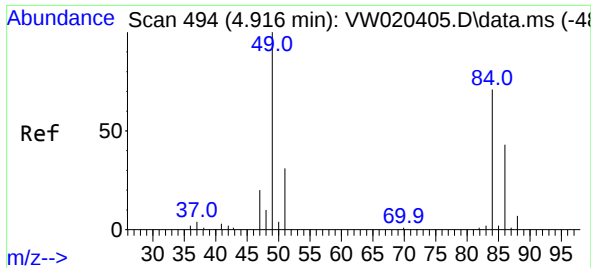

#16
Methylene chloride
Concen: 5.406 ug/L
RT: 4.915 min Scan# 494
Delta R.T. -0.000 min
Lab File: VW020422.D
Acq: 08 Oct 2021 20:51

Instrument :
MSVOA_W
ClientSampleId :
C0AC8

Tgt Ion:	84	Resp:	14003
Ion	Ratio	Lower	Upper
84	100		
86	63.2	44.7	83.1
49	140.7	101.7	188.9

