

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100821\
 Data File : VW020425.D
 Acq On : 08 Oct 2021 22:03
 Operator : SY/VA
 Sample : M4126-04
 Misc : 5.82g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AA4

Quant Time: Oct 09 04:21:30 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100821SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Oct 09 04:18:42 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.848	114	253892	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	226237	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	90103	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	88410	23.931	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	95.720%
7) Chloroethane-d5	2.879	69	47538	24.360	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	97.440%
11) 1,1-Dichloroethene-d2	4.013	63	123220	16.277	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	65.120%
21) 2-Butanone-d5	7.086	46	38772	34.485	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	68.960%
24) Chloroform-d	7.653	84	182460	22.545	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	90.200%
26) 1,2-Dichloroethane-d4	8.311	65	98968	21.411	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	85.640%
32) Benzene-d6	8.275	84	357021	23.991	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	95.960%
36) 1,2-Dichloropropane-d6	9.274	67	114957	23.702	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	94.800%
41) Toluene-d8	10.323	98	314514	23.555	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	94.200%
43) trans-1,3-Dichloroprop...	10.579	79	39270	19.925	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	79.680%
47) 2-Hexanone-d5	10.926	63	25569	34.270	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	68.540%
56) 1,1,2,2-Tetrachloroeth...	12.694	84	69883	19.062	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	76.240%
66) 1,2-Dichlorobenzene-d4	13.853	152	83315	23.638	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	94.560%
Target Compounds						Qvalue
16) Methylene chloride	4.915	84	21708	4.398	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100821\
Data File : VW020425.D
Acq On : 08 Oct 2021 22:03
Operator : SY/VA
Sample : M4126-04
Misc : 5.82g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0AA4

Quant Time: Oct 09 04:21:30 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100821SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Oct 09 04:18:42 2021
Response via : Initial Calibration

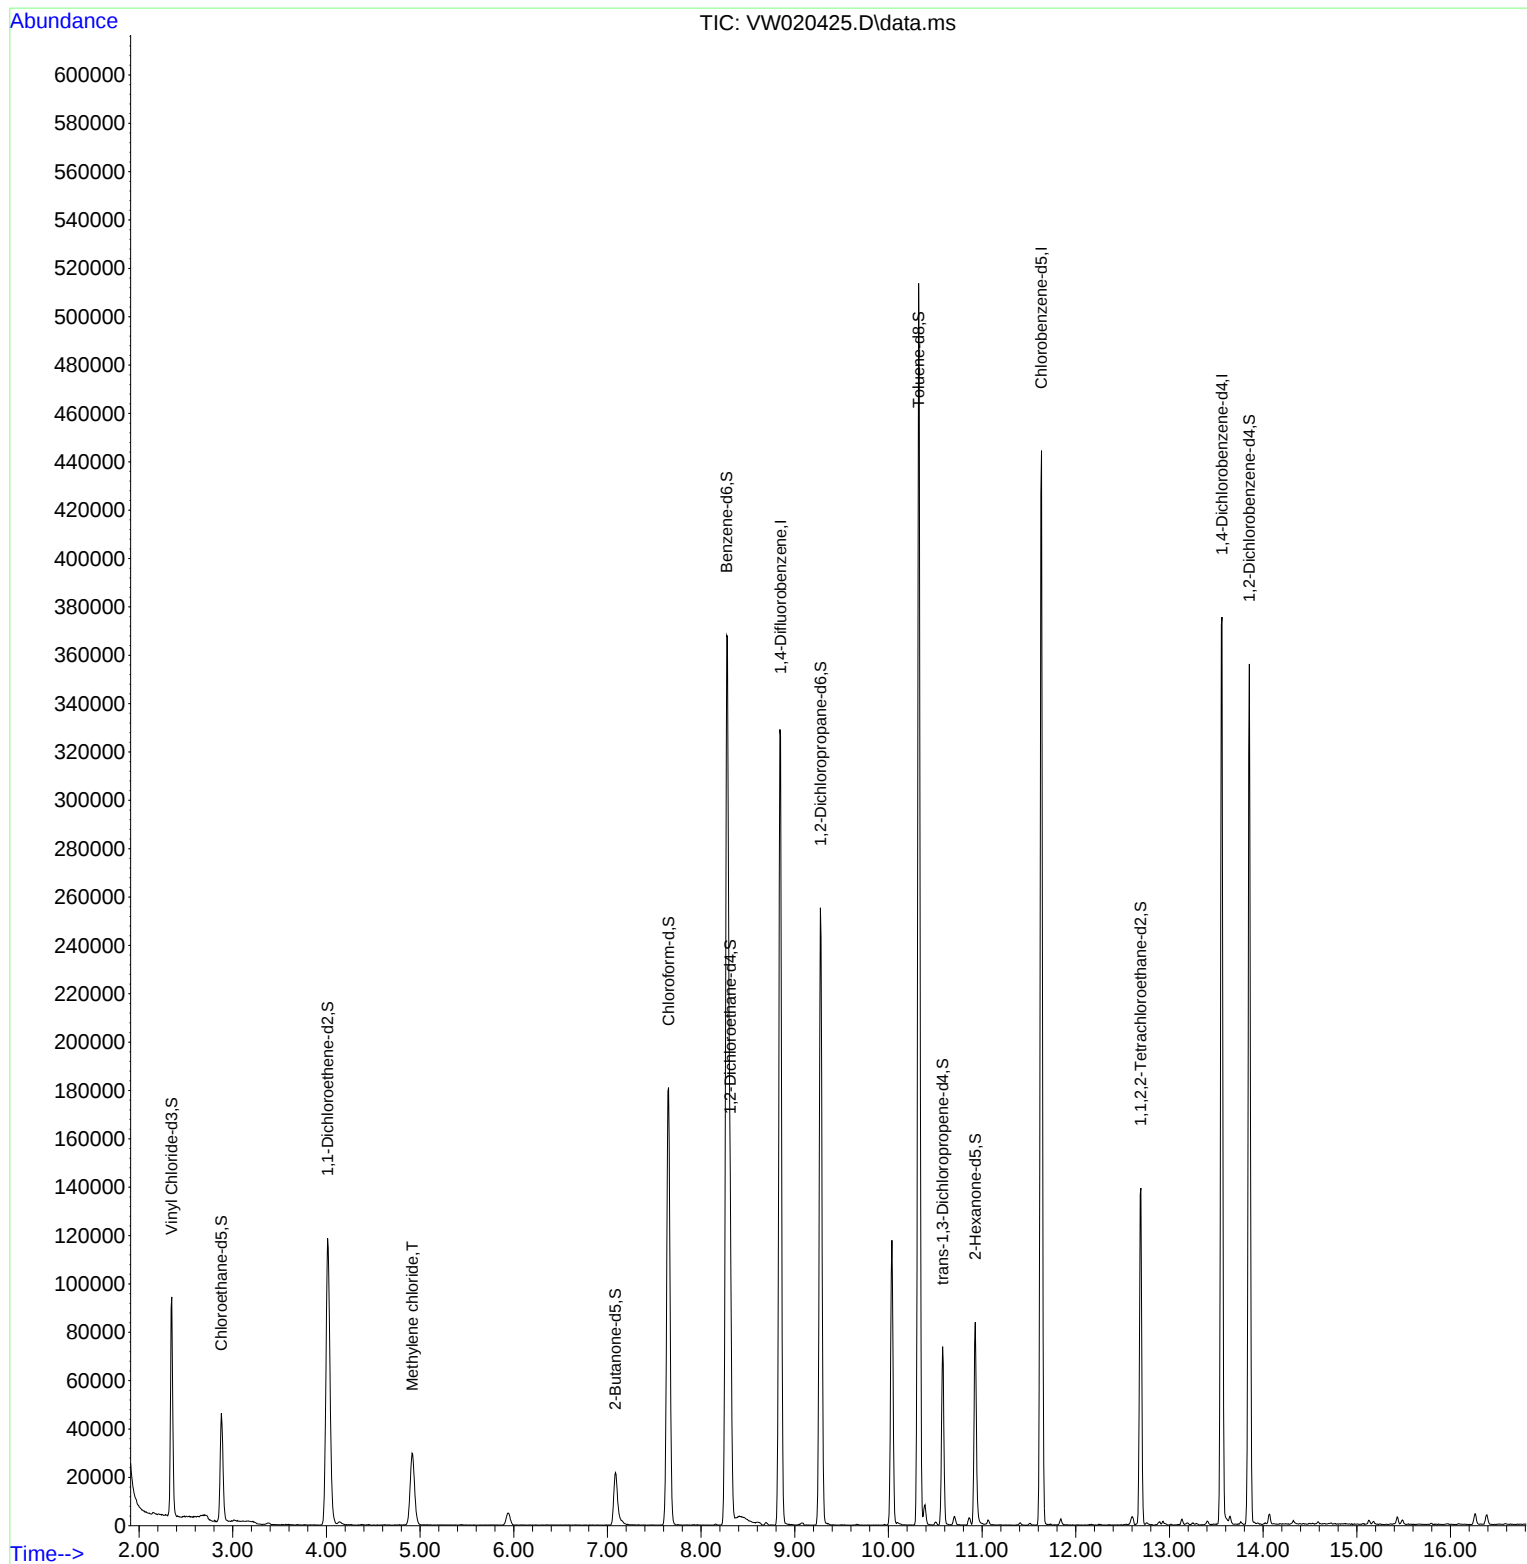

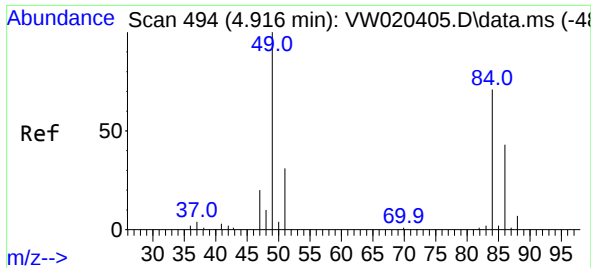

#16
Methylene chloride
Concen: 4.398 ug/L
RT: 4.915 min Scan# 494
Delta R.T. -0.000 min
Lab File: VW020425.D
Acq: 08 Oct 2021 22:03

Instrument :
MSVOA_W
ClientSampleId :
C0AA4

Tgt Ion: 84 Resp: 21708

Ion	Ratio	Lower	Upper
84	100		
86	63.7	44.7	83.1
49	143.8	101.7	188.9

