

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100821\
 Data File : VW020427.D
 Acq On : 08 Oct 2021 22:51
 Operator : SY/VA
 Sample : VIBLK167
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK467

Quant Time: Oct 09 04:21:45 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100821SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Oct 09 04:18:42 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	198821	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	192307	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	84381	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	62369	21.558	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	86.240%		
7) Chloroethane-d5	2.879	69	31649	20.710	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	82.840%		
11) 1,1-Dichloroethene-d2	4.013	63	88664	14.957	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	59.840%		
21) 2-Butanone-d5	7.086	46	40493	45.991	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	91.980%		
24) Chloroform-d	7.653	84	139853	22.067	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	88.280%		
26) 1,2-Dichloroethane-d4	8.305	65	83993	23.205	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	92.800%		
32) Benzene-d6	8.275	84	271051	21.428	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	85.720%		
36) 1,2-Dichloropropane-d6	9.274	67	90227	21.886	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	87.560%		
41) Toluene-d8	10.323	98	244393	21.533	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	86.120%		
43) trans-1,3-Dichloroprop...	10.579	79	35422	21.143	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	84.560%		
47) 2-Hexanone-d5	10.927	63	27670	43.629	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	87.260%		
56) 1,1,2,2-Tetrachloroeth...	12.695	84	69435	22.281	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	89.120%		
66) 1,2-Dichlorobenzene-d4	13.853	152	81199	24.600	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	98.400%		
Target Compounds						Qvalue
16) Methylene chloride	4.915	84	22091	5.716	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100821\
Data File : VW020427.D
Acq On : 08 Oct 2021 22:51
Operator : SY/VA
Sample : VIBLK167
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK467

Quant Time: Oct 09 04:21:45 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100821SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Oct 09 04:18:42 2021
Response via : Initial Calibration

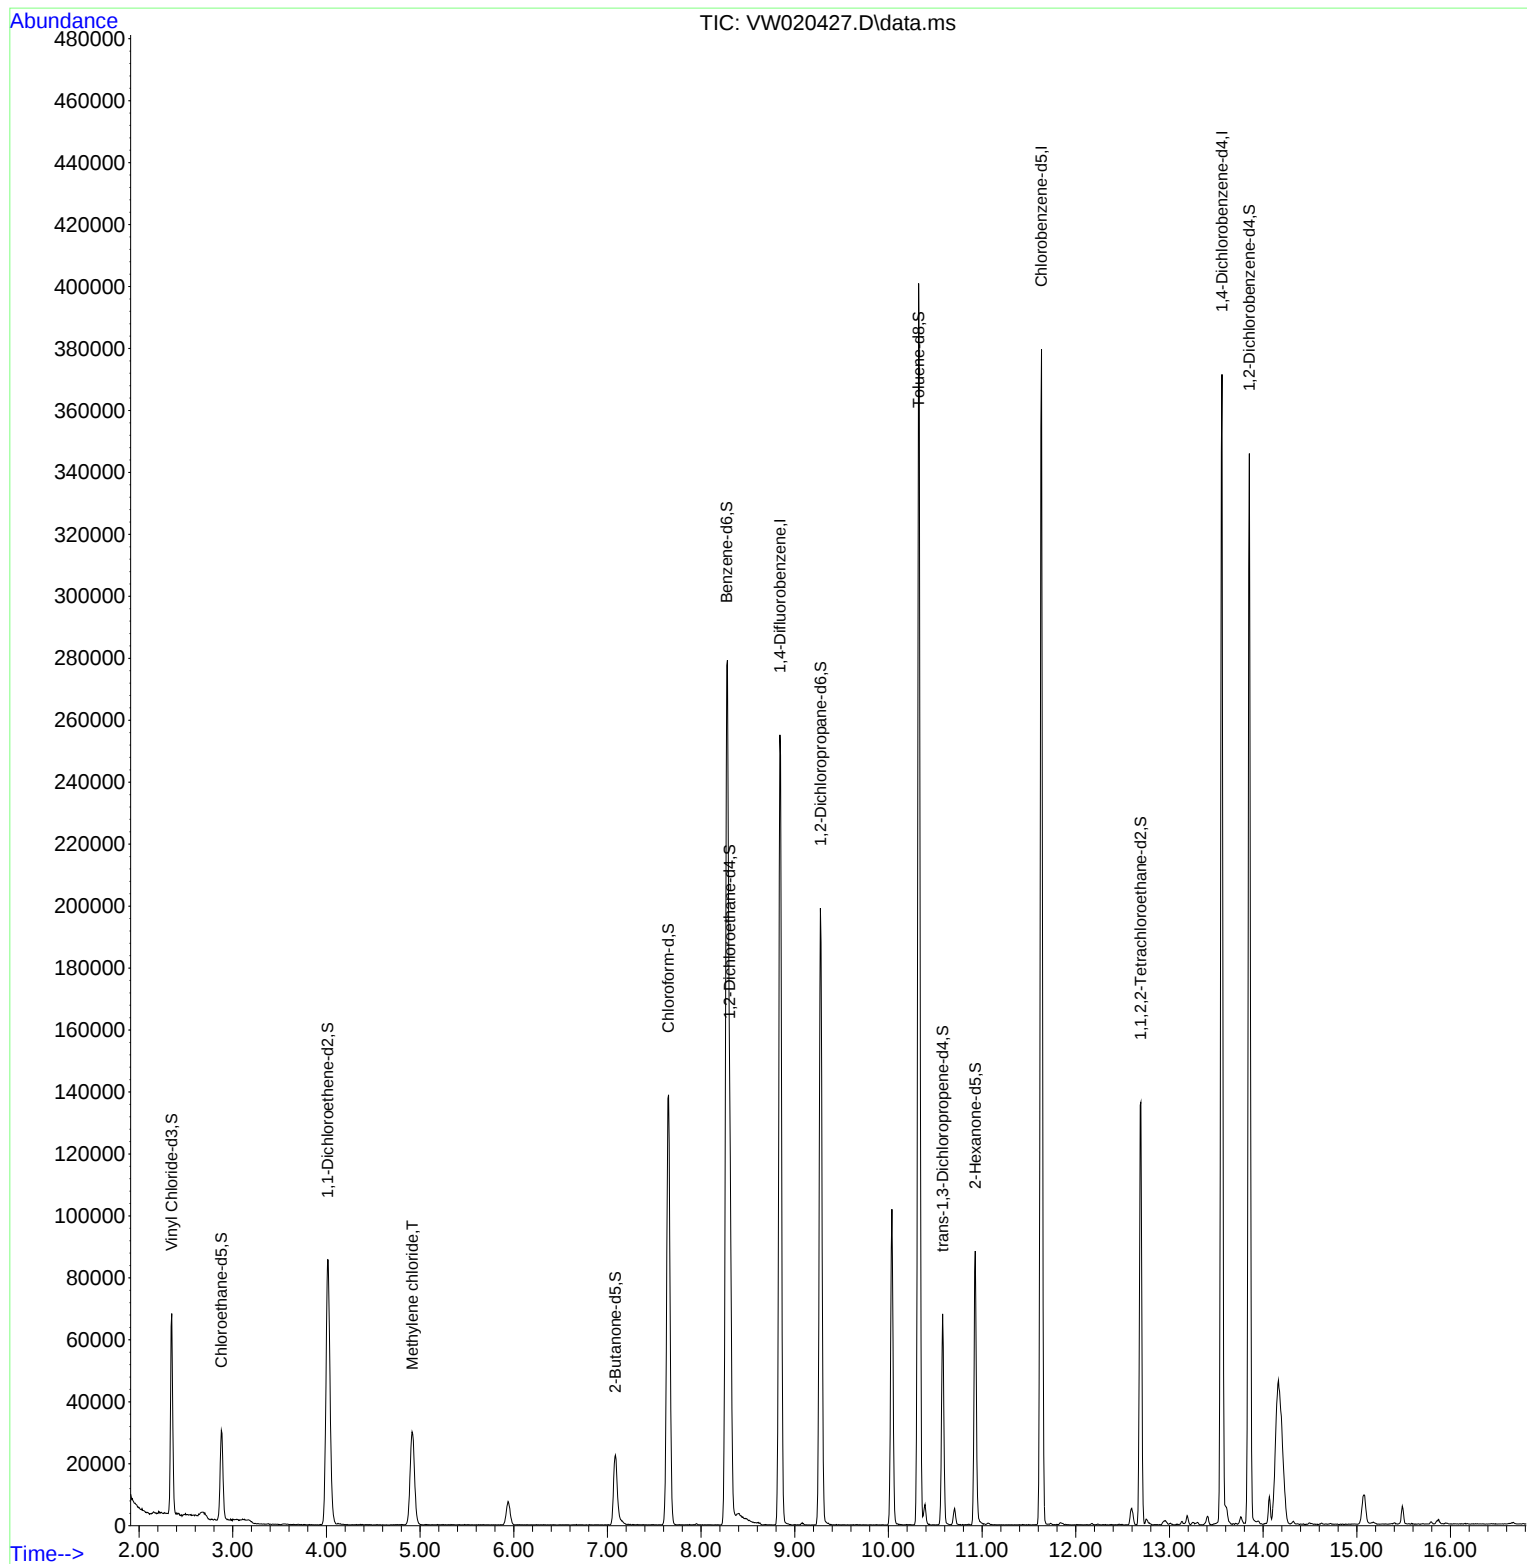

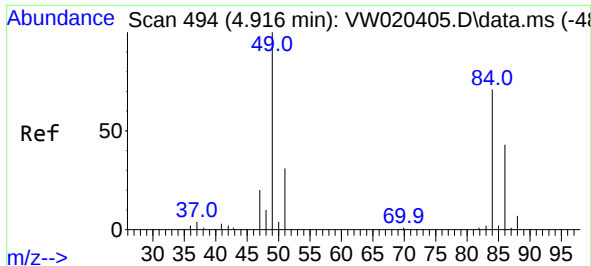

#16
Methylene chloride
Concen: 5.716 ug/L
RT: 4.915 min Scan# 494
Delta R.T. -0.000 min
Lab File: VW020427.D
Acq: 08 Oct 2021 22:51

Instrument :
MSVOA_W
ClientSampleId :
VIBLK467

Tgt Ion: 84 Resp: 22091

Ion	Ratio	Lower	Upper
84	100		
86	64.7	44.7	83.1
49	142.8	101.7	188.9

