
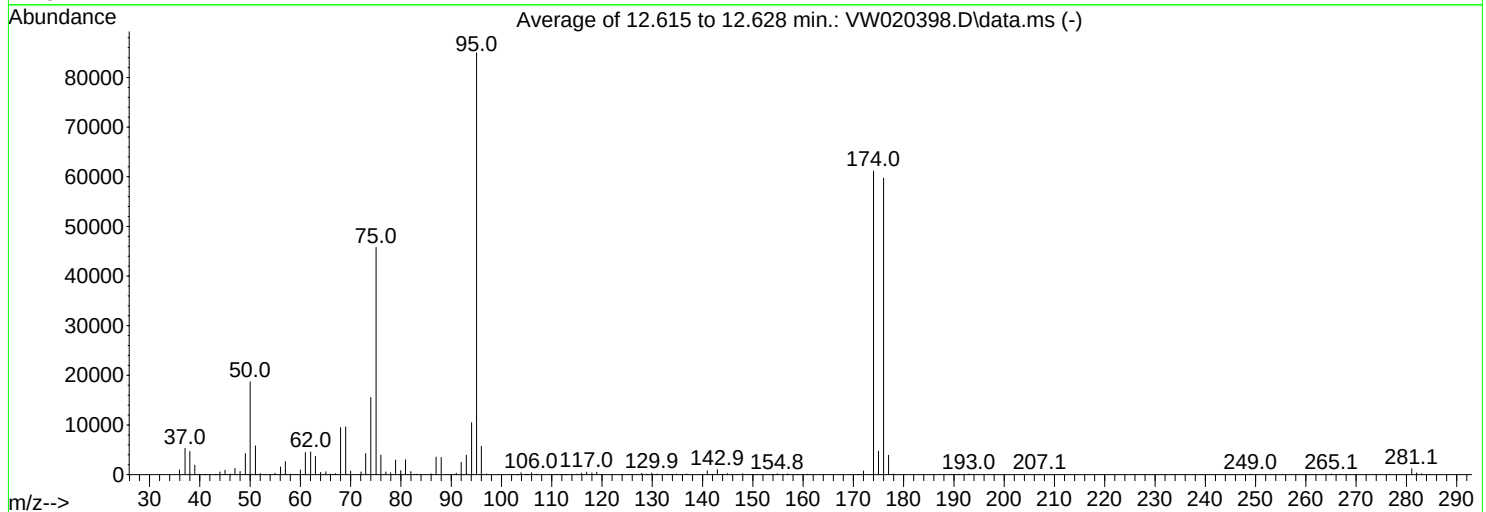


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100821\
 Data File : VW020398.D
 Acq On : 08 Oct 2021 09:24
 Operator : SY/VA
 Sample : BFB448
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB448

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100821SMA.M
 Title : SFAM01.0
 Last Update : Sat Oct 09 04:18:42 2021

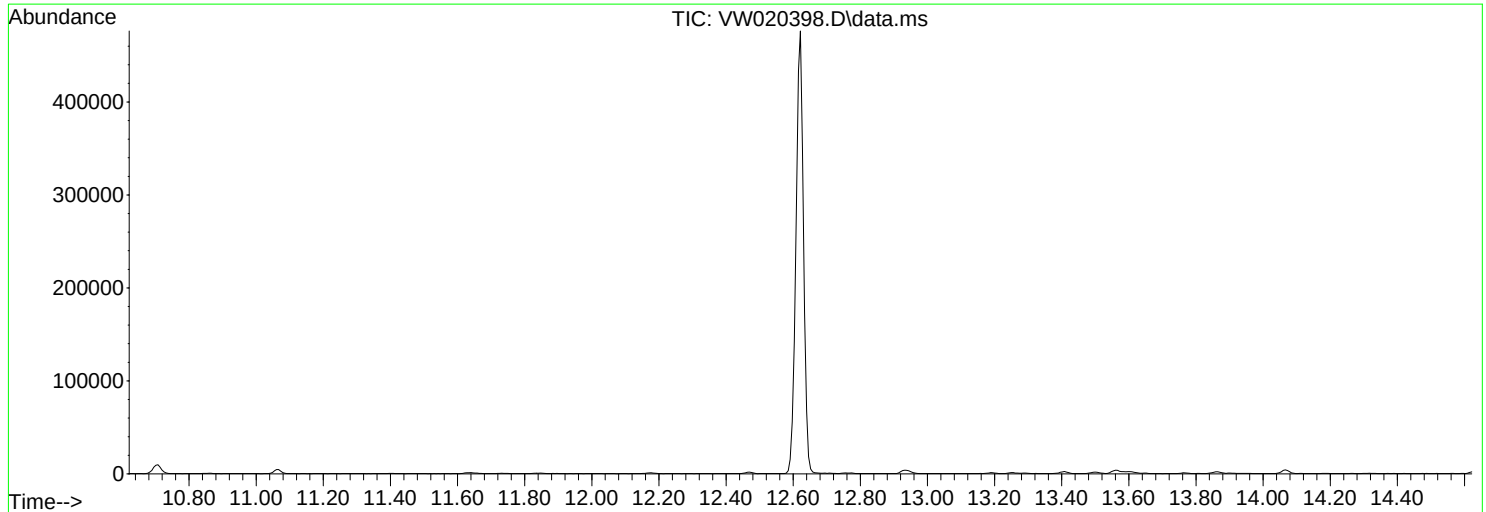

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.0	18694	PASS
75	95	30	80	53.9	45752	PASS
95	95	100	100	100.0	84957	PASS
96	95	5	9	6.7	5700	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	72.0	61147	PASS
175	174	5	9	7.7	4723	PASS
176	174	95	105	97.7	59725	PASS
177	176	5	10	6.5	3898	PASS

m/z	Abundance
35.90	1016.0
37.00	6019.0
38.00	5279.0
39.00	2117.0
39.90	226.0
40.90	52.0
44.00	754.0
45.00	983.0
46.00	122.0
47.00	1328.0
48.00	798.0
49.00	4635.0
50.00	20872.0
51.00	6463.0
52.10	321.0
53.00	92.0
55.00	342.0
56.10	1708.0
57.00	2998.0
58.00	166.0
60.00	1127.0
61.00	4932.0
62.00	5084.0
63.00	4089.0
64.00	530.0
65.00	603.0
66.00	98.0
67.00	242.0
68.00	10551.0
69.00	11105.0
70.00	720.0
72.10	609.0
73.00	4764.0
74.00	17576.0
75.00	51072.0
76.00	4430.0
77.00	642.0
78.00	470.0
78.90	3273.0
79.90	896.0
80.90	3401.0
81.90	650.0
83.10	85.0
86.00	183.0
87.00	3972.0
88.00	3899.0
90.90	336.0
92.00	2910.0
93.00	4506.0
94.00	11728.0
95.00	96928.0
96.00	6634.0
97.00	225.0
103.20	53.0
103.90	421.0
104.90	130.0
106.00	403.0
107.00	93.0
109.90	66.0
110.90	104.0
111.80	81.0
113.00	87.0
114.90	132.0
115.90	394.0
116.90	570.0
118.00	443.0
119.00	479.0
123.90	56.0
127.90	259.0
128.90	154.0
129.90	365.0
130.90	160.0
132.90	120.0
134.90	130.0
136.80	132.0
140.00	100.0
141.00	809.0
142.10	117.0
142.90	1142.0
143.80	84.0
144.90	243.0
145.90	106.0
147.10	64.0
147.90	173.0
149.00	81.0
149.90	108.0
153.90	58.0
154.80	192.0
156.90	185.0
159.00	131.0
160.90	101.0
170.90	110.0

Instrument :
MSVOA_W
ClientSampleId :
BFB448

172.00	822.0
174.00	72784.0
175.00	5324.0
176.00	67592.0
177.00	4370.0
178.00	156.0
190.80	83.0
193.00	119.0
207.10	112.0
249.00	111.0
265.10	151.0
281.10	949.0
282.10	372.0
283.00	171.0

Instrument :
MSVOA_W
ClientSampleId :
BFB448

m/z	Abundance
36.00	632.0
37.00	4082.0
38.00	3646.0
39.00	1360.0
40.00	175.0
44.00	623.0
45.00	704.0
46.00	125.0
47.00	1025.0
48.10	398.0
49.00	3322.0
50.00	14218.0
51.00	4475.0
52.10	168.0
54.90	215.0
56.00	1171.0
57.00	2087.0
58.00	70.0
60.00	709.0
61.00	3731.0
62.10	3643.0
63.00	2844.0
64.00	272.0
65.00	420.0
66.00	58.0
67.00	206.0
68.00	7434.0
69.00	7433.0
70.00	605.0
72.00	487.0
73.00	3169.0
74.00	12360.0
75.10	36200.0
76.00	2883.0
77.00	418.0
77.90	284.0
79.00	2248.0
80.00	638.0
80.90	2384.0
82.00	515.0
83.00	83.0
85.90	93.0
87.00	2988.0
88.00	2814.0
91.10	262.0
92.00	1988.0
93.00	3021.0
94.10	8507.0
95.00	69616.0
96.00	4404.0
97.10	129.0
103.90	317.0
104.80	101.0
105.20	81.0
105.90	331.0
107.00	106.0
112.00	78.0
112.70	55.0
114.80	51.0
115.90	298.0
116.90	445.0
118.00	290.0
118.90	391.0
127.90	254.0
128.90	101.0
129.90	248.0
131.00	129.0
133.10	56.0
134.90	120.0
136.90	125.0
140.90	717.0
142.00	98.0
143.00	853.0
143.90	53.0
145.00	138.0
145.80	80.0
146.90	91.0
147.90	148.0
149.90	63.0
154.90	171.0
156.90	141.0
158.80	72.0
161.00	63.0
171.10	85.0
172.00	563.0
174.00	57904.0
175.00	3944.0
176.00	53712.0
177.00	3236.0
178.00	89.0
191.00	51.0
193.10	50.0

Instrument :
MSVOA_W
ClientSampleId :
BFB448

249.00	58.0
281.10	556.0
281.90	178.0
283.00	109.0

Instrument :
MSVOA_W
ClientSampleId :
BFB448

Scan 1749 (12.567 min): VW020398.D\data.ms
BFB448

m/z	Abundance
39.90	130.0
44.10	173.0

Instrument :
MSVOA_W
ClientSampleId :
BFB448

m/z	Abundance
36.00	1123.0
37.10	5734.0
38.00	5077.0
39.00	2223.0
40.00	244.0
43.10	56.0
44.00	844.0
45.00	985.0
46.20	176.0
47.00	1379.0
48.00	790.0
49.10	4845.0
50.00	20992.0
51.10	6456.0
52.00	221.0
53.00	85.0
54.90	306.0
56.00	1726.0
57.00	2812.0
58.10	160.0
58.90	77.0
60.00	1003.0
61.00	4806.0
62.00	4997.0
63.00	4109.0
64.00	586.0
65.10	682.0
66.00	114.0
67.00	277.0
68.00	10441.0
69.00	10385.0
70.00	797.0
72.00	580.0
73.00	4815.0
74.00	16696.0
75.00	49984.0
76.00	4467.0
77.00	571.0
77.90	362.0
78.90	3388.0
80.00	863.0
80.90	3209.0
81.90	684.0
83.00	92.0
86.00	187.0
87.00	3727.0
88.00	3673.0
91.00	320.0
92.00	2584.0
93.00	4323.0
94.00	11229.0
95.10	88328.0
96.00	6062.0
97.10	145.0
103.00	69.0
103.90	420.0
105.00	170.0
105.90	381.0
107.00	85.0
109.90	72.0
110.90	113.0
111.80	88.0
112.90	98.0
115.00	94.0
115.90	300.0
117.00	586.0
118.00	333.0
118.90	587.0
125.10	76.0
127.90	291.0
128.90	149.0
129.90	339.0
130.90	109.0
133.00	166.0
133.90	55.0
134.80	128.0
136.90	145.0
140.00	57.0
140.90	792.0
142.00	95.0
143.00	1004.0
143.90	67.0
145.00	276.0
145.90	126.0
147.10	77.0
148.00	234.0
149.00	76.0
149.90	75.0
154.90	264.0
156.90	198.0
158.80	125.0
160.90	93.0

Instrument :
MSVOA_W
ClientSampleId :
BFB448

172.00	881.0
174.00	52752.0
175.00	4900.0
176.00	57872.0
177.00	4088.0
177.90	117.0
191.10	123.0
193.00	181.0
207.10	117.0
249.00	153.0
265.10	203.0
266.80	66.0
281.00	2058.0
282.10	477.0
283.00	208.0

Instrument :
MSVOA_W
ClientSampleId :
BFB448