

Quantitation Report (QT/LSC Reviewed)


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW100920\
 Data File : VW016852.D
 Acq On : 08 Oct 2020 14:14
 Operator : SY/VA
 Sample : L4284-04
 Misc : 5.03G/10ML/MSVOA W/SOIL
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BG3W1

Manual Integrations
 APPROVED

MMDadoda
 10/12/2020 1:56:51 PM

Quant Time: Oct 09 09:21:33 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100720S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Oct 08 11:39:44 2020
 Response via : Initial Calibration

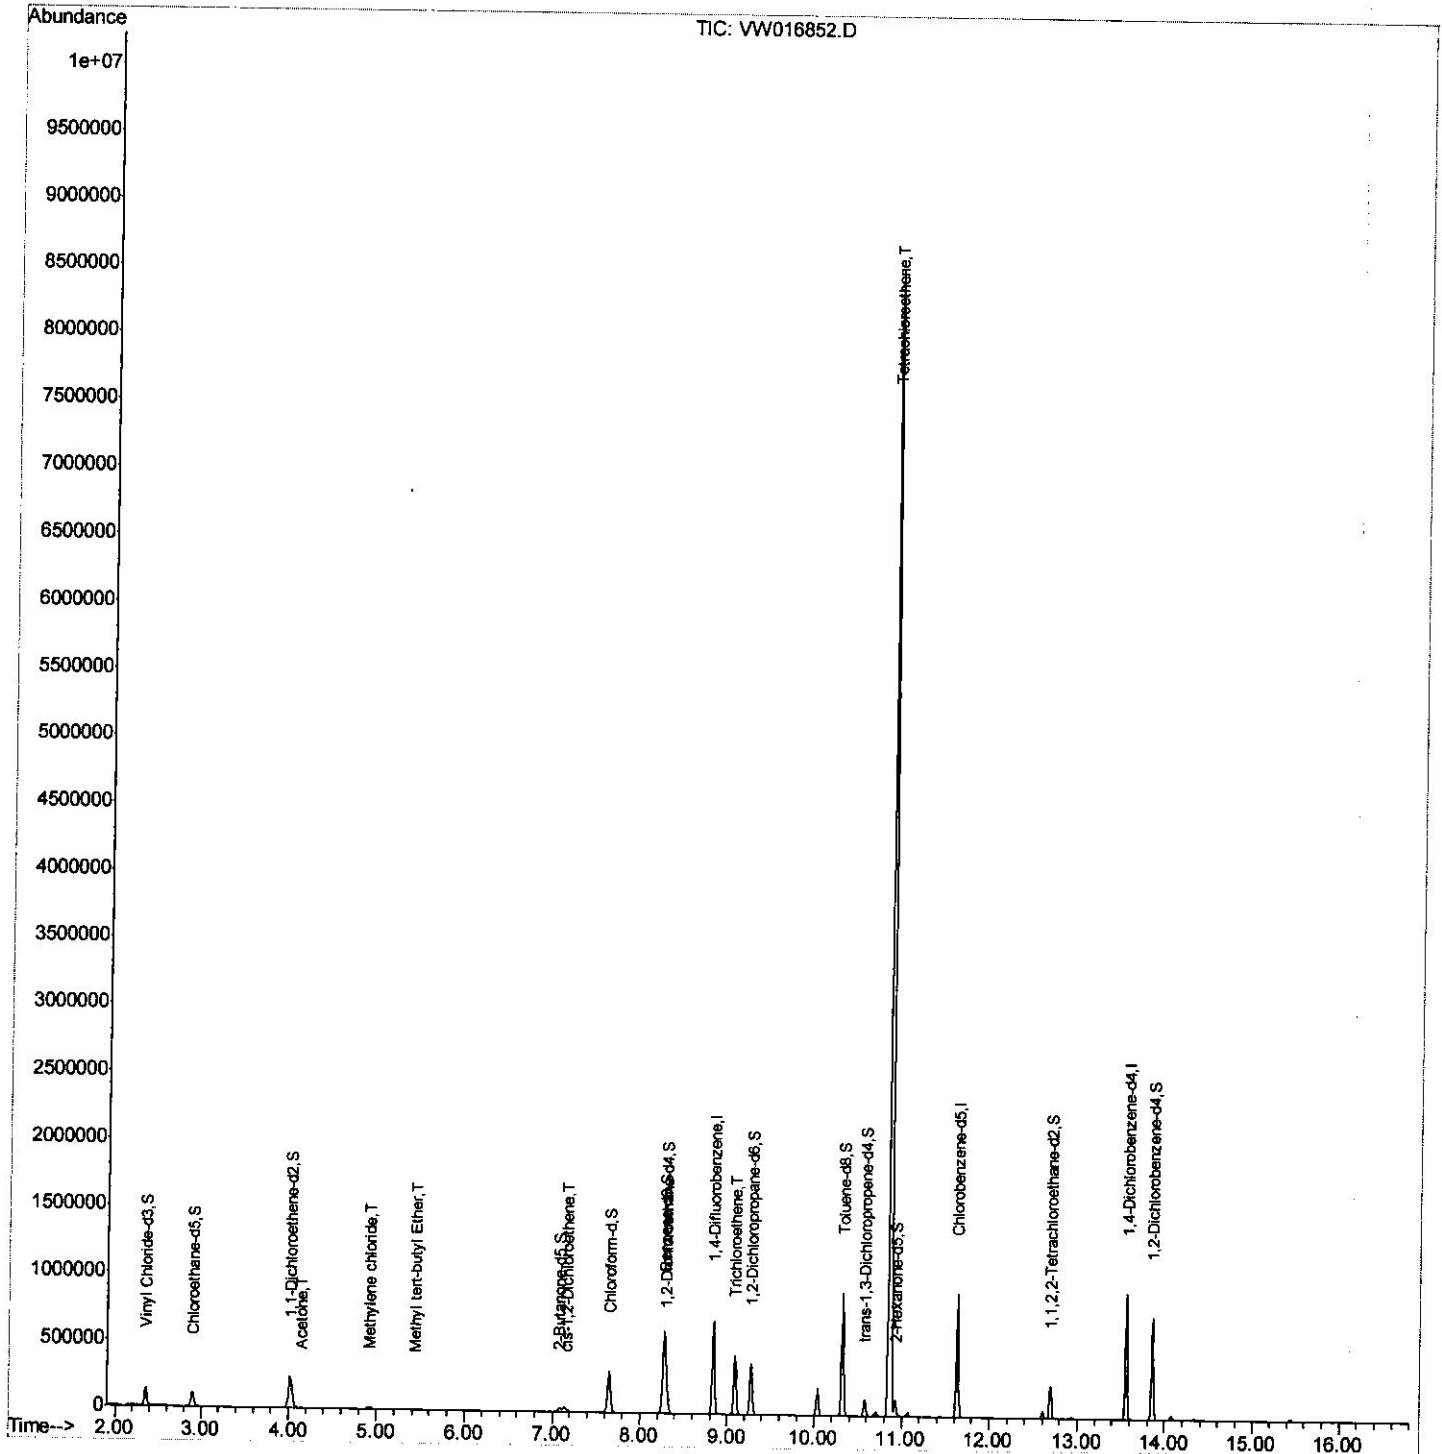

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW100920\
 Data File : VW016852.D
 Acq On : 08 Oct 2020 14:14
 Operator : SY/VA
 Sample : L4284-04
 Misc : 5.03G/10ML/MSVOA W/SOIL
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BG3W1

Manual Integrations
 APPROVED

MMDadoda
 10/12/2020 1:56:51 PM

Quant Time: Oct 09 08:09:55 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100720S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Oct 08 11:39:44 2020
 Response via : Initial Calibration

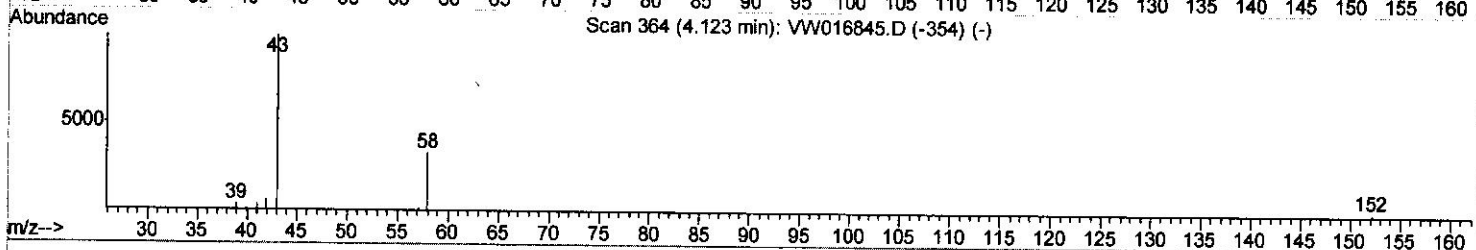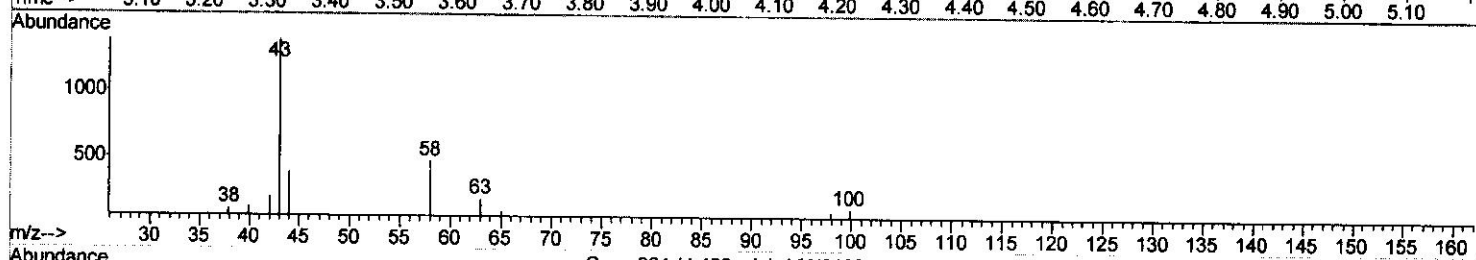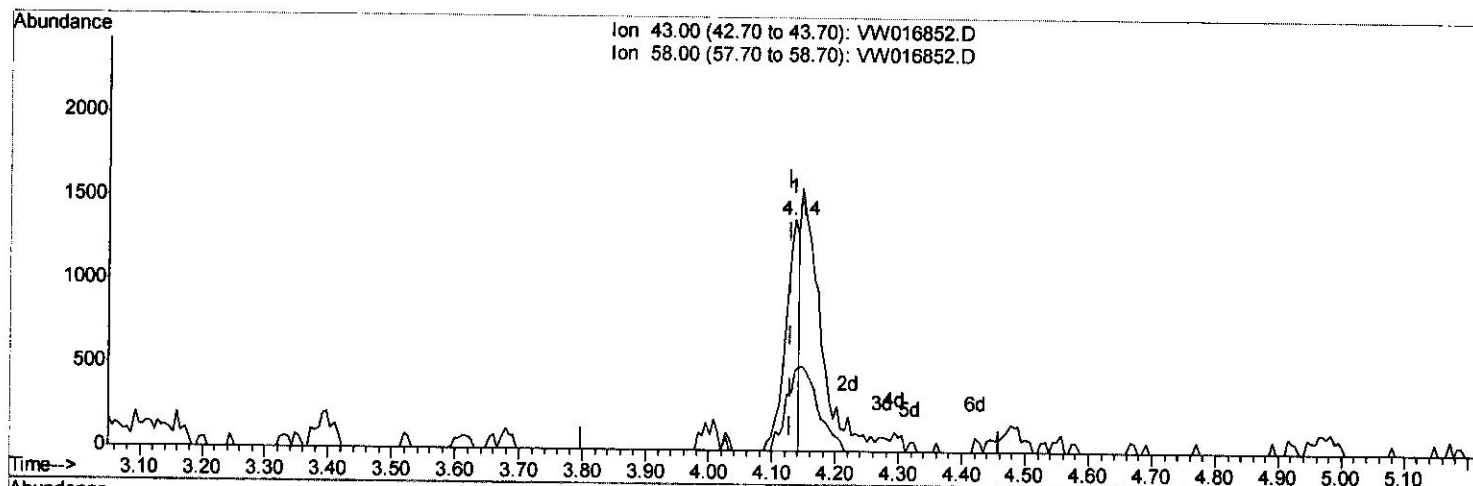

TIC: VW016852.D

(13) Acetone (T)

4.135min (+0.006) 2.05ug/L

response 2145

Ion	Exp%	Act%
43.00	100	100
58.00	33.80	78.37#
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW100920\
 Data File : VW016852.D
 Acq On : 08 Oct 2020 14:14
 Operator : SY/VA
 Sample : L4284-04
 Misc : 5.03G/10ML/MSVOA W/SOIL
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BG3W1

Manual Integrations
 APPROVED

MMDadoda
 10/12/2020 1:56:51 PM

Quant Time: Oct 09 08:09:55 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100720S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Oct 08 11:39:44 2020
 Response via : Initial Calibration

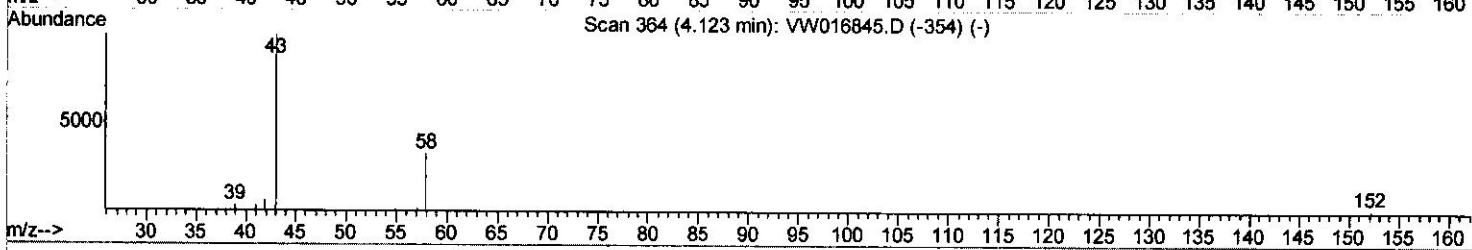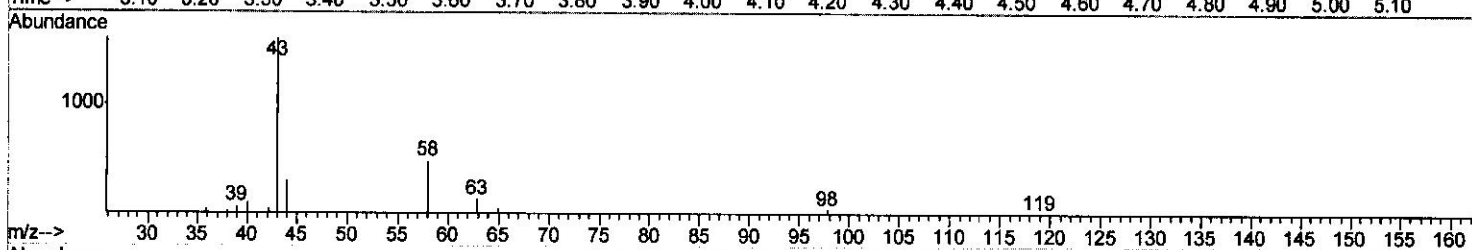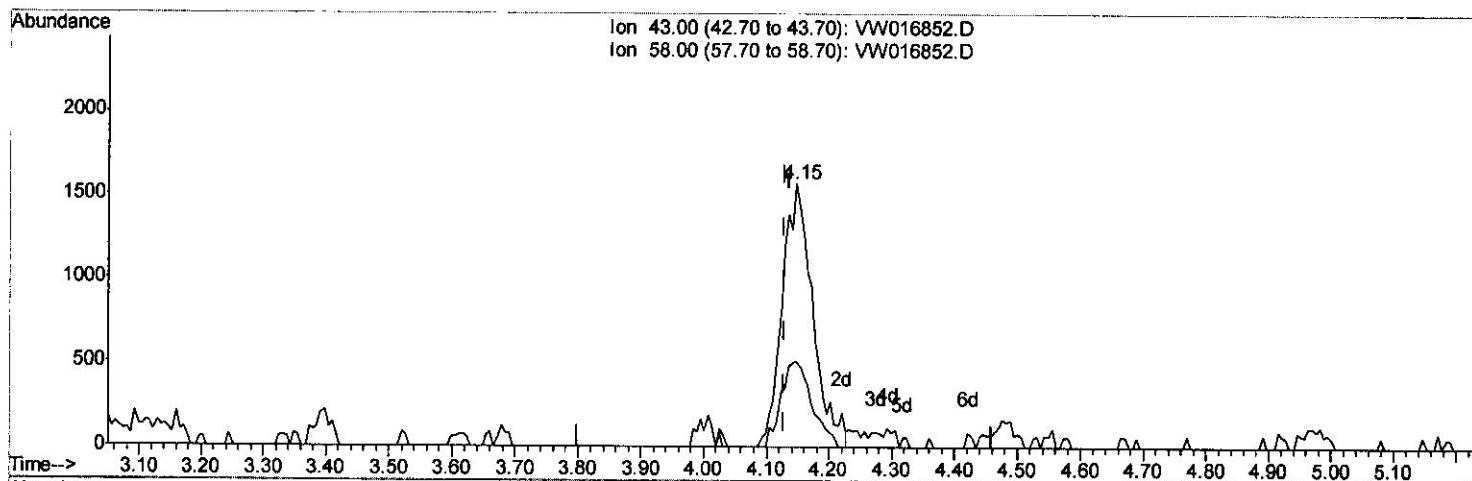

TIC: VW016852.D

(13) Acetone (T)

4.147min (+0.018) 5.07ug/L m

response 5309

Ion	Exp%	Act%
43.00	100	100
58.00	33.80	31.66
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (QT/LSC Reviewed)

Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW100920\
 Data File : VW016852.D
 Acq On : 08 Oct 2020 14:14
 Operator : SY/VA
 Sample : L4284-04
 Misc : 5.03G/10ML/MSVOA W/SOIL
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_W
 Client Sampled :
 BG3W1

Manual Integrations
 APPROVED

MMDadoda
 10/12/2020 1:56:51 PM

Quant Time: Oct 09 09:21:33 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100720S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Oct 08 11:39:44 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	619084	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	549970	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	259953	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	167163	27.37	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	109.48%
7) Chloroethane-d5	2.90	69	137538	26.85	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	107.40%
10) 1,1-Dichloroethene-d2	4.02	63	243862	18.80	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	75.20%
20) 2-Butanone-d5	7.09	46	52117	37.68	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	75.36%
24) Chloroform-d	7.65	84	328442	25.14	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	100.56%
26) 1,2-Dichloroethane-d4	8.31	65	154262	24.45	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	97.80%
29) Benzene-d6	8.27	84	679449	27.20	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	108.80%
33) 1,2-Dichloropropane-d6	9.27	67	179396	26.72	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	106.88%
37) Toluene-d8	10.32	98	640156	27.16	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	108.64%
38) trans-1,3-Dichloropropene-	10.58	79	70144	23.69	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	94.76%
39) 2-Hexanone-d5	10.93	63	43499	41.90	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	83.80%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	116794	21.54	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	86.16%
61) 1,2-Dichlorobenzene-d4	13.85	152	213175	25.85	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	103.40%

Target Compounds

13) Acetone	4.15	43	5309m	5.071	ug/L	
16) Methylene chloride	4.92	84	13817	1.617	ug/L	94
17) Methyl tert-butyl Ether	5.43	73	2489	0.278	ug/L	# 82
22) cis-1,2-Dichloroethene	7.17	96	1986	0.233	ug/L	# 70
35) Trichloroethene	9.09	95	153281	18.348	ug/L	98
47) Tetrachloroethene	10.87	164	2059093	265.857	ug/L	100

M.D
 10/12/20

(#) = qualifier out of range (m) = manual integration (+) = signals summed