


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW100920\
 Data File : VW016844.D
 Acq On : 08 Oct 2020 08:34
 Operator : SY/VA
 Sample : BFB11
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB11

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100720S.M
 Title : VOC Analysis
 Last Update : Fri Oct 09 10:40:32 2020

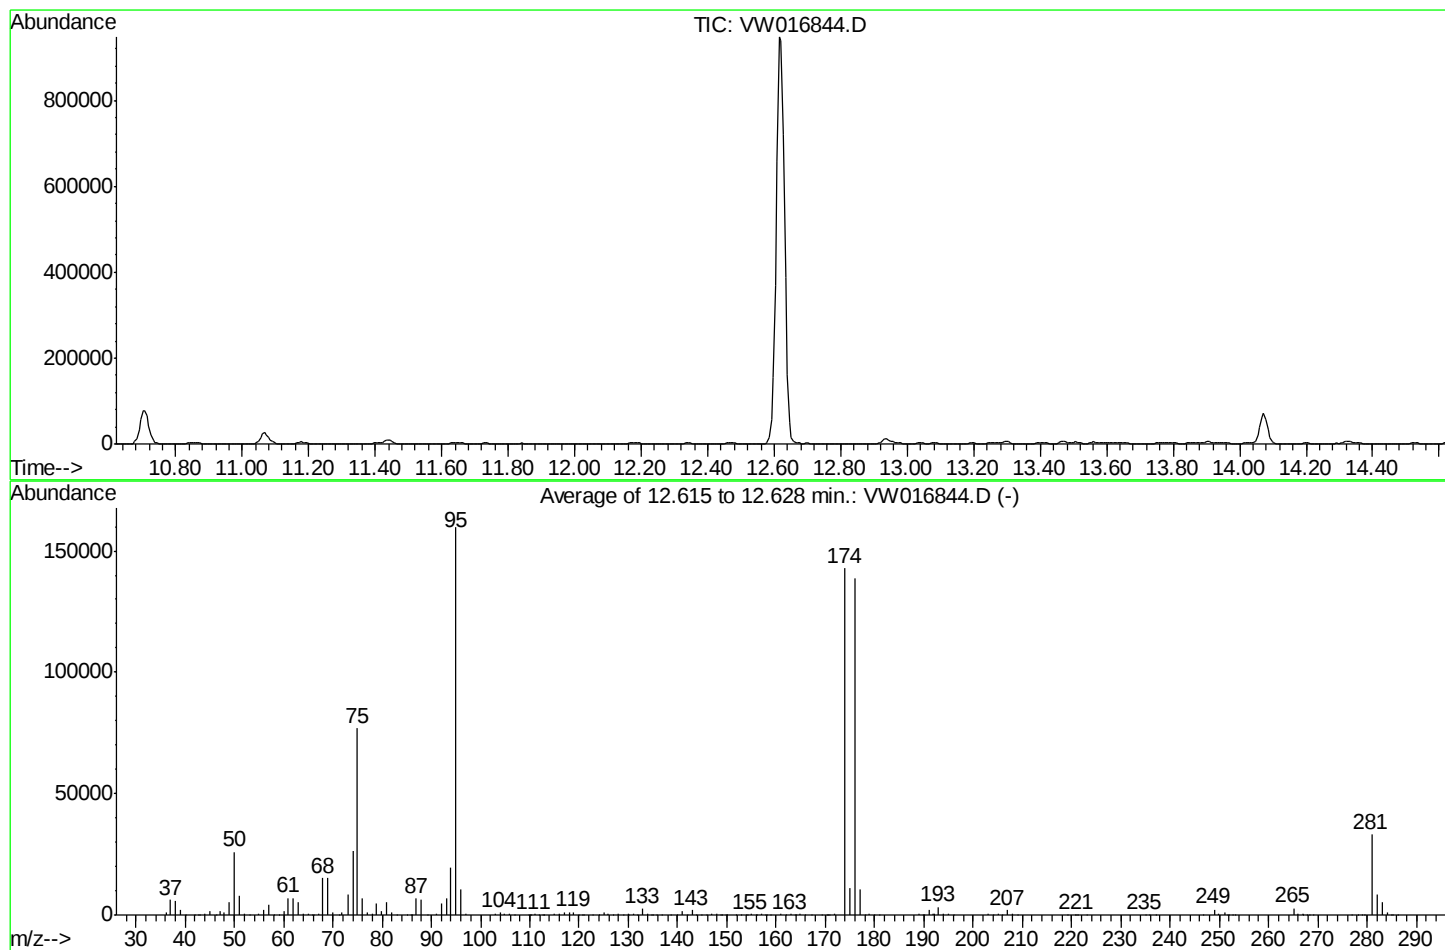

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.2	25949	PASS
75	95	30	80	48.1	76856	PASS
95	95	100	100	100.0	159701	PASS
96	95	5	9	6.8	10790	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	89.4	142720	PASS
175	174	5	9	7.8	11188	PASS
176	174	95	101	97.0	138437	PASS
177	176	5	9	7.5	10321	PASS

m/z	Abundance
36.00	1277.0
37.00	7034.0
38.00	6455.0
39.00	2401.0
40.10	318.0
42.00	81.0
43.10	146.0
44.00	1172.0
45.00	1892.0
46.20	155.0
47.00	1557.0
47.90	949.0
49.00	5948.0
50.00	29384.0
51.00	8955.0
52.00	401.0
53.10	78.0
55.00	474.0
56.00	2284.0
57.00	4513.0
58.10	180.0
59.10	406.0
60.10	1408.0
61.00	7734.0
62.00	7473.0
63.00	6374.0
64.00	725.0
65.10	358.0
66.10	98.0
67.00	489.0
68.00	16472.0
69.00	17488.0
70.10	1394.0
71.90	1011.0
73.00	10754.0
74.00	28760.0
75.00	82232.0
76.00	7697.0
77.00	924.0
78.10	665.0
78.90	5210.0
79.90	1462.0
80.90	5416.0
82.00	1284.0
83.10	153.0
84.90	56.0
85.80	220.0
87.00	7126.0
88.00	6641.0
90.90	875.0
92.00	4900.0
93.00	7422.0
94.00	21528.0
95.00	169664.0
96.00	11586.0
97.10	309.0
103.10	793.0
104.00	984.0
104.90	512.0
105.90	773.0
106.90	224.0
110.00	432.0
111.00	466.0
111.90	251.0
112.90	137.0
114.90	448.0
115.80	677.0
116.90	1286.0
118.00	1182.0
118.90	1608.0
120.00	165.0
120.70	138.0
121.10	125.0
122.80	124.0
123.90	185.0
125.00	1455.0
125.80	381.0
126.80	111.0
127.80	800.0
128.90	322.0
129.90	681.0
130.90	422.0
131.90	180.0
133.00	4004.0
133.80	1307.0
134.70	570.0
136.80	318.0
139.90	161.0
141.00	1791.0
142.90	1859.0
143.80	121.0
144.90	417.0

Instrument :
MSVOA_W
ClientSampleId :
BFB11

145.90	249.0
147.00	690.0
147.90	520.0
148.80	358.0
150.10	260.0
152.90	135.0
154.00	72.0
154.90	489.0
155.90	96.0
157.00	311.0
158.10	162.0
158.80	294.0
160.90	474.0
162.00	124.0
162.90	764.0
163.80	103.0
165.00	591.0
165.80	133.0
167.00	102.0
169.00	75.0
170.90	83.0
171.90	690.0
173.90	139968.0
175.00	11150.0
175.90	135360.0
177.00	10740.0
178.00	601.0
178.90	1121.0
179.90	214.0
181.00	139.0
189.00	548.0
189.90	176.0
191.00	3874.0
191.90	937.0
193.00	5103.0
193.90	1054.0
195.00	449.0
195.90	126.0
202.90	564.0
204.00	79.0
204.90	896.0
206.10	251.0
207.00	3294.0
208.00	791.0
208.90	509.0
219.10	78.0
221.00	215.0
223.00	100.0
235.00	453.0
235.90	157.0
237.10	146.0
246.80	70.0
249.10	3231.0
250.00	971.0
251.00	1558.0
252.00	289.0
252.80	216.0
265.10	4181.0
266.00	1169.0
266.90	769.0
267.80	127.0
268.20	145.0
269.10	103.0
276.90	123.0
278.20	129.0
279.10	227.0
281.00	46792.0
282.10	13806.0
283.10	8067.0
284.10	1754.0
285.00	545.0
286.10	152.0

Instrument :
MSVOA_W
ClientSampleId :
BFB11

m/z	Abundance
36.10	1178.0
37.00	6788.0
38.00	6010.0
39.00	2325.0
40.00	226.0
40.90	62.0
43.00	190.0
44.00	1181.0
45.00	1304.0
47.00	1999.0
48.00	874.0
49.00	5997.0
50.00	27912.0
51.00	8901.0
52.00	453.0
53.10	51.0
54.90	317.0
55.10	318.0
56.00	2157.0
57.00	4476.0
58.00	206.0
59.00	187.0
60.00	1608.0
61.00	7455.0
62.00	7556.0
63.00	5823.0
64.00	611.0
65.00	410.0
65.70	53.0
67.10	446.0
68.00	16464.0
69.00	16936.0
70.00	1222.0
71.90	977.0
73.00	9427.0
74.00	29248.0
75.00	86576.0
76.10	7344.0
77.00	787.0
77.90	686.0
78.90	4978.0
79.90	1741.0
80.90	5900.0
81.90	1279.0
82.90	119.0
85.70	91.0
86.10	201.0
86.90	7545.0
87.90	7191.0
89.20	71.0
90.90	724.0
92.00	5217.0
93.00	7597.0
94.00	21376.0
95.00	177536.0
96.00	12293.0
96.90	357.0
102.90	520.0
103.90	912.0
104.80	353.0
105.90	744.0
107.00	204.0
109.70	209.0
110.20	274.0
110.90	297.0
111.90	102.0
112.60	169.0
113.00	156.0
114.80	289.0
115.90	736.0
116.90	1153.0
117.90	827.0
118.90	1569.0
120.00	103.0
120.90	179.0
122.80	99.0
124.00	95.0
124.90	636.0
125.80	399.0
126.80	66.0
127.90	821.0
128.80	287.0
129.90	705.0
131.00	267.0
132.00	104.0
132.90	2202.0
134.90	507.0
135.70	52.0
136.90	330.0
140.00	228.0
140.90	1676.0
142.00	350.0

Instrument :
MSVOA_W
ClientSampleId :
BFB11

142.90	2285.0
143.80	118.0
144.80	279.0
145.90	266.0
146.80	442.0
147.90	397.0
149.00	162.0
149.70	246.0
151.90	112.0
153.00	134.0
154.10	61.0
155.00	486.0
156.10	199.0
156.90	335.0
158.00	89.0
158.90	329.0
161.00	425.0
162.00	102.0
162.90	489.0
164.10	102.0
165.00	290.0
165.80	101.0
167.10	58.0
169.20	62.0
170.30	70.0
171.90	750.0
173.90	147392.0
175.00	12037.0
175.90	150656.0
177.00	10900.0
179.00	437.0
179.90	122.0
180.90	75.0
189.00	250.0
190.10	194.0
191.10	2292.0
192.10	571.0
193.00	3042.0
194.00	485.0
194.90	448.0
195.90	57.0
203.00	294.0
204.00	112.0
205.00	548.0
205.90	208.0
207.00	1907.0
208.00	387.0
209.00	227.0
220.60	81.0
221.20	84.0
235.00	194.0
249.00	2384.0
249.80	384.0
251.00	1120.0
251.90	272.0
253.10	97.0
265.00	2772.0
266.00	532.0
267.10	707.0
267.80	120.0
268.30	56.0
269.20	59.0
277.00	64.0
278.90	228.0
279.60	253.0
281.00	34400.0
282.10	8605.0
283.00	5408.0
284.10	1129.0
285.20	372.0

Instrument :
MSVOA_W
ClientSampleId :
BFB11

m/z	Abundance
36.00	789.0
37.00	4867.0
38.00	4428.0
39.10	1555.0
40.00	207.0
42.80	131.0
44.00	724.0
45.00	883.0
46.20	95.0
47.00	1080.0
47.90	792.0
49.00	4403.0
50.00	20552.0
51.00	6304.0
52.00	217.0
53.00	57.0
54.90	357.0
56.00	1823.0
57.00	3262.0
57.90	89.0
59.00	165.0
60.00	1143.0
61.00	5405.0
62.00	5320.0
63.00	3848.0
64.10	408.0
65.00	326.0
65.70	68.0
66.90	324.0
68.00	12341.0
69.00	11735.0
70.00	877.0
71.20	56.0
72.00	614.0
73.00	5870.0
74.00	21408.0
75.00	61760.0
76.00	5225.0
77.00	846.0
77.90	452.0
78.90	3719.0
80.00	1156.0
80.90	3885.0
81.90	967.0
82.90	127.0
85.00	97.0
86.10	152.0
87.00	5333.0
87.90	5169.0
90.90	580.0
92.00	3902.0
93.00	6201.0
94.00	16007.0
95.00	131904.0
96.00	8491.0
97.00	228.0
102.90	244.0
103.90	684.0
104.90	302.0
105.90	489.0
107.00	127.0
110.10	146.0
110.90	177.0
111.80	214.0
112.70	88.0
112.90	89.0
114.90	262.0
116.00	471.0
117.00	979.0
117.90	710.0
119.00	663.0
120.90	88.0
122.80	57.0
123.90	150.0
124.90	370.0
125.80	191.0
126.80	81.0
127.90	567.0
128.80	219.0
130.10	474.0
130.90	283.0
133.10	971.0
133.70	295.0
134.90	356.0
135.80	104.0
136.80	215.0
138.70	74.0
140.90	1361.0
142.10	187.0
142.90	1804.0
143.90	58.0
144.80	82.0

Instrument :
MSVOA_W
ClientSampleId :
BFB11

145.90	210.0
146.80	304.0
147.90	431.0
148.80	162.0
150.00	165.0
152.00	121.0
152.80	88.0
153.80	111.0
155.00	353.0
156.00	111.0
156.90	390.0
157.80	76.0
158.90	184.0
160.90	292.0
162.80	141.0
164.80	159.0
170.50	63.0
171.80	694.0
174.00	140800.0
175.00	10378.0
175.90	129296.0
177.00	9325.0
178.00	244.0
178.90	283.0
189.10	84.0
189.90	75.0
191.00	776.0
192.10	323.0
193.00	1503.0
194.10	261.0
194.90	169.0
202.90	169.0
205.10	290.0
206.00	115.0
207.00	1193.0
208.00	191.0
209.00	91.0
234.80	119.0
248.90	1111.0
249.90	252.0
251.00	305.0
251.60	94.0
252.00	87.0
265.00	1363.0
266.00	377.0
267.10	213.0
279.40	70.0
281.00	18040.0
282.10	3572.0
283.10	2897.0
284.00	592.0
285.10	145.0

Instrument :
MSVOA_W
ClientSampleId :
BFB11

Scan 1749 (12.567 min): VW016844.D
BFB11

m/z	Abundance
40.00	191.0
41.00	61.0
43.00	57.0
44.10	286.0
55.00	56.0
55.90	75.0
169.00	57.0
207.00	73.0

Instrument :
MSVOA_W
ClientSampleId :
BFB11