

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100923\
 Data File : VW027274.D
 Acq On : 09 Oct 2023 11:40
 Operator : SY/MD
 Sample : 04771-06RE
 Misc : 5.54g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EX05J0RE

Quant Time: Oct 10 01:19:34 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092723SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Oct 07 00:22:13 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	1031357	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	871309	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	302910	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.369	65	268440	16.566	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	66.280%		
7) Chloroethane-d5	2.899	69	248120	19.374	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	77.480%		
11) 1,1-Dichloroethene-d2	4.027	65	134943	20.044	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	80.160%		
21) 2-Butanone-d5	7.075	46	160705	47.973	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	95.940%		
24) Chloroform-d	7.648	84	652407	21.614	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	86.440%		
26) 1,2-Dichloroethane-d4	8.307	65	330588	22.853	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	91.400%		
32) Benzene-d6	8.276	84	1307693	24.489	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	97.960%		
36) 1,2-Dichloropropane-d6	9.270	67	416067	26.026	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	104.120%		
41) Toluene-d8	10.318	98	1058787	22.469	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	89.880%		
43) trans-1,3-Dichloroprop...	10.574	79	143122	22.813	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	91.240%		
47) 2-Hexanone-d5	10.922	63	106414	43.513	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	87.020%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	291850	23.854	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	95.400%		
66) 1,2-Dichlorobenzene-d4	13.848	152	214041	21.075	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	84.280%		
Target Compounds						Qvalue
31) Carbon tetrachloride	8.069	117	59954	2.931	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100923\
Data File : VW027274.D
Acq On : 09 Oct 2023 11:40
Operator : SY/MD
Sample : 04771-06RE
Misc : 5.54g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EX05J0RE

Quant Time: Oct 10 01:19:34 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092723SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Oct 07 00:22:13 2023
Response via : Initial Calibration

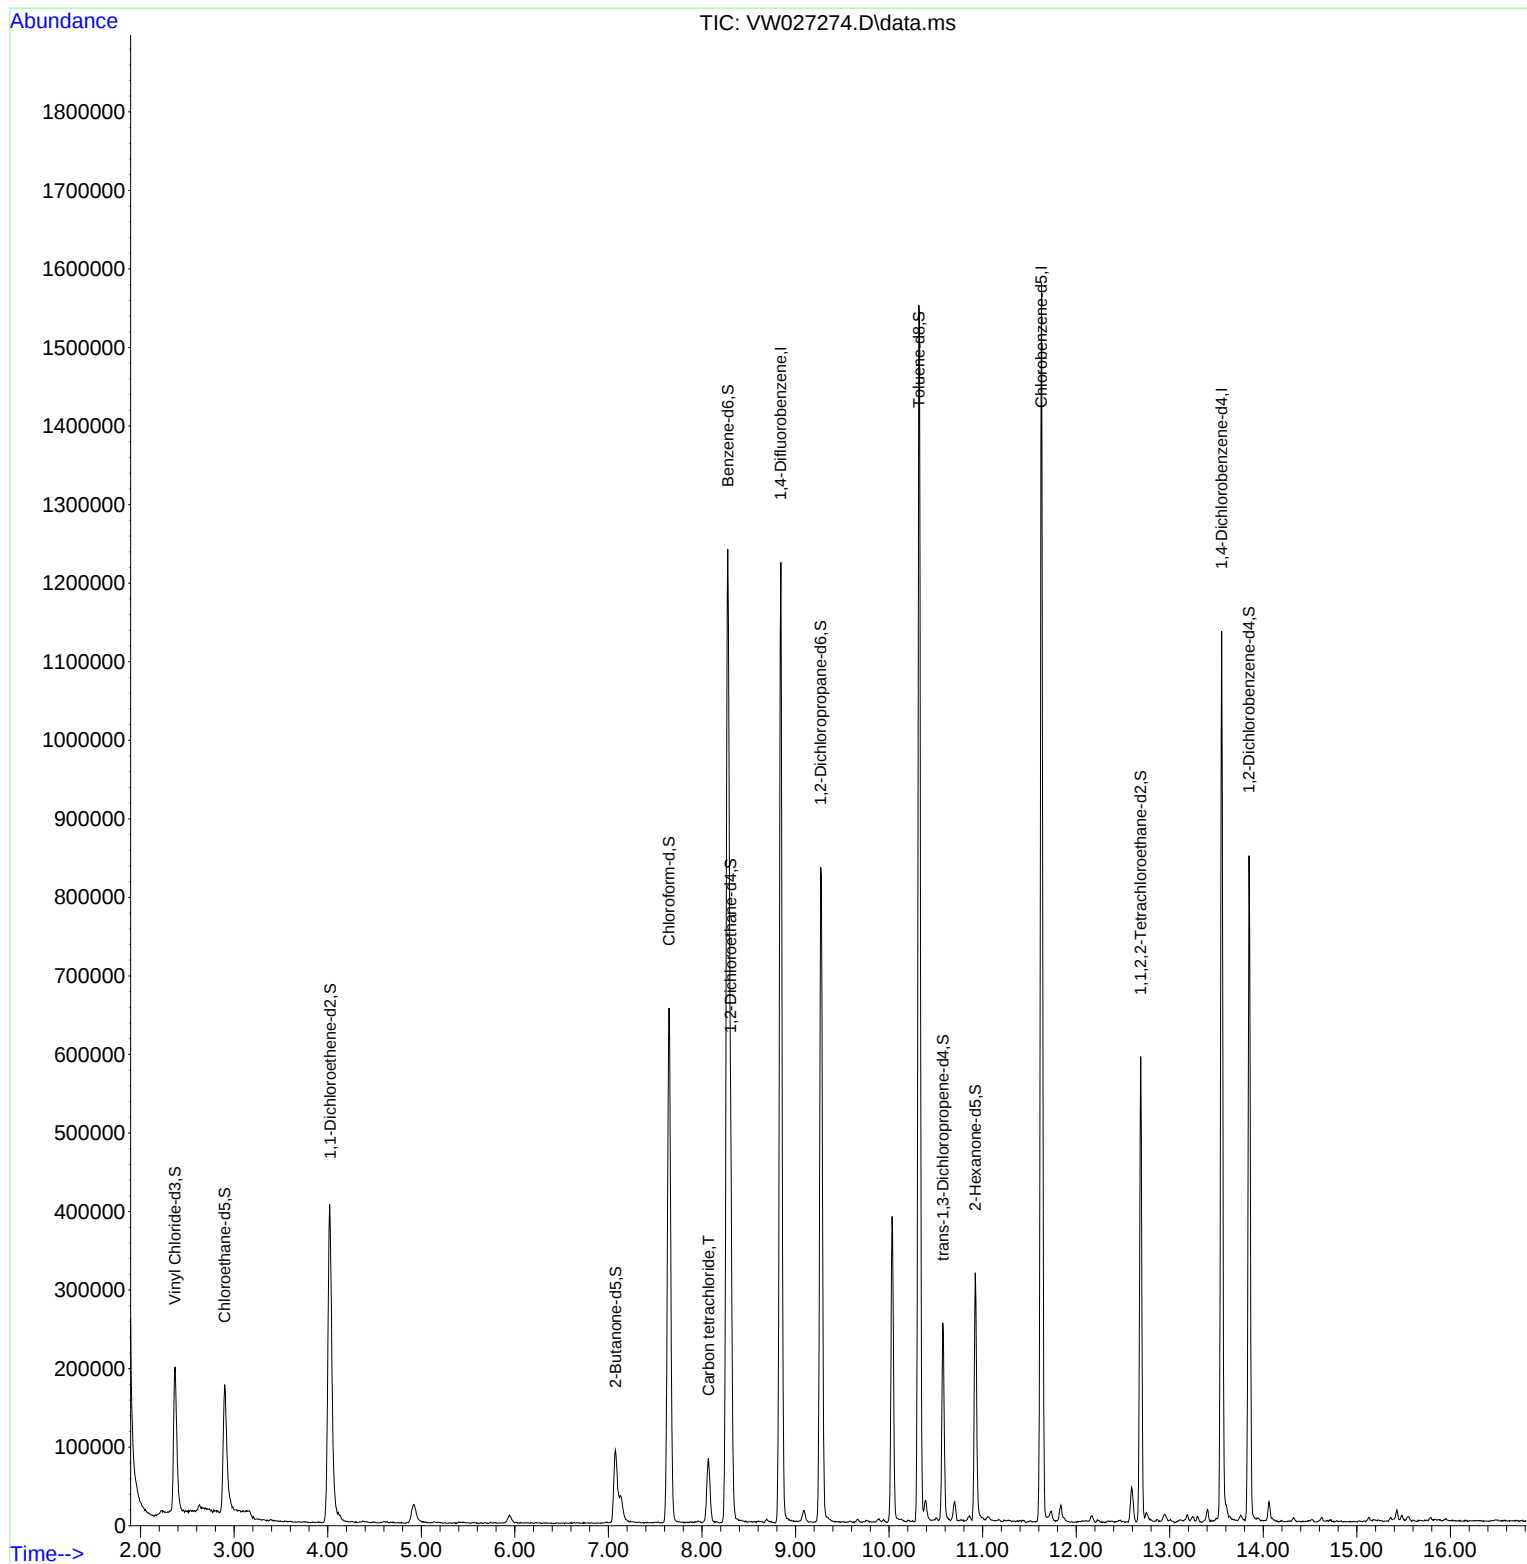

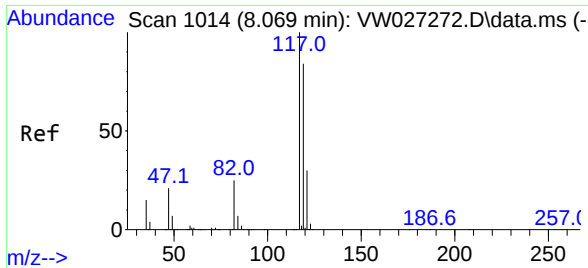

#31
Carbon tetrachloride
Concen: 2.931 ug/L
RT: 8.069 min Scan# 10
Delta R.T. -0.000 min
Lab File: VW027274.D
Acq: 09 Oct 2023 11:40

Instrument :
MSVOA_W
ClientSampleId :
EX05J0RE

Tgt Ion:117 Resp: 59954
Ion Ratio Lower Upper
117 100
119 97.7 77.0 115.6

