

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100923\
 Data File : VW027275.D
 Acq On : 09 Oct 2023 12:04
 Operator : SY/MD
 Sample : 04771-07RE
 Misc : 3.69g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 E05J2RE

Quant Time: Oct 10 01:19:42 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092723SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Oct 07 00:22:13 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	972647	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	888145	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	321057	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.369	65	308710	20.201	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	80.800%
7) Chloroethane-d5	2.899	69	276802	22.918	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	91.680%
11) 1,1-Dichloroethene-d2	4.021	65	129245	20.356	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	81.440%
21) 2-Butanone-d5	7.075	46	167567	53.041	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	106.080%
24) Chloroform-d	7.648	84	646345	22.706	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	90.840%
26) 1,2-Dichloroethane-d4	8.307	65	328969	24.114	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	96.440%
32) Benzene-d6	8.276	84	1300629	23.895	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	95.560%
36) 1,2-Dichloropropane-d6	9.270	67	419027	25.714	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	102.840%
41) Toluene-d8	10.319	98	1063678	22.145	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	88.600%
43) trans-1,3-Dichloroprop...	10.581	79	145292	22.719	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	90.880%
47) 2-Hexanone-d5	10.922	63	113835	45.666	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	91.340%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	328350	26.329	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	105.320%
66) 1,2-Dichlorobenzene-d4	13.855	152	284024	26.385	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	105.520%
Target Compounds						
13) Acetone	4.125	43	15934	4.082	ug/L	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100923\
Data File : VW027275.D
Acq On : 09 Oct 2023 12:04
Operator : SY/MD
Sample : 04771-07RE
Misc : 3.69g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
E05J2RE

Quant Time: Oct 10 01:19:42 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092723SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Oct 07 00:22:13 2023
Response via : Initial Calibration

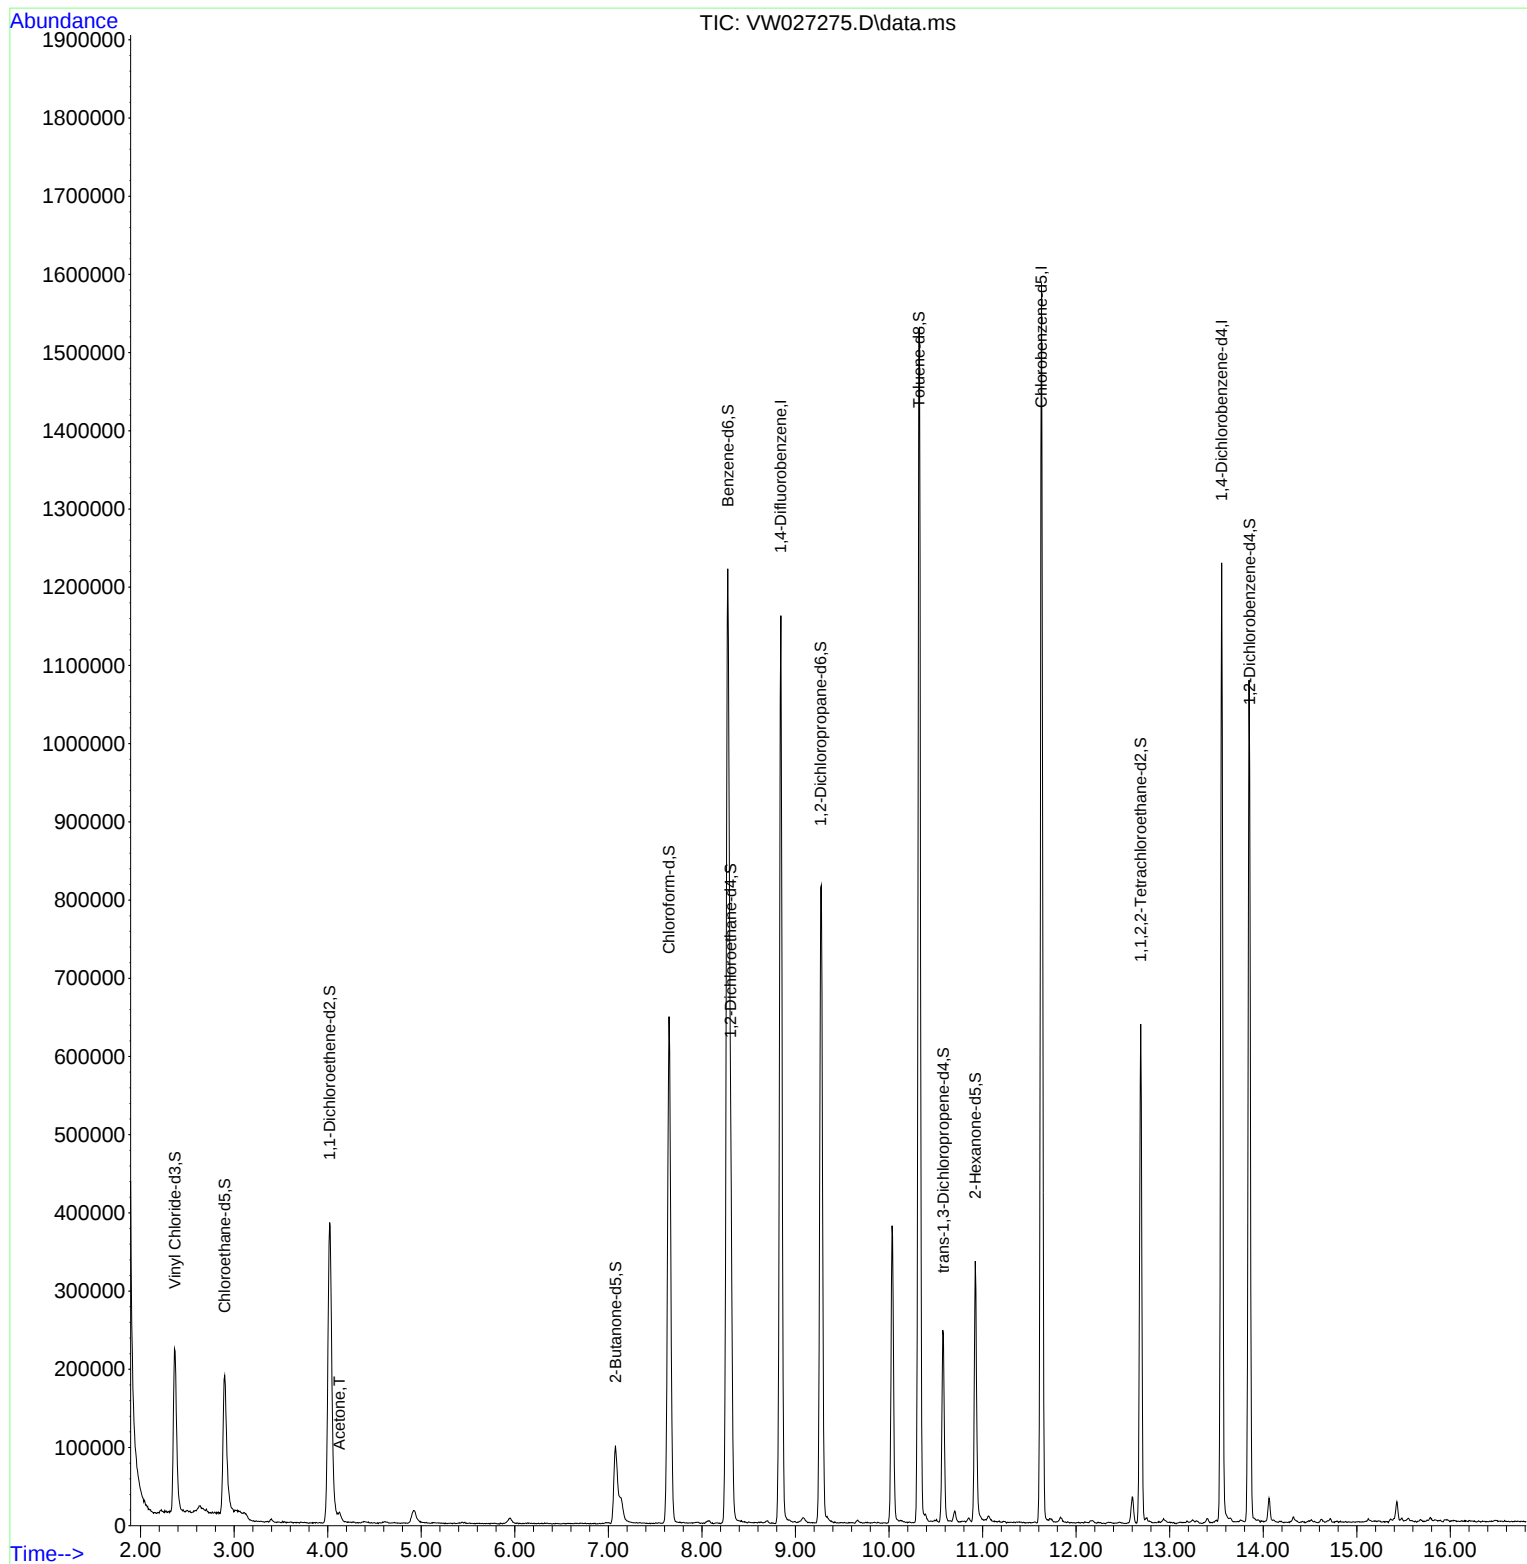

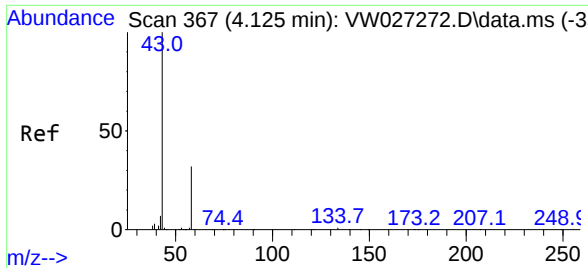

#13
 Acetone
 Concen: 4.082 ug/L
 RT: 4.125 min Scan# 30
 Delta R.T. 0.006 min
 Lab File: VW027275.D
 Acq: 09 Oct 2023 12:04

Instrument :
 MSVOA_W
 ClientSampleId :
 E05J2RE

Tgt Ion: 43 Resp: 15934
 Ion Ratio Lower Upper
 43 100
 58 34.9 0.0 70.4

