

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW101018\
 Data File : VW005961.D
 Acq On : 10 Oct 2018 01:49
 Operator : SY/AP
 Sample : J5326-01RE
 Misc : 9.25G/5ML/MSVOA_W/SOIL
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 FL-PIT-1

Quant Time: Oct 10 03:00:12 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W100818S.M
 Quant Title : SW846 8260
 QLast Update : Tue Oct 09 02:14:04 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.95	168	254361	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.84	114	390021	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.63	117	341859	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.56	152	155379	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.31	65	127710	51.72	ug/l	0.00
Spiked Amount 50.000			Recovery	=	103.44%	
35) Dibromofluoromethane	7.88	113	125281	50.31	ug/l	0.00
Spiked Amount 50.000			Recovery	=	100.62%	
50) Toluene-d8	10.33	98	465501	48.59	ug/l	0.00
Spiked Amount 50.000			Recovery	=	97.18%	
62) 4-Bromofluorobenzene	12.62	95	151030	41.43	ug/l	0.00
Spiked Amount 50.000			Recovery	=	82.86%	
Target Compounds						
					Qvalue	
16) Acetone	4.15	43	14706	29.816	ug/l	99
20) Methylene Chloride	4.92	84	17213	6.966	ug/l	94
25) 2-Butanone	7.16	43	1776	2.532	ug/l #	65
31) Cyclohexane	7.95	56	4832	1.118	ug/l #	1
36) 1,1-Dichloropropene	7.95	75	16582	4.437	ug/l #	49
38) Carbon Tetrachloride	7.95	117	22629	5.636	ug/l #	14
76) 1,2,3-Trichloropropane	12.62	75	77437	55.792	ug/l #	100
81) trans-1,4-Dichloro-2-buten	12.62	75	77437	117.783	ug/l #	11

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_W\DATA\VW101018\
Data File : VW005961.D
Acq On : 10 Oct 2018 01:49
Operator : SY/AP
Sample : J5326-01RE
Misc : 9.25G/5ML/MSVOA_W/SOIL
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
FL-PIT-1

Quant Time: Oct 10 03:00:12 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\82W100818S.M
Quant Title : SW846 8260
QLast Update : Tue Oct 09 02:14:04 2018
Response via : Initial Calibration

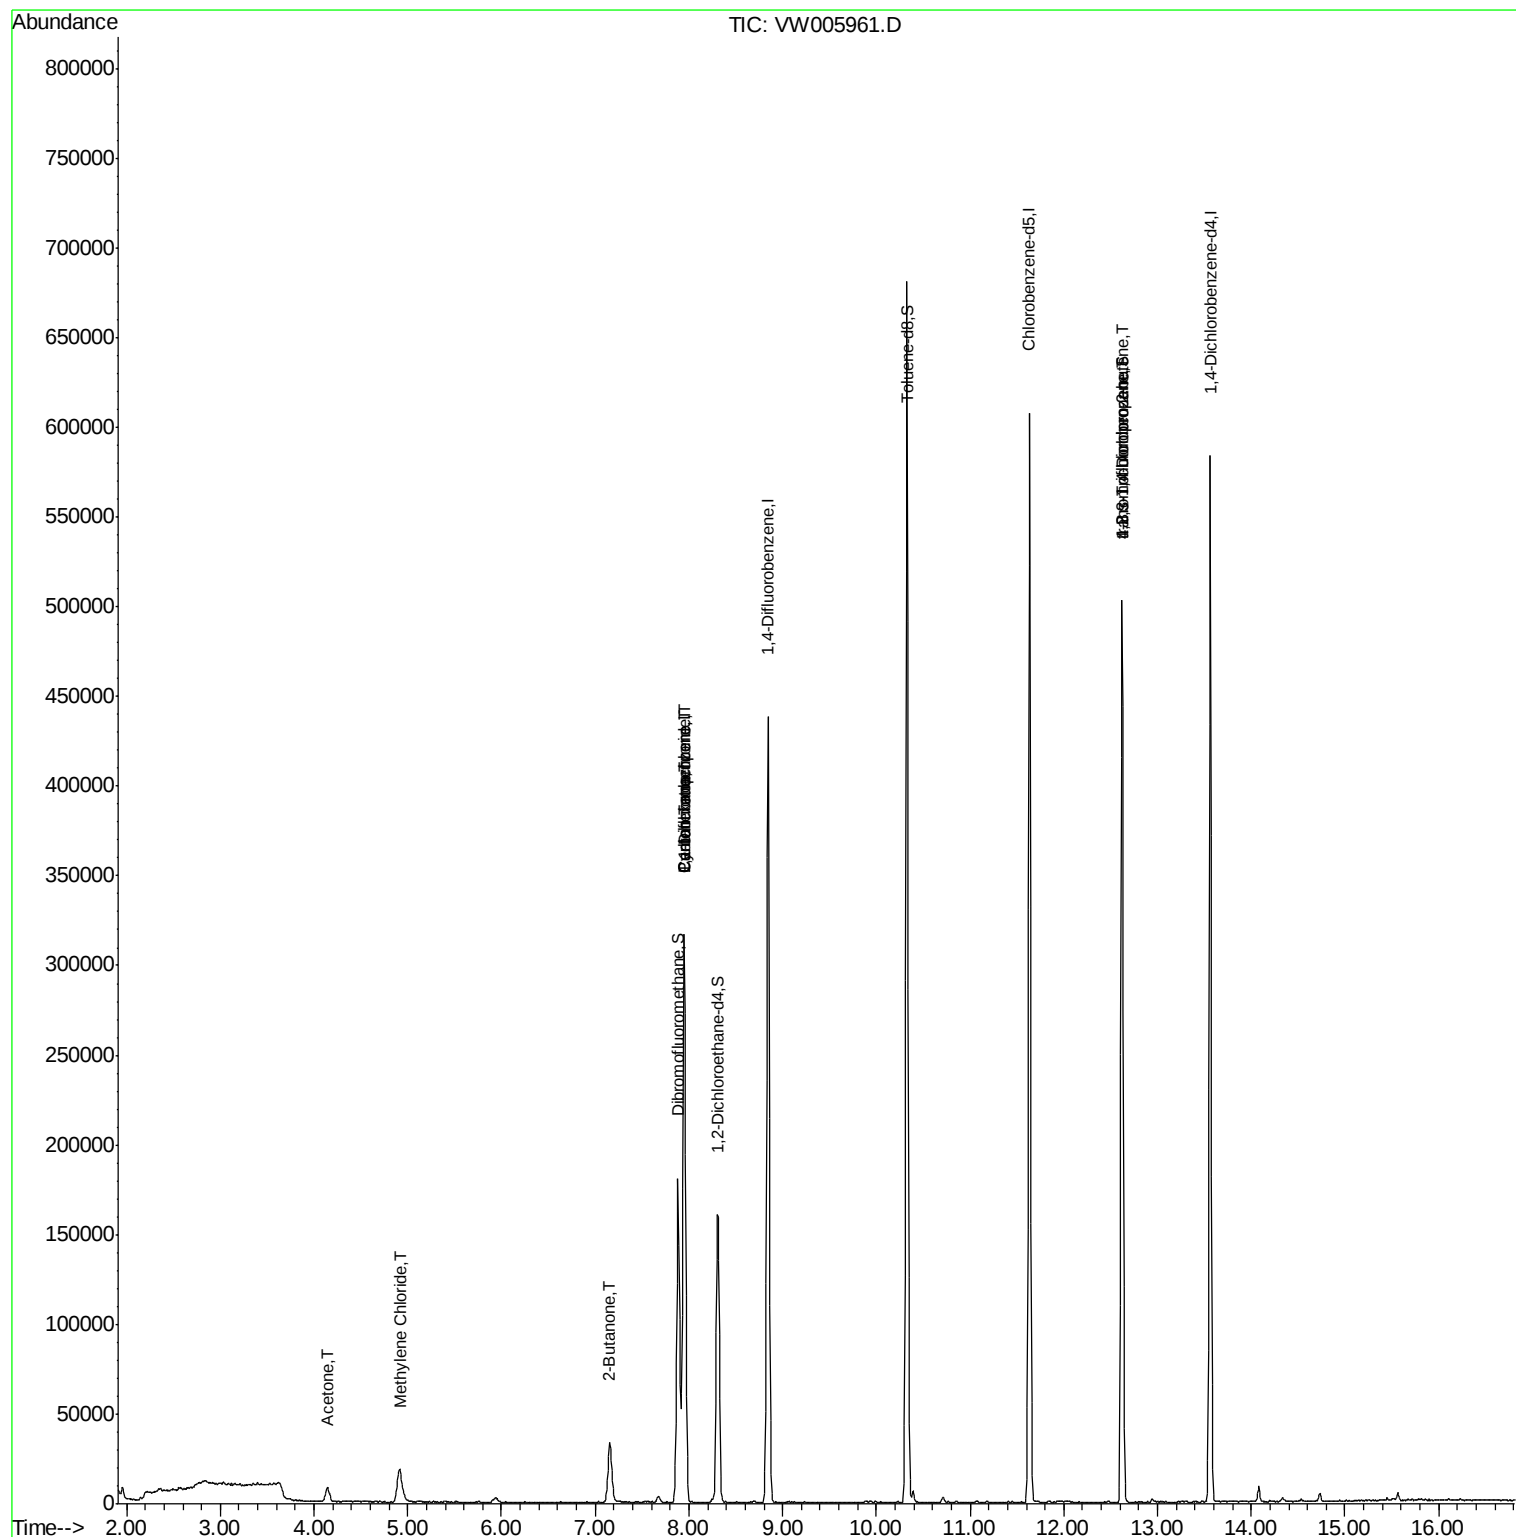



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.95 min Scan# 992

Delta R.T. 0.00 min

Lab File: VW005961.D

Acq: 10 Oct 2018 01:49

Instrument :

MSVOA_W

ClientSampleId :


FL-PIT-1

Tgt Ion:168 Resp: 254361

Ion Ratio Lower Upper

168 100

99 49.6 40.9 61.3

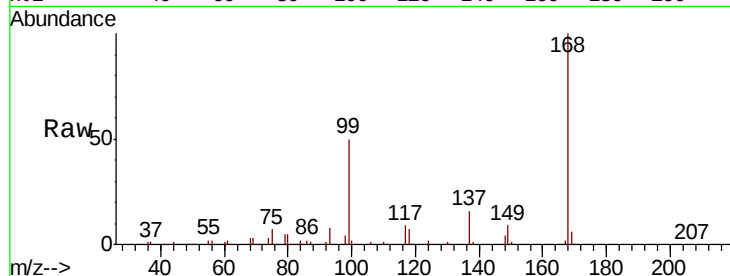

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VW



7.95

100000

50000

0

Time-->



#16

Acetone

Concen: 29.816 ug/l

RT: 4.15 min Scan# 368

Delta R.T. 0.01 min

Lab File: VW005961.D


Acq: 10 Oct 2018 01:49

Tgt Ion: 43 Resp: 14706

Ion Ratio Lower Upper

43 100

58 30.1 24.7 37.1



Abundance Ion 43.00 (42.70 to 43.70): VW

Ion 58.00 (57.70 to 58.70): VW

4.15

5000

4000


3000

2000

1000

0

Time-->






#20
Methylene Chloride
Concen: 6.966 ug/l
RT: 4.92 min Scan# 494
Delta R.T. 0.01 min
Lab File: VW005961.D
Acq: 10 Oct 2018 01:49

Instrument :
MSVOA_W
ClientSampled :
FL-PIT-1

Tgt Ion:	84	Resp:	17213
Ion	Ratio	Lower	Upper
84	100		
49	115.5	99.9	149.9
51	37.9	31.1	46.7
86	68.3	51.8	77.6






Abundance

Ion 83.90 (83.60 to 84.60): VW

Ion 48.90 (48.60 to 49.60): VW


Ion 50.90 (50.60 to 51.60): VW

Ion 85.90 (85.60 to 86.60): VW

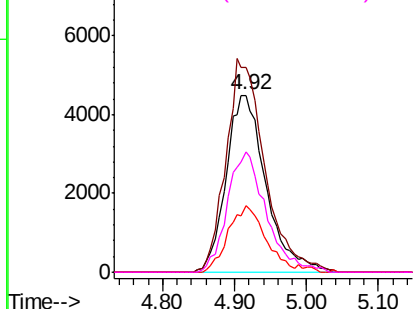

#25
2-Butanone
Concen: 2.532 ug/l
RT: 7.16 min Scan# 862
Delta R.T. -0.02 min
Lab File: VW005961.D
Acq: 10 Oct 2018 01:49



Tgt Ion:	43	Resp:	1776
Ion	Ratio	Lower	Upper
43	100		
72	8.5	21.0	31.4#




Abundance

Ion 43.00 (42.70 to 43.70): VW

Ion 72.00 (71.70 to 72.70): VW

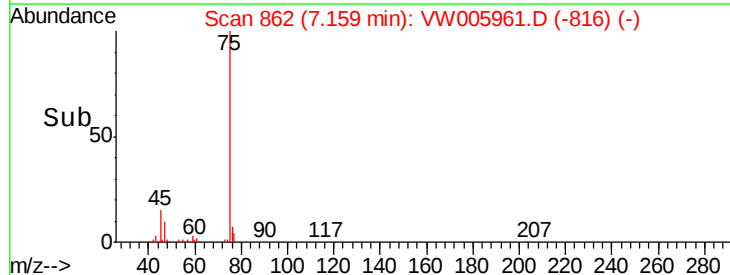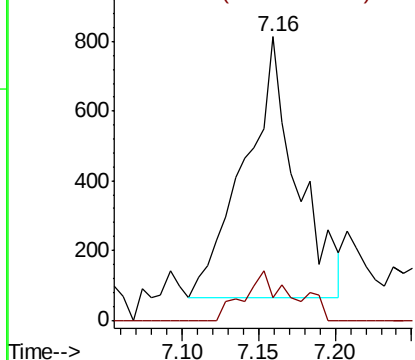


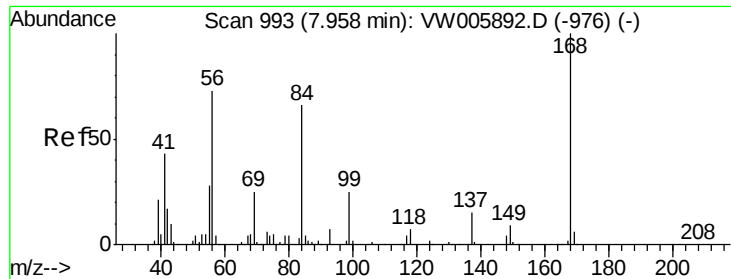




#31
Cyclohexane
Concen: 1.118 ug/l
RT: 7.95 min Scan# 992
Delta R.T. -0.01 min
Lab File: VW005961.D
Acq: 10 Oct 2018 01:49

Instrument :
MSVOA_W
ClientSampleId :
FL-PIT-1

Tgt Ion: 56 Resp: 4832
Ion Ratio Lower Upper
56 100
69 175.6 27.9 41.9#
84 135.1 72.3 108.5#

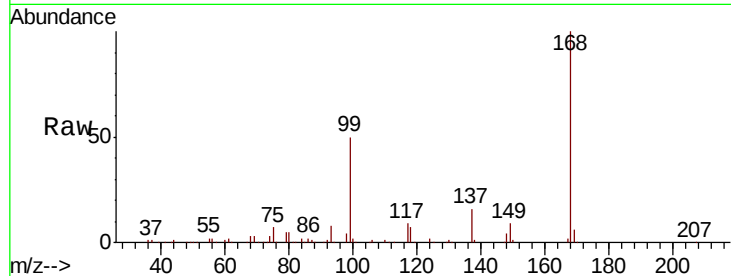


Abundance Ion 56.00 (55.70 to 56.70): VW
Ion 69.00 (68.70 to 69.70): VW
Ion 84.00 (83.70 to 84.70): VW

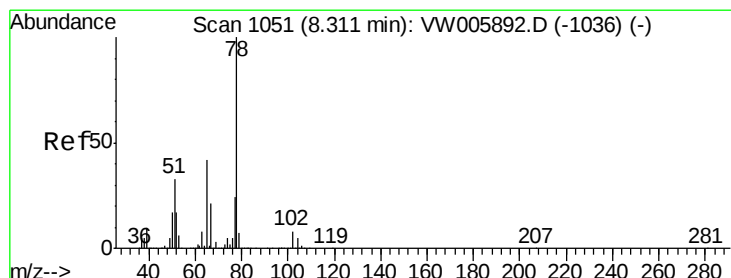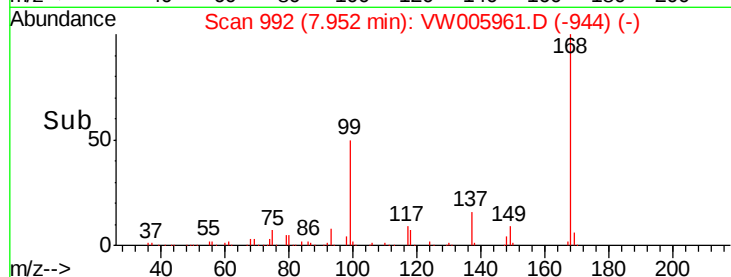
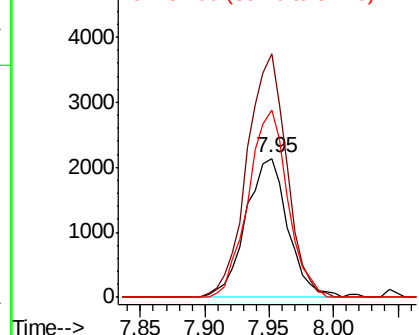



#33
1,2-Dichloroethane-d4
Concen: 51.720 ug/l
RT: 8.31 min Scan# 1050
Delta R.T. -0.01 min
Lab File: VW005961.D
Acq: 10 Oct 2018 01:49

Tgt Ion: 65 Resp: 127710
Ion Ratio Lower Upper
65 100
67 52.0 0.0 104.6

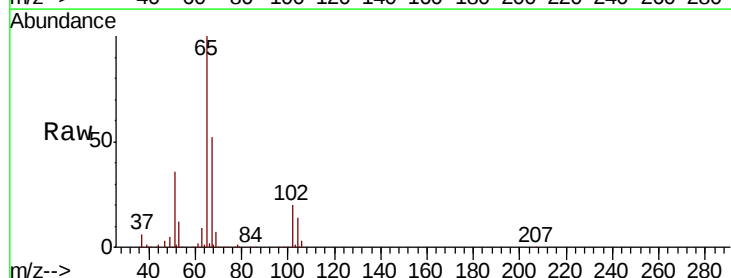

Abundance Ion 64.90 (64.60 to 65.60): VW
Ion 66.90 (66.60 to 67.60): VW

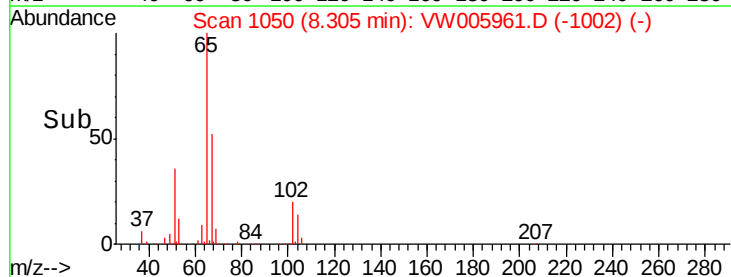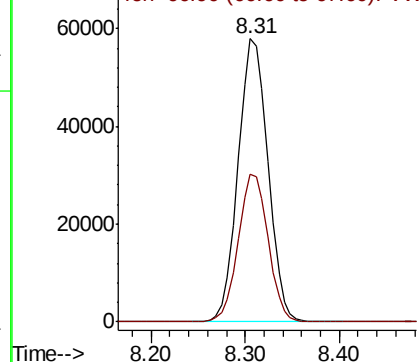







#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.84 min Scan# 1138
Delta R.T. 0.00 min
Lab File: VW005961.D
Acq: 10 Oct 2018 01:49

Instrument :
MSVOA_W
ClientSampled :
FL-PIT-1

Tgt Ion:114 Resp: 390021
Ion Ratio Lower Upper
114 100
63 19.1 0.0 39.2
88 14.6 0.0 30.8

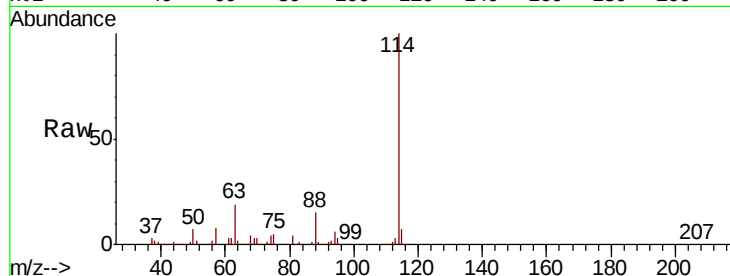


Abundance Ion 113.90 (113.60 to 114.60): V
Ion 63.00 (62.70 to 63.70): VW
Ion 87.90 (87.60 to 88.60): VW


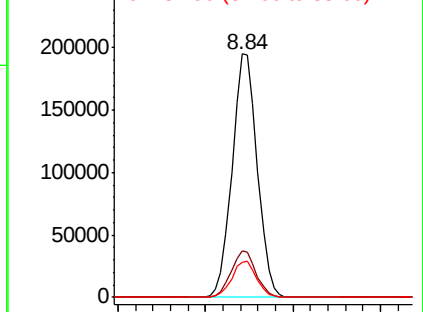



#35
Dibromofluoromethane
Concen: 50.311 ug/l
RT: 7.88 min Scan# 981
Delta R.T. 0.00 min
Lab File: VW005961.D
Acq: 10 Oct 2018 01:49

Tgt Ion:113 Resp: 125281
Ion Ratio Lower Upper
113 100
111 102.2 82.0 123.0
192 22.2 18.3 27.5



Abundance Ion 112.80 (112.50 to 113.50): V
Ion 110.80 (110.50 to 111.50): V
Ion 191.70 (191.40 to 192.40): V




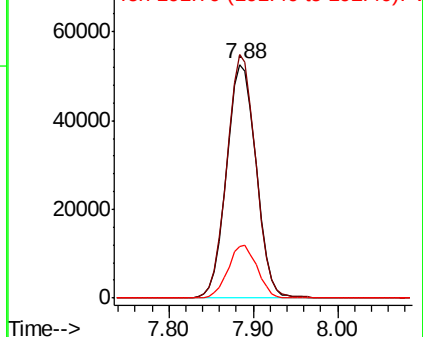




#36
 1,1-Dichloropropene
 Concen: 4.437 ug/l
 RT: 7.95 min Scan# 992
 Delta R.T. -0.13 min
 Lab File: VW005961.D
 Acq: 10 Oct 2018 01:49




Instrument :
 MSVOA_W
 ClientSampled :
 FL-PIT-1


Tgt Ion: 75 Resp: 16582
 Ion Ratio Lower Upper
 75 100
 110 9.5 18.6 56.0#
 77 0.0 24.7 37.1#

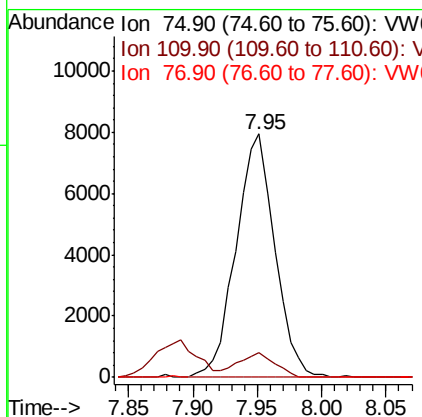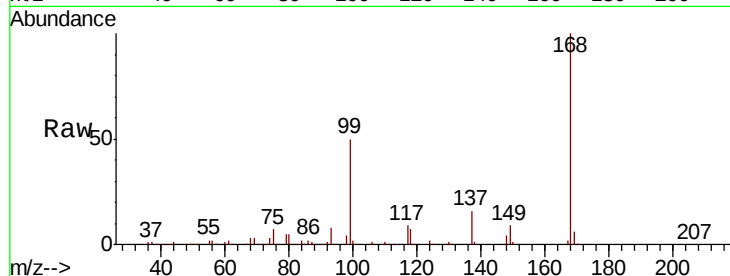

#38
 Carbon Tetrachloride
 Concen: 5.636 ug/l
 RT: 7.95 min Scan# 992
 Delta R.T. -0.12 min
 Lab File: VW005961.D
 Acq: 10 Oct 2018 01:49

Tgt Ion: 117 Resp: 22629
 Ion Ratio Lower Upper
 117 100
 119 3.5 78.6 117.8#
 121 0.0 25.3 37.9#

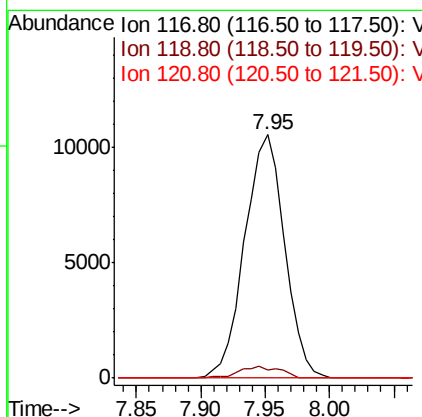



#50

Toluene-d8

Concen: 48.588 ug/l

RT: 10.33 min Scan# 1382

Delta R.T. 0.00 min

Lab File: VW005961.D

Acq: 10 Oct 2018 01:49

Instrument :

MSVOA_W

ClientSampleId :





FL-PIT-1

Tgt Ion: 98 Resp: 465501

Ion Ratio Lower Upper

98 100

100 64.2 51.9 77.9

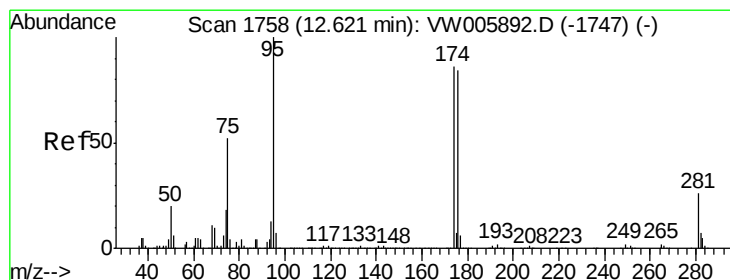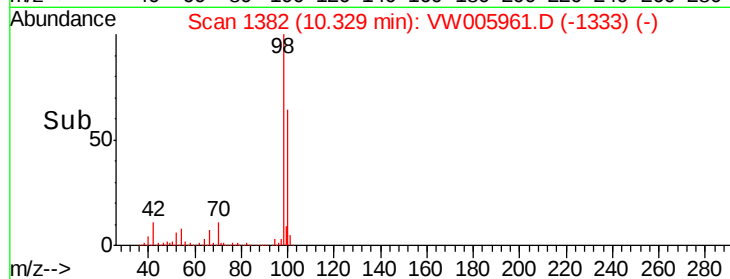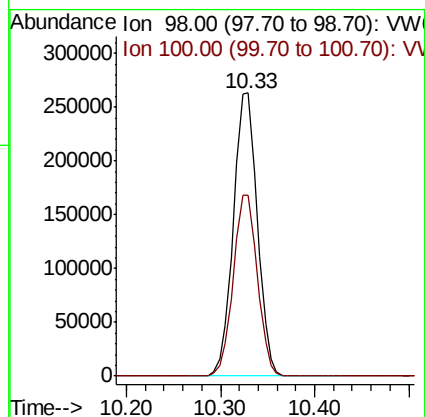

#62

4-Bromofluorobenzene

Concen: 41.434 ug/l

RT: 12.62 min Scan# 1758

Delta R.T. 0.00 min

Lab File: VW005961.D

Acq: 10 Oct 2018 01:49




Tgt Ion: 95 Resp: 151030


Ion Ratio Lower Upper

95 100

174 92.8 0.0 176.4

176 90.2 0.0 173.0


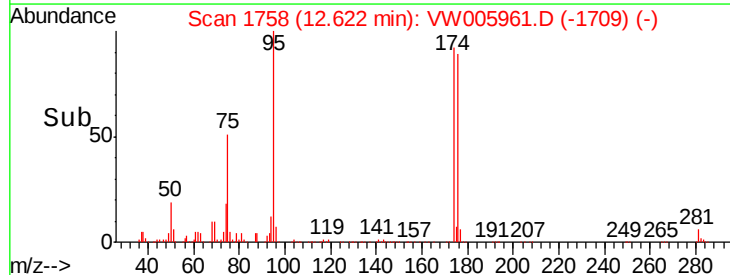
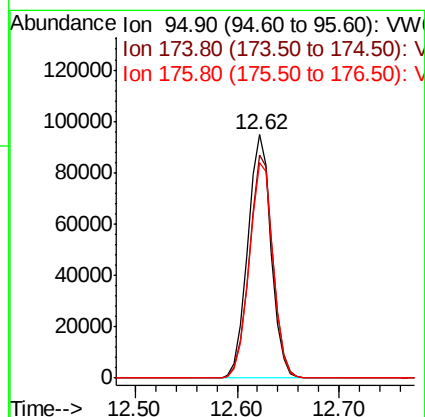





#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.63 min Scan# 1596
Delta R.T. 0.00 min
Lab File: VW005961.D
Acq: 10 Oct 2018 01:49




Instrument :
MSVOA_W
ClientSampled :
FL-PIT-1


Tgt Ion:117 Resp: 341859
Ion Ratio Lower Upper
117 100
82 52.0 43.5 65.3
119 32.9 25.4 38.2

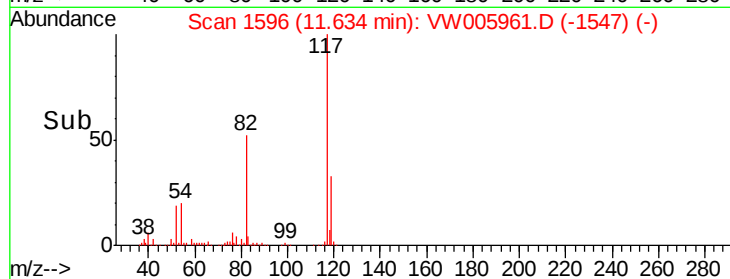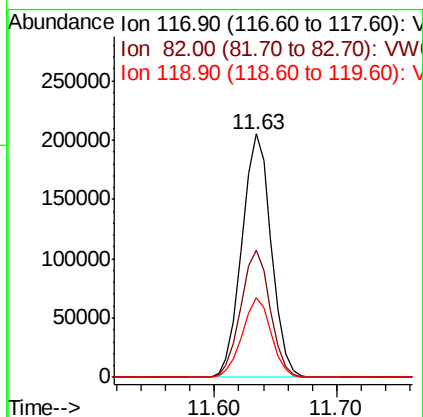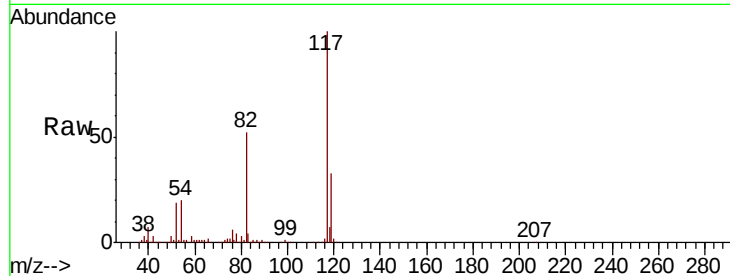

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.56 min Scan# 1912
Delta R.T. -0.01 min
Lab File: VW005961.D
Acq: 10 Oct 2018 01:49

Tgt Ion:152 Resp: 155379
Ion Ratio Lower Upper
152 100
115 55.9 28.3 85.0
150 158.4 0.0 349.2

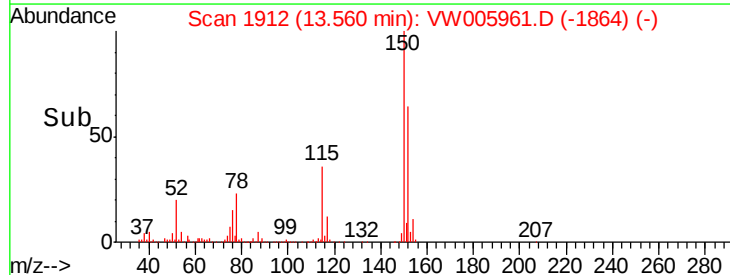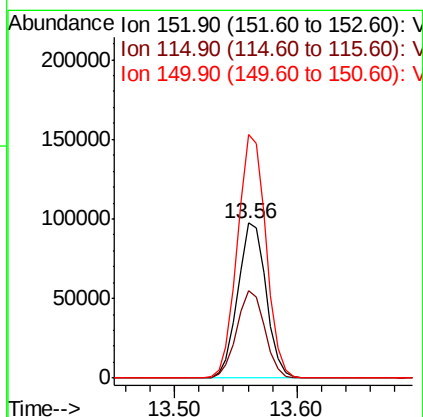



#76

1,2,3-Trichloropropane

Concen: 55.792 ug/l

RT: 12.62 min Scan# 1758

Delta R.T. -0.15 min

Lab File: VW005961.D

Acq: 10 Oct 2018 01:49

Instrument :

MSVOA_W

ClientSampled :





FL-PIT-1

Tgt Ion: 75 Resp: 77437

Ion Ratio Lower Upper

75 100

77 1.2 0.0 0.0#

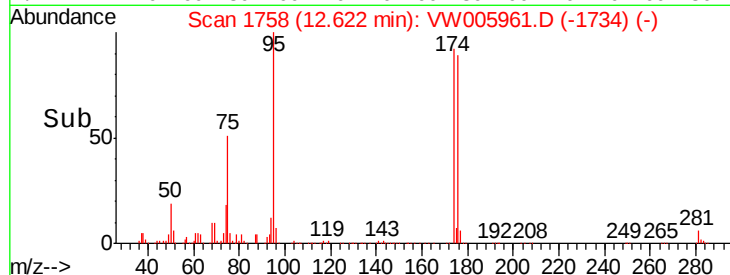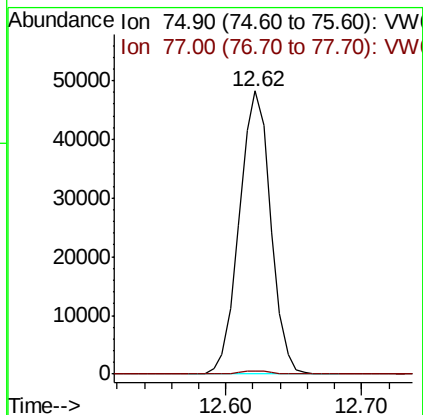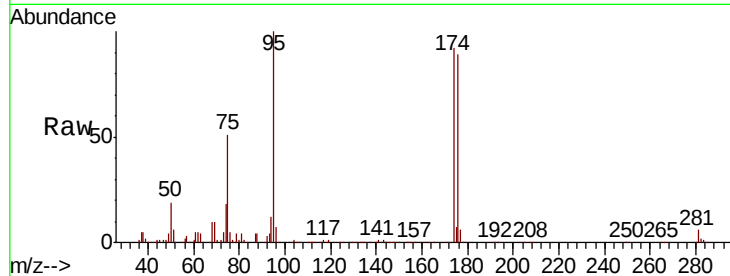

#81

trans-1,4-Dichloro-2-butene

Concen: 117.783 ug/l

RT: 12.62 min Scan# 1758

Delta R.T. 0.10 min

Lab File: VW005961.D

Acq: 10 Oct 2018 01:49

Tgt Ion: 75 Resp: 77437

Ion Ratio Lower Upper

75 100

53 0.0 76.5 114.7#

89 0.0 37.6 56.4#

