

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW101018\
 Data File : VW005953.D
 Acq On : 09 Oct 2018 22:22
 Operator : SY/AP
 Sample : J5200-07RE
 Misc : 6.22G/5ML/MSVOA W/SOIL
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 OR-03-100818-BRE

Quant Time: Oct 10 01:27:43 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W100818S.M
 Quant Title : SW846 8260
 QLast Update : Tue Oct 09 02:14:04 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.95	168	258956	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.85	114	367884	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.63	117	248209	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.57	152	128898	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.31	65	135243	53.80	ug/l	0.00
Spiked Amount 50.000			Recovery	=	107.60%	
35) Dibromofluoromethane	7.88	113	129270	55.04	ug/l	0.00
Spiked Amount 50.000			Recovery	=	110.08%	
50) Toluene-d8	10.33	98	259359	28.70	ug/l	0.00
Spiked Amount 50.000			Recovery	=	57.40%	
62) 4-Bromofluorobenzene	12.62	95	137617	40.03	ug/l	0.00
Spiked Amount 50.000			Recovery	=	80.06%	
Target Compounds						
20) Methylene Chloride	4.90	84	7178	2.853	ug/l #	Qvalue 87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW101018\
Data File : VW005953.D
Acq On : 09 Oct 2018 22:22
Operator : SY/AP
Sample : J5200-07RE
Misc : 6.22G/5ML/MSVOA W/SOIL
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
OR-03-100818-BRE

Quant Time: Oct 10 01:27:43 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\82W100818S.M
Quant Title : SW846 8260
QLast Update : Tue Oct 09 02:14:04 2018
Response via : Initial Calibration

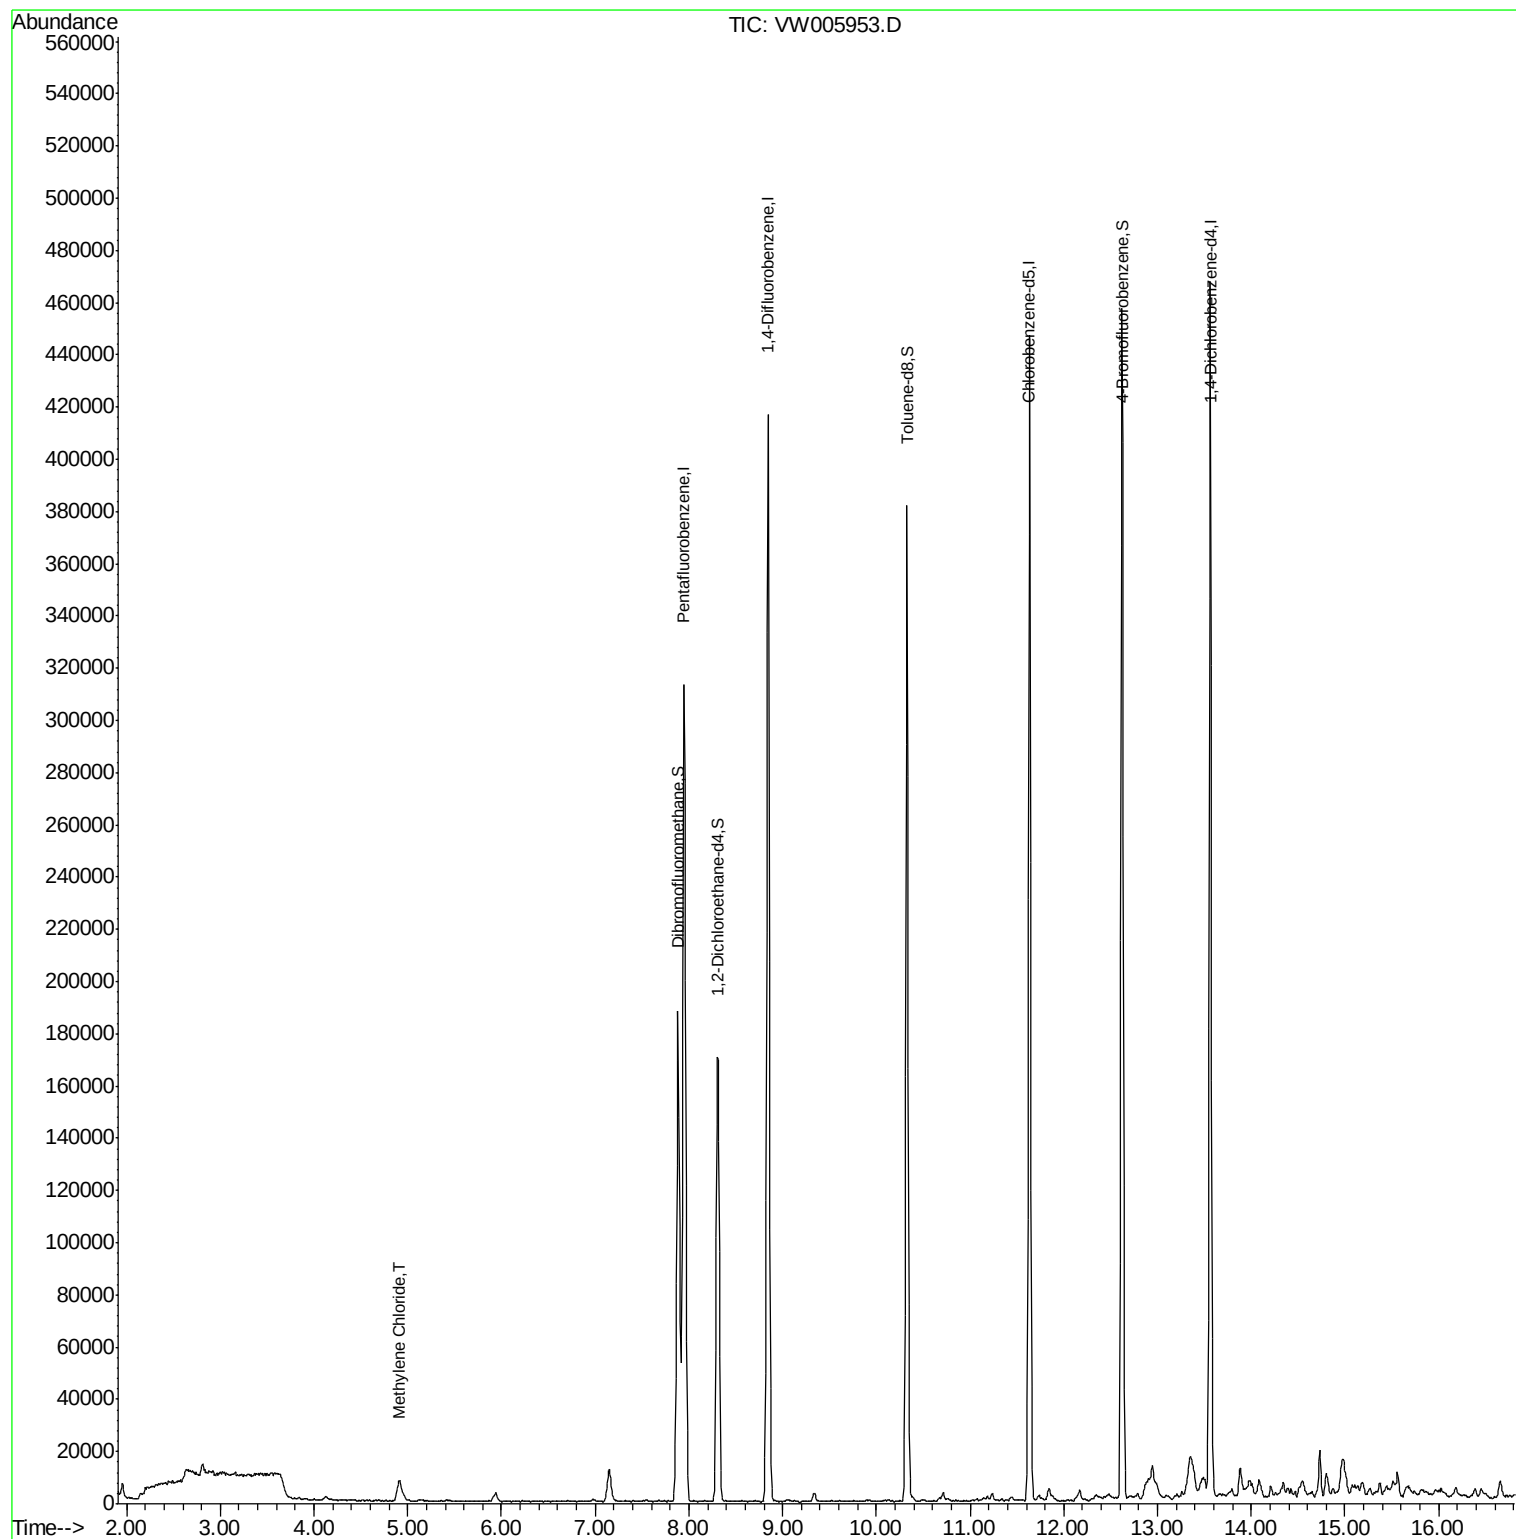

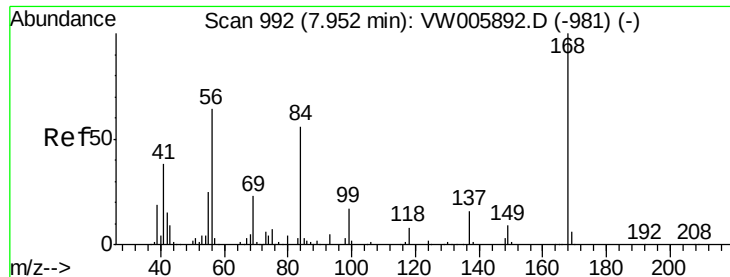

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.95 min Scan# 992

Delta R.T. -0.00 min

Lab File: VW005953.D

Acq: 09 Oct 2018 22:22

Instrument :

MSVOA_W

ClientSampleId :


OR-03-100818-BRE

Tot Ion:168 Resp: 258956

Ion Ratio Lower Upper

168 100

99 49.1 40.9 61.3

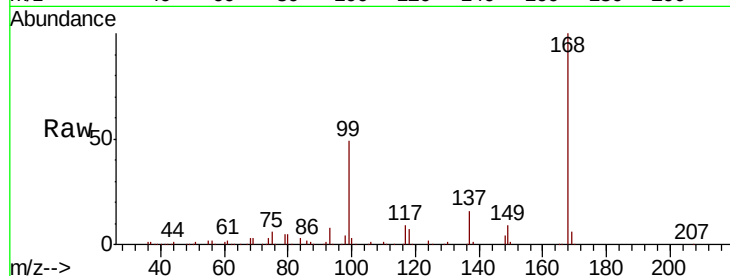

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VW



7.95

100000

50000

0

Time-->

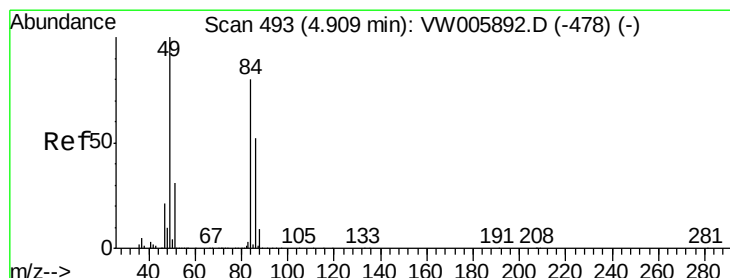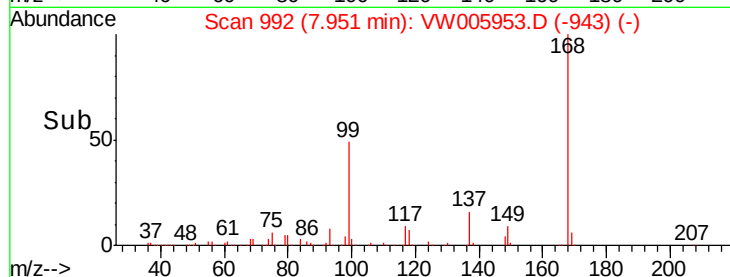

#20

Methylene Chloride

Concen: 2.853 ug/l

RT: 4.90 min Scan# 492

Delta R.T. -0.01 min

Lab File: VW005953.D

Acq: 09 Oct 2018 22:22

Tgt Ion: 84 Resp: 7178


Ion Ratio Lower Upper

84 100

49 106.1 99.9 149.9

51 30.4 31.1 46.7#

86 69.1 51.8 77.6

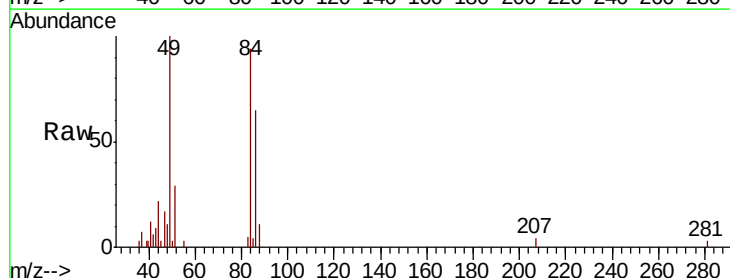

Abundance Ion 83.90 (83.60 to 84.60): VW

Ion 48.90 (48.60 to 49.60): VW

Ion 50.90 (50.60 to 51.60): VW

Ion 85.90 (85.60 to 86.60): VW

4.90


3000


2000

1000

0

Time-->




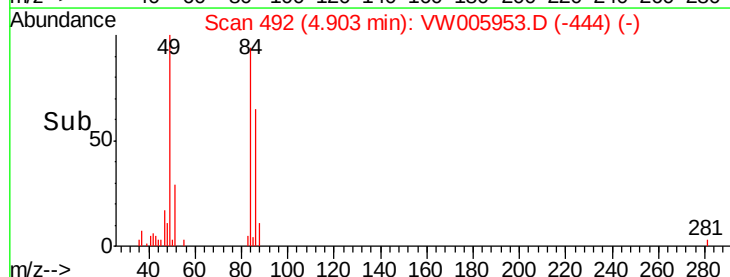


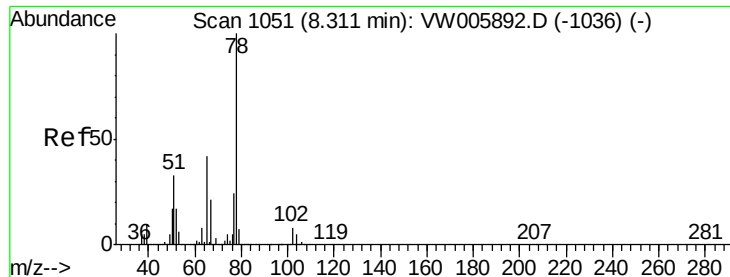

#33
 1,2-Dichloroethane-d4
 Concen: 53.798 ug/l
 RT: 8.31 min Scan# 1051
 Delta R.T. -0.00 min
 Lab File: VW005953.D
 Acq: 09 Oct 2018 22:22




Instrument :
 MSVOA_W
 ClientSampleId :
 OR-03-100818-BRE


Tot Ion: 65 Resp: 135243
 Ion Ratio Lower Upper
 65 100
 67 52.0 0.0 104.6

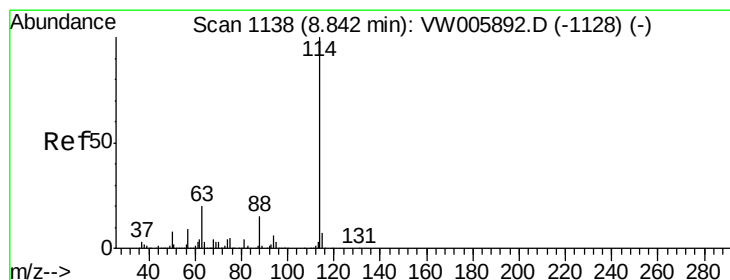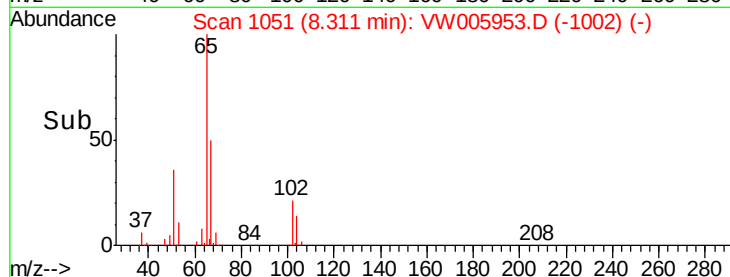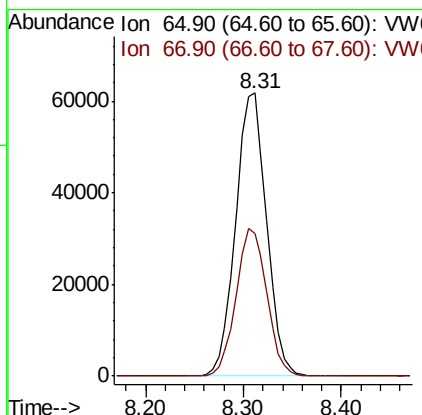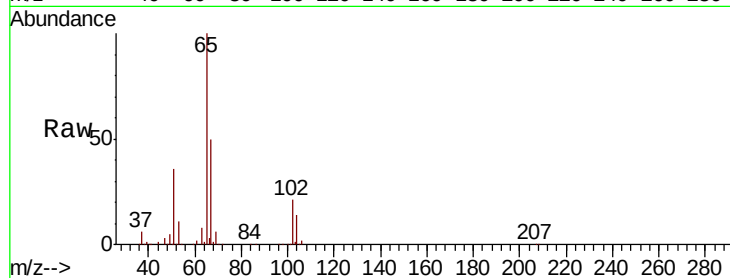

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.85 min Scan# 1139
 Delta R.T. 0.01 min
 Lab File: VW005953.D
 Acq: 09 Oct 2018 22:22

Tgt Ion: 114 Resp: 367884
 Ion Ratio Lower Upper
 114 100
 63 18.3 0.0 39.2
 88 14.8 0.0 30.8

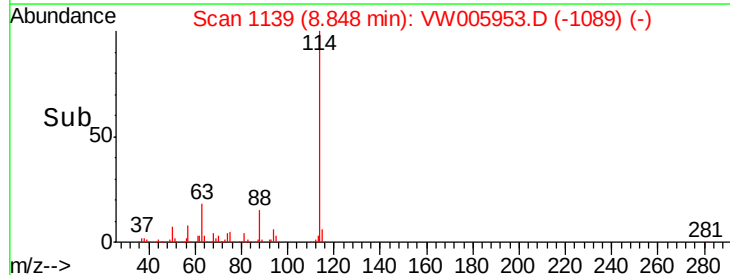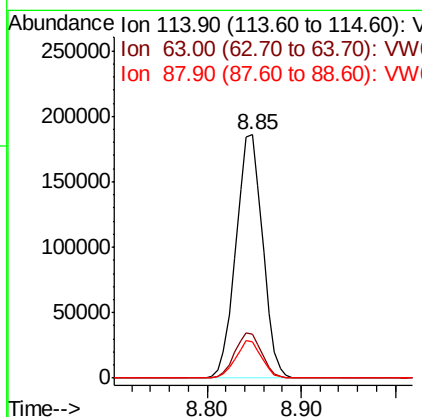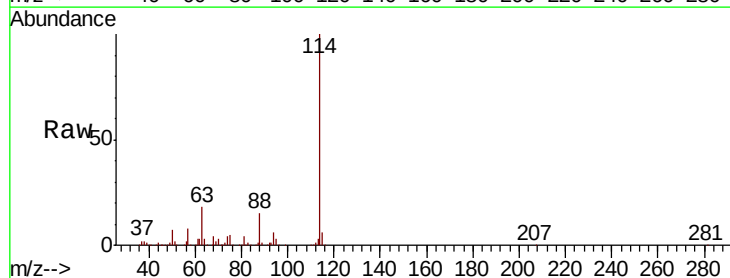


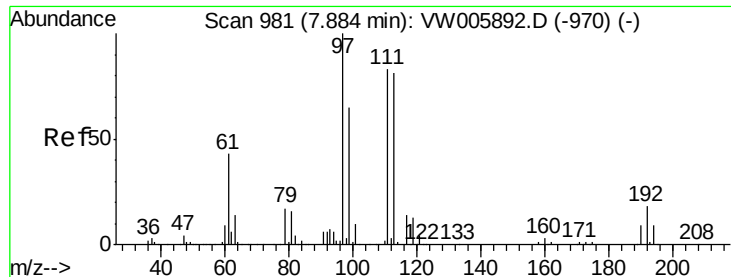




#35
 Dibromofluoromethane
 Concen: 55.037 ug/l
 RT: 7.88 min Scan# 981
 Delta R.T. -0.00 min
 Lab File: VW005953.D
 Acq: 09 Oct 2018 22:22

Instrument :
 MSVOA_W
 ClientSampleId :
 OR-03-100818-BRE

Tot Ion	Ratio	Lower	Upper
113	100		
111	102.9	82.0	123.0
192	22.3	18.3	27.5

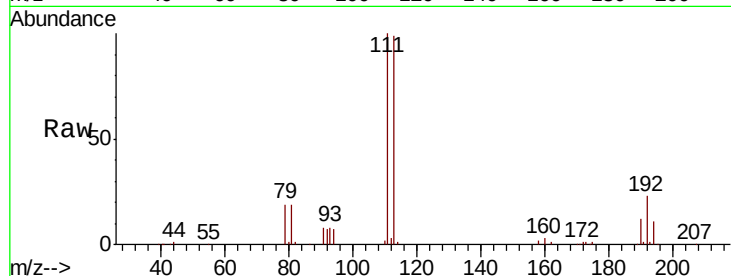


Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V

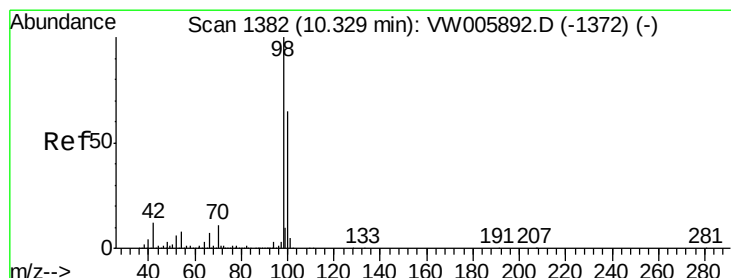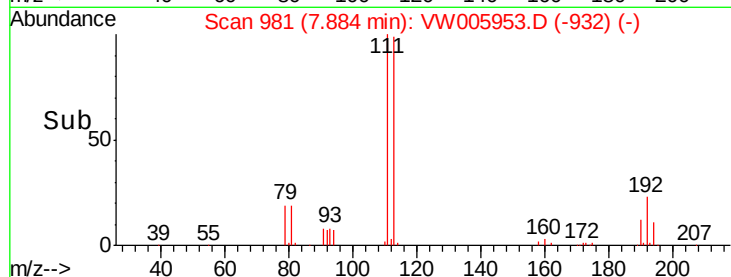
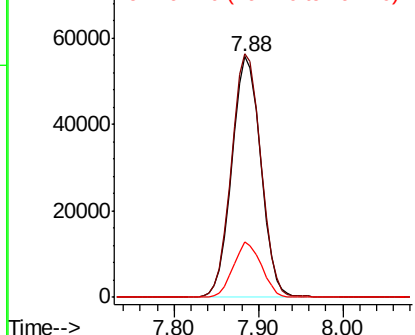



#50
 Toluene-d8
 Concen: 28.700 ug/l
 RT: 10.33 min Scan# 1382
 Delta R.T. -0.00 min
 Lab File: VW005953.D
 Acq: 09 Oct 2018 22:22

Tgt Ion	Ratio	Lower	Upper
98	100		
100	64.6	51.9	77.9

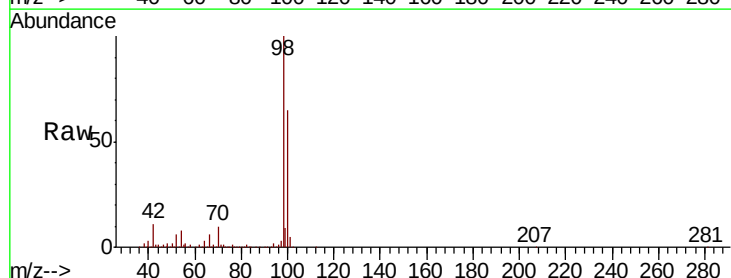

Abundance Ion 98.00 (97.70 to 98.70): VW
 Ion 100.00 (99.70 to 100.70): V

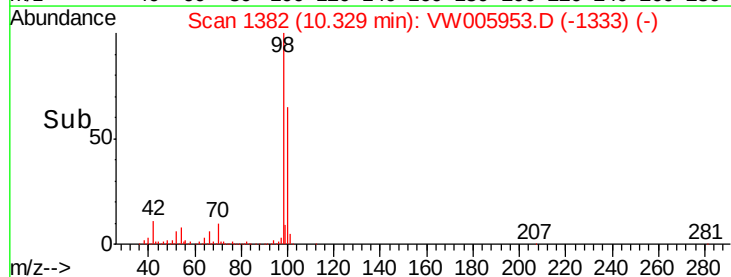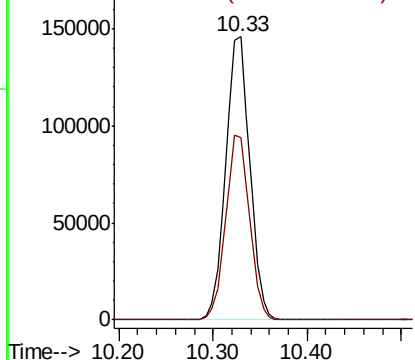

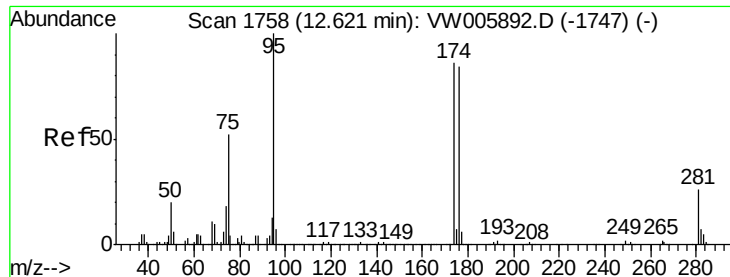

#62

4-Bromofluorobenzene

Concen: 40.026 ug/l

RT: 12.62 min Scan# 1758

Delta R.T. -0.00 min

Lab File: VW005953.D

Acq: 09 Oct 2018 22:22

Instrument :

MSVOA_W

ClientSampleId :

OR-03-100818-BRE


Tot Ion: 95 Resp: 137617

Ion Ratio Lower Upper




95 100

174 93.8 0.0 176.4

176 90.6 0.0 173.0

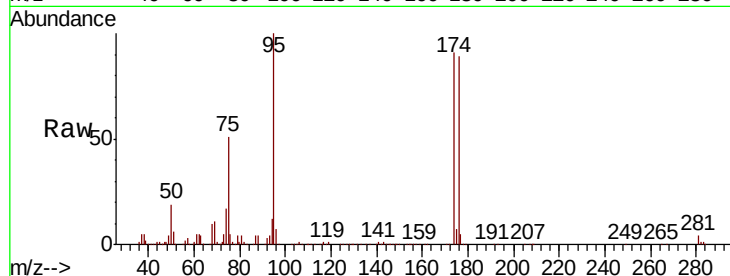

Abundance Ion 94.90 (94.60 to 95.60): VW
Ion 173.80 (173.50 to 174.50): VW
Ion 175.80 (175.50 to 176.50): VW

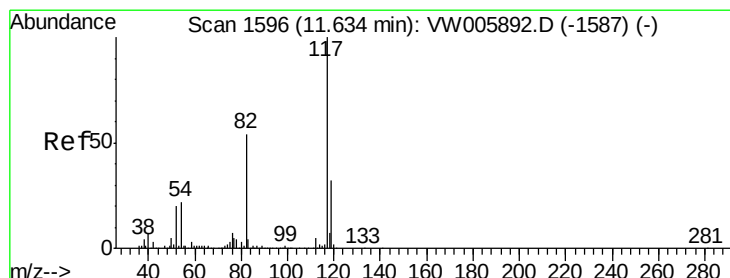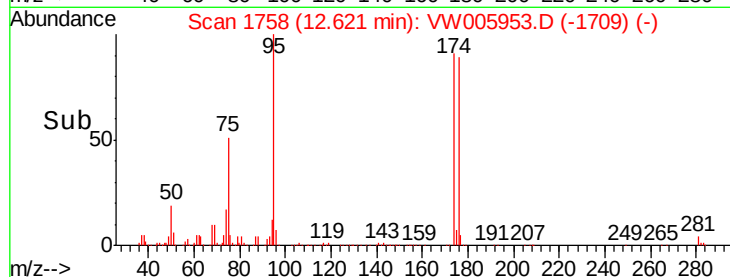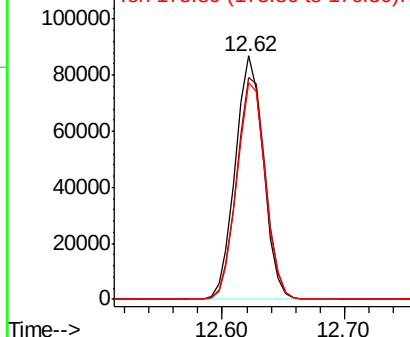

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.63 min Scan# 1596

Delta R.T. -0.00 min

Lab File: VW005953.D

Acq: 09 Oct 2018 22:22


Tgt Ion: 117 Resp: 248209

Ion Ratio Lower Upper



117 100


82 52.8 43.5 65.3

119 32.5 25.4 38.2

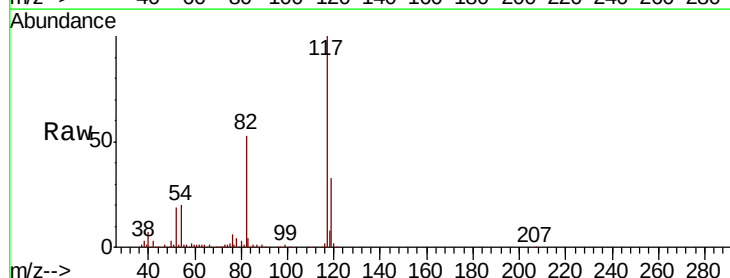

Abundance Ion 116.90 (116.60 to 117.60): VW
Ion 82.00 (81.70 to 82.70): VW
Ion 118.90 (118.60 to 119.60): VW

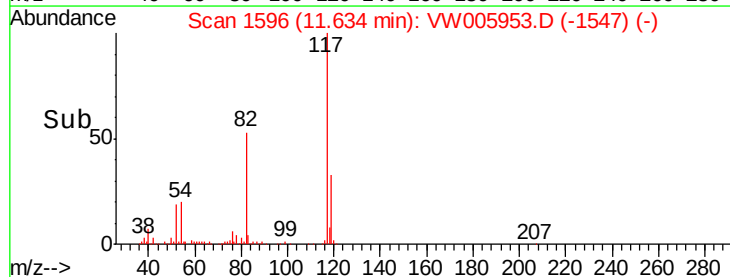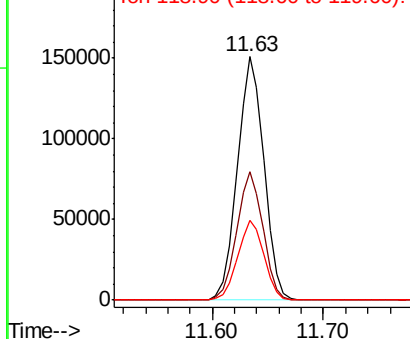

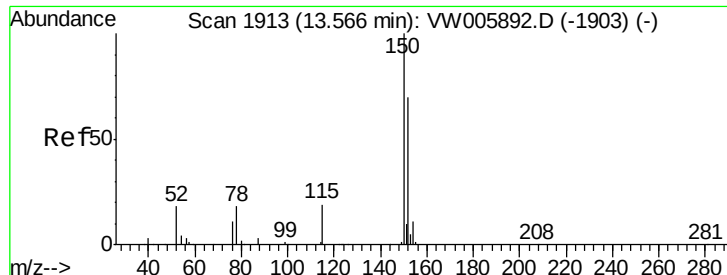

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.57 min Scan# 1913

Delta R.T. -0.00 min

Lab File: VW005953.D

Acq: 09 Oct 2018 22:22

Instrument :

MSVOA_W

ClientSampleId :

OR-03-100818-BRE


Tot Ion:152 Resp: 128898

Ion Ratio Lower Upper

152 100

115 54.4 28.3 85.0

150 154.7 0.0 349.2

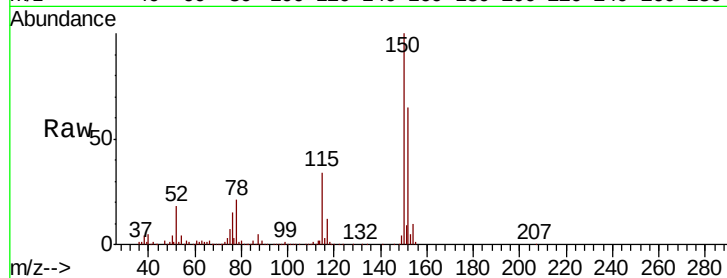

Abundance

Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

