


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW101018\
 Data File : VW005972.D
 Acq On : 10 Oct 2018 07:25
 Operator : SY/AP
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA W/SOIL
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W100818S.M
 Title : SW846 8260
 Last Update : Tue Oct 09 02:14:04 2018

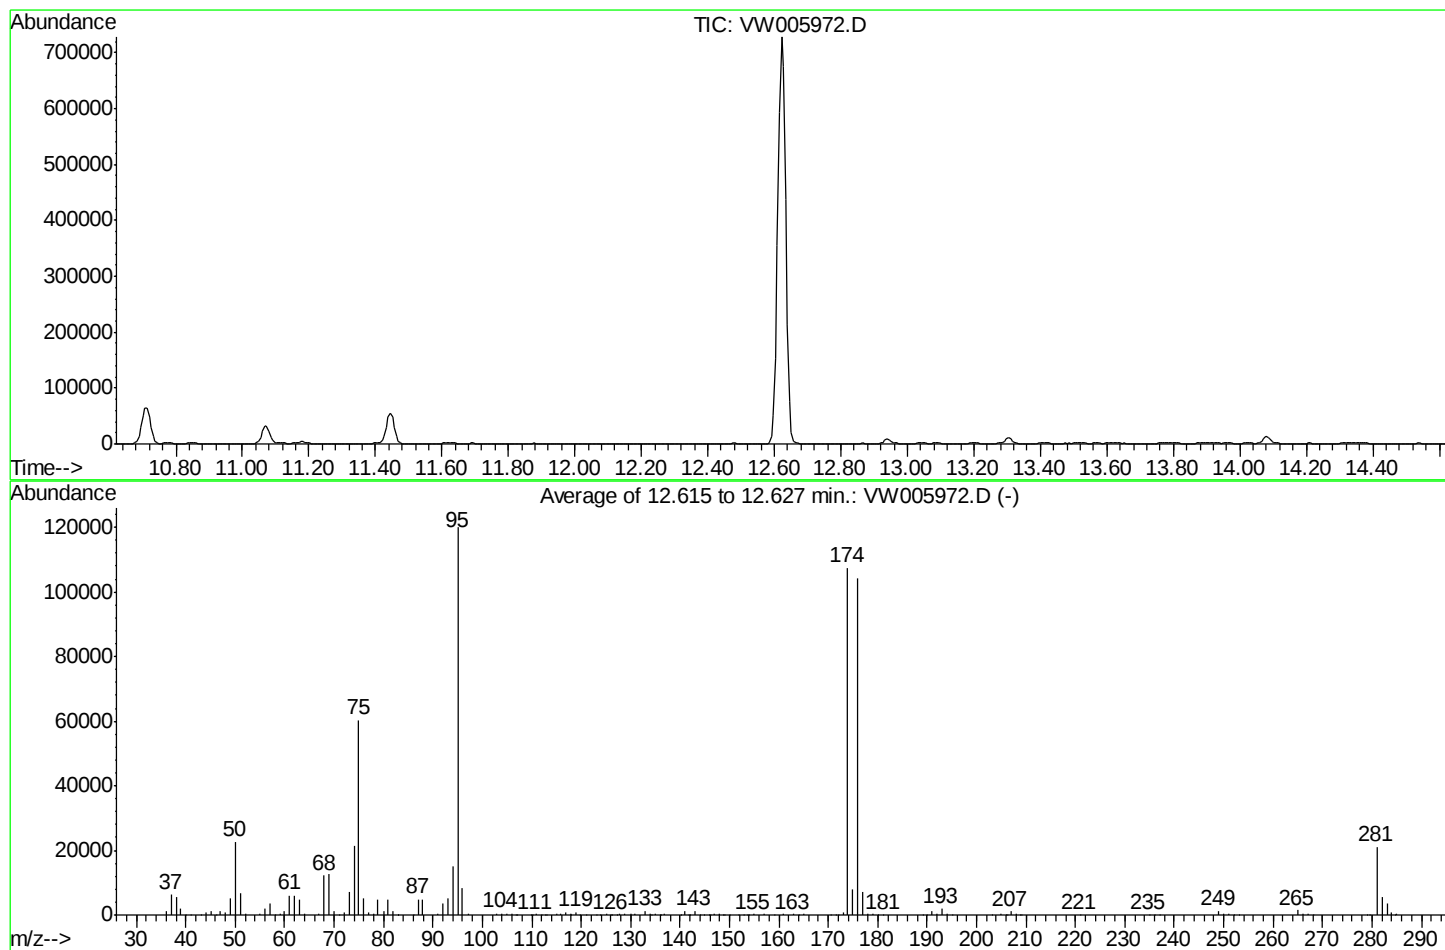

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.9	22656	PASS
75	95	30	60	50.3	60360	PASS
95	95	100	100	100.0	120013	PASS
96	95	5	9	7.1	8472	PASS
173	174	0.00	2	0.8	828	PASS
174	95	50	100	89.6	107554	PASS
175	174	5	9	7.5	8063	PASS
176	174	95	101	97.1	104386	PASS
177	176	5	9	7.0	7285	PASS