

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW101019\
 Data File : VW013529.D
 Acq On : 10 Oct 2019 20:03
 Operator : SY/VA
 Sample : K5267-09
 Misc : 6.49G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 11 09:03:54 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM101019S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Oct 11 07:46:37 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	406452	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	367365	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	171907	25.00	ug/L	0.00

System Monitoring Compounds


4) Vinyl Chloride-d3	2.35	65	84905	18.25	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	73.00%
7) Chloroethane-d5	2.89	69	74771	20.94	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	83.76%
10) 1,1-Dichloroethene-d2	4.01	63	137149	14.20	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	56.80%
20) 2-Butanone-d5	7.08	46	72370	51.65	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	103.30%
24) Chloroform-d	7.65	84	211918	24.00	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	96.00%
26) 1,2-Dichloroethane-d4	8.31	65	114816	25.10	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	100.40%
29) Benzene-d6	8.27	84	445106	22.62	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	90.48%
33) 1,2-Dichloropropane-d6	9.27	67	141317	24.21	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	96.84%
37) Toluene-d8	10.32	98	407365	21.81	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	87.24%
38) trans-1,3-Dichloropropene-	10.58	79	56309	21.65	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	86.60%
39) 2-Hexanone-d5	10.92	63	57204	48.98	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	97.96%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	114953	24.56	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	98.24%
61) 1,2-Dichlorobenzene-d4	13.85	152	150224	24.32	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	97.28%


Target Compounds					Ovalue
59) 1,2,3-Trichloropropane	13.55	75	17625	4.923 ug/L	91

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW101019\
Data File : VW013529.D
Acq On : 10 Oct 2019 20:03
Operator : SY/VA
Sample : K5267-09
Misc : 6.49G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 11 09:03:54 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM101019S.M
Quant Title : VOC Analysis
QLast Update : Fri Oct 11 07:46:37 2019
Response via : Initial Calibration

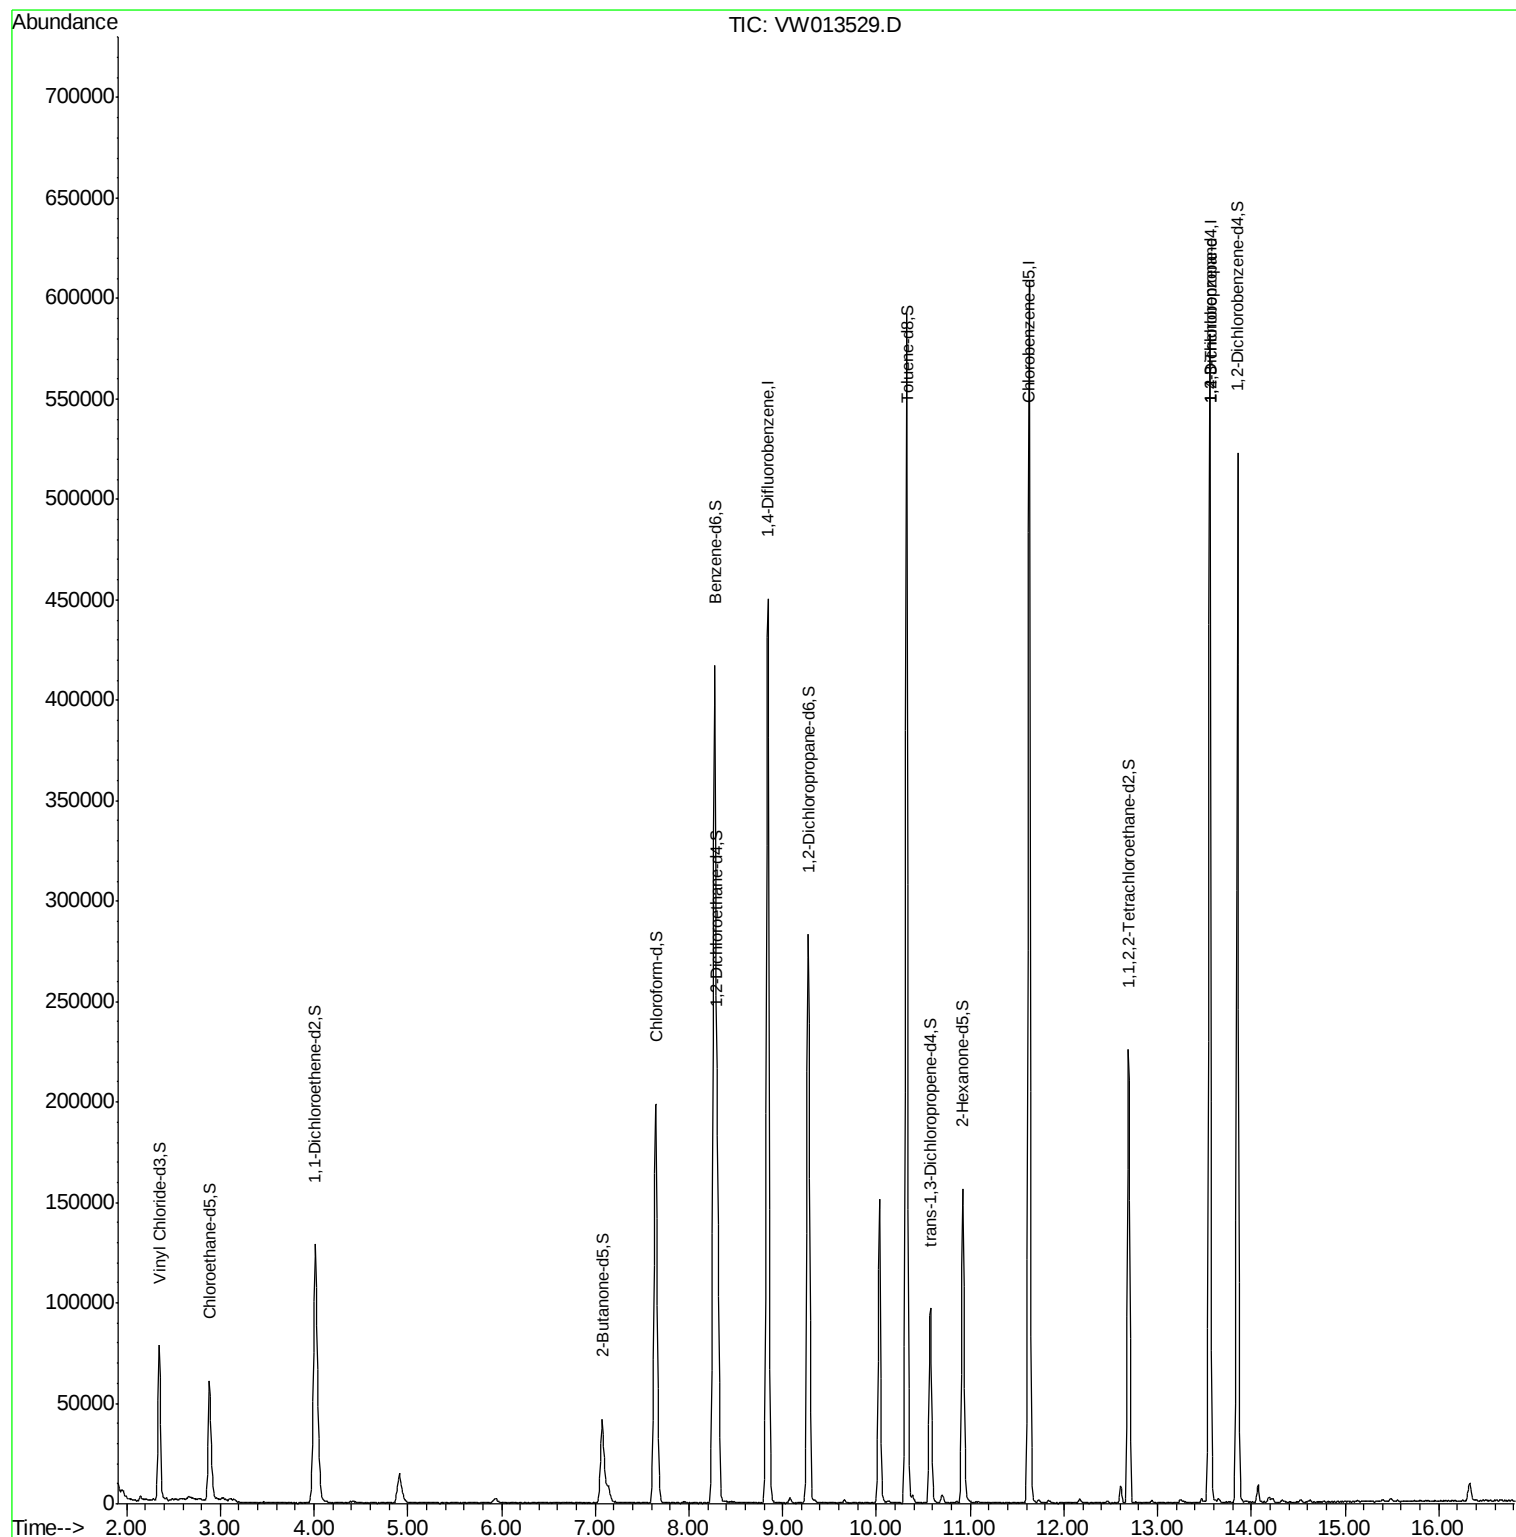

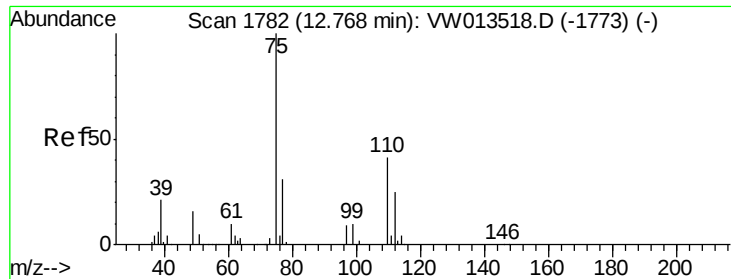

#59

1,2,3-Trichloropropane
 Concen: 4.923 ug/L
 RT: 13.55 min Scan# 1911
 Delta R.T. 0.79 min
 Lab File: VW013529.D
 Acq: 10 Oct 2019 20:03

Tot Ion: 75 Resp: 17625
 Ion Ratio Lower Upper
 75 100
 77 36.7 25.5 38.3

