


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW101020\
 Data File : VW016857.D
 Acq On : 09 Oct 2020 12:48
 Operator : SY/VA
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W101020S.M
 Title : SW846 8260
 Last Update : Sat Oct 10 05:14:48 2020

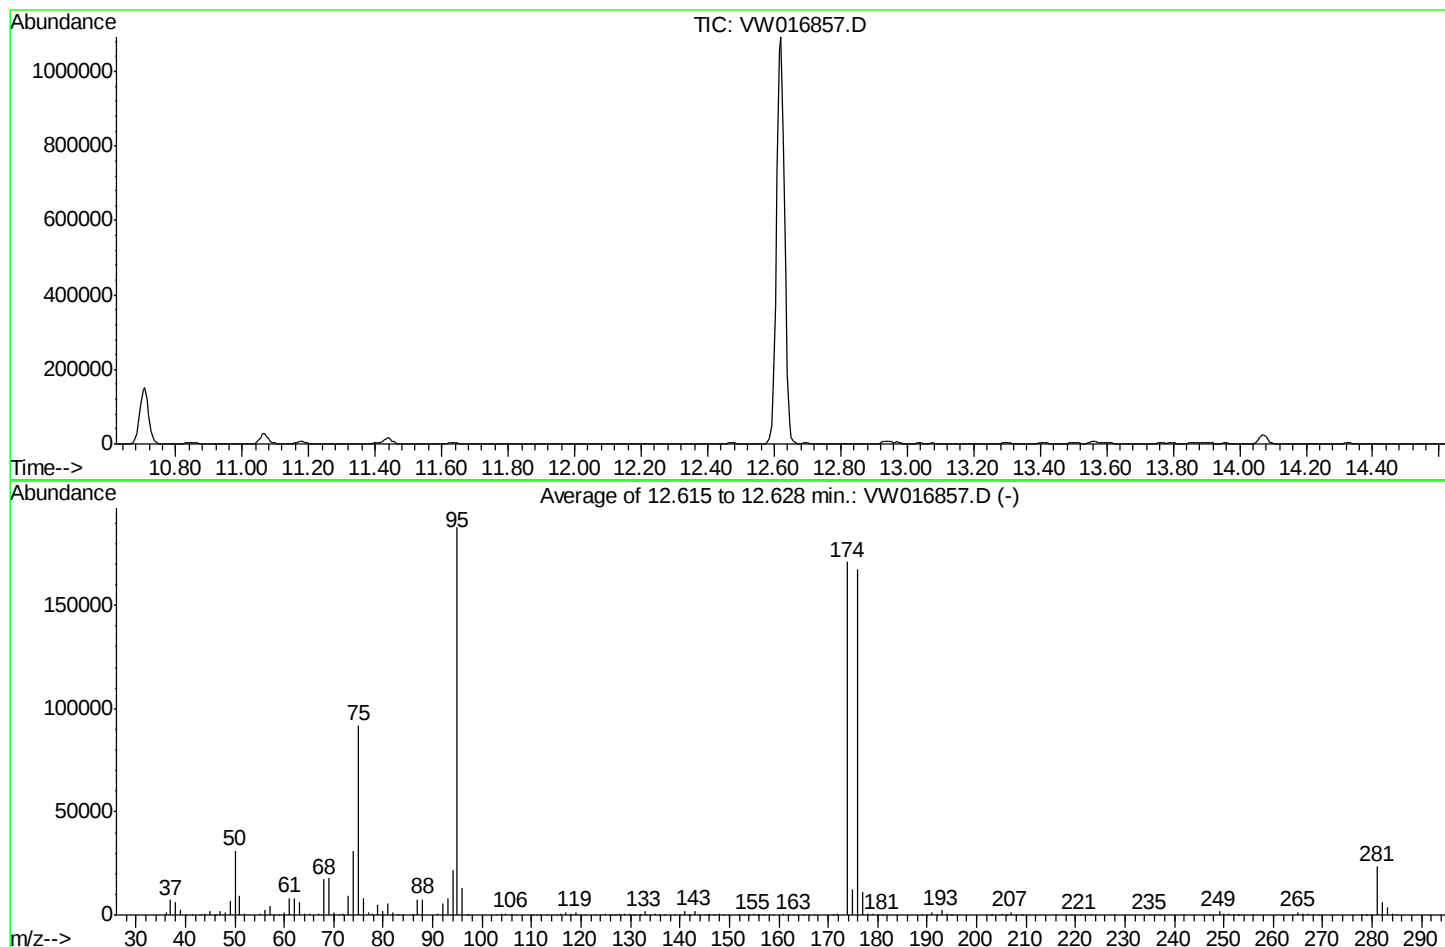

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1748

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.6	31234	PASS
75	95	30	60	48.7	91546	PASS
95	95	100	100	100.0	187861	PASS
96	95	5	9	6.9	13010	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	91.1	171093	PASS
175	174	5	9	7.4	12644	PASS
176	174	95	101	97.8	167296	PASS
177	176	5	9	6.7	11289	PASS