

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101024\
 Data File : VW030501.D
 Acq On : 10 Oct 2024 10:08
 Operator : SY/MD
 Sample : P4329-08
 Misc : 5.26g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Oct 11 01:20:46 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Oct 11 01:19:48 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.837	114	637576	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	607728	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	282616	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	222493	22.201	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	88.800%
7) Chloroethane-d5	2.893	69	177684	23.423	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	93.680%
11) 1,1-Dichloroethene-d2	4.015	65	88436	21.216	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	84.880%
21) 2-Butanone-d5	7.075	46	76930	42.655	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	85.320%
24) Chloroform-d	7.642	84	404842	22.203	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	88.800%
26) 1,2-Dichloroethane-d4	8.301	65	224624	23.691	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	94.760%
32) Benzene-d6	8.270	84	797634	22.613	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	90.440%
36) 1,2-Dichloropropane-d6	9.270	67	236855	22.878	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	91.520%
41) Toluene-d8	10.319	98	753039	23.386	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	93.560%
43) trans-1,3-Dichloroprop...	10.575	79	97826	22.566	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	90.280%
47) 2-Hexanone-d5	10.922	63	59583	44.684	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	89.360%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	164987	21.700	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	86.800%
66) 1,2-Dichlorobenzene-d4	13.849	152	228838	23.931	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	95.720%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.038	75	8417	0.565	ug/L	# 79


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101024\
Data File : VW030501.D
Acq On : 10 Oct 2024 10:08
Operator : SY/MD
Sample : P4329-08
Misc : 5.26g/10mL/MSVOA_W/SOIL/B
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Oct 11 01:20:46 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Oct 11 01:19:48 2024
Response via : Initial Calibration

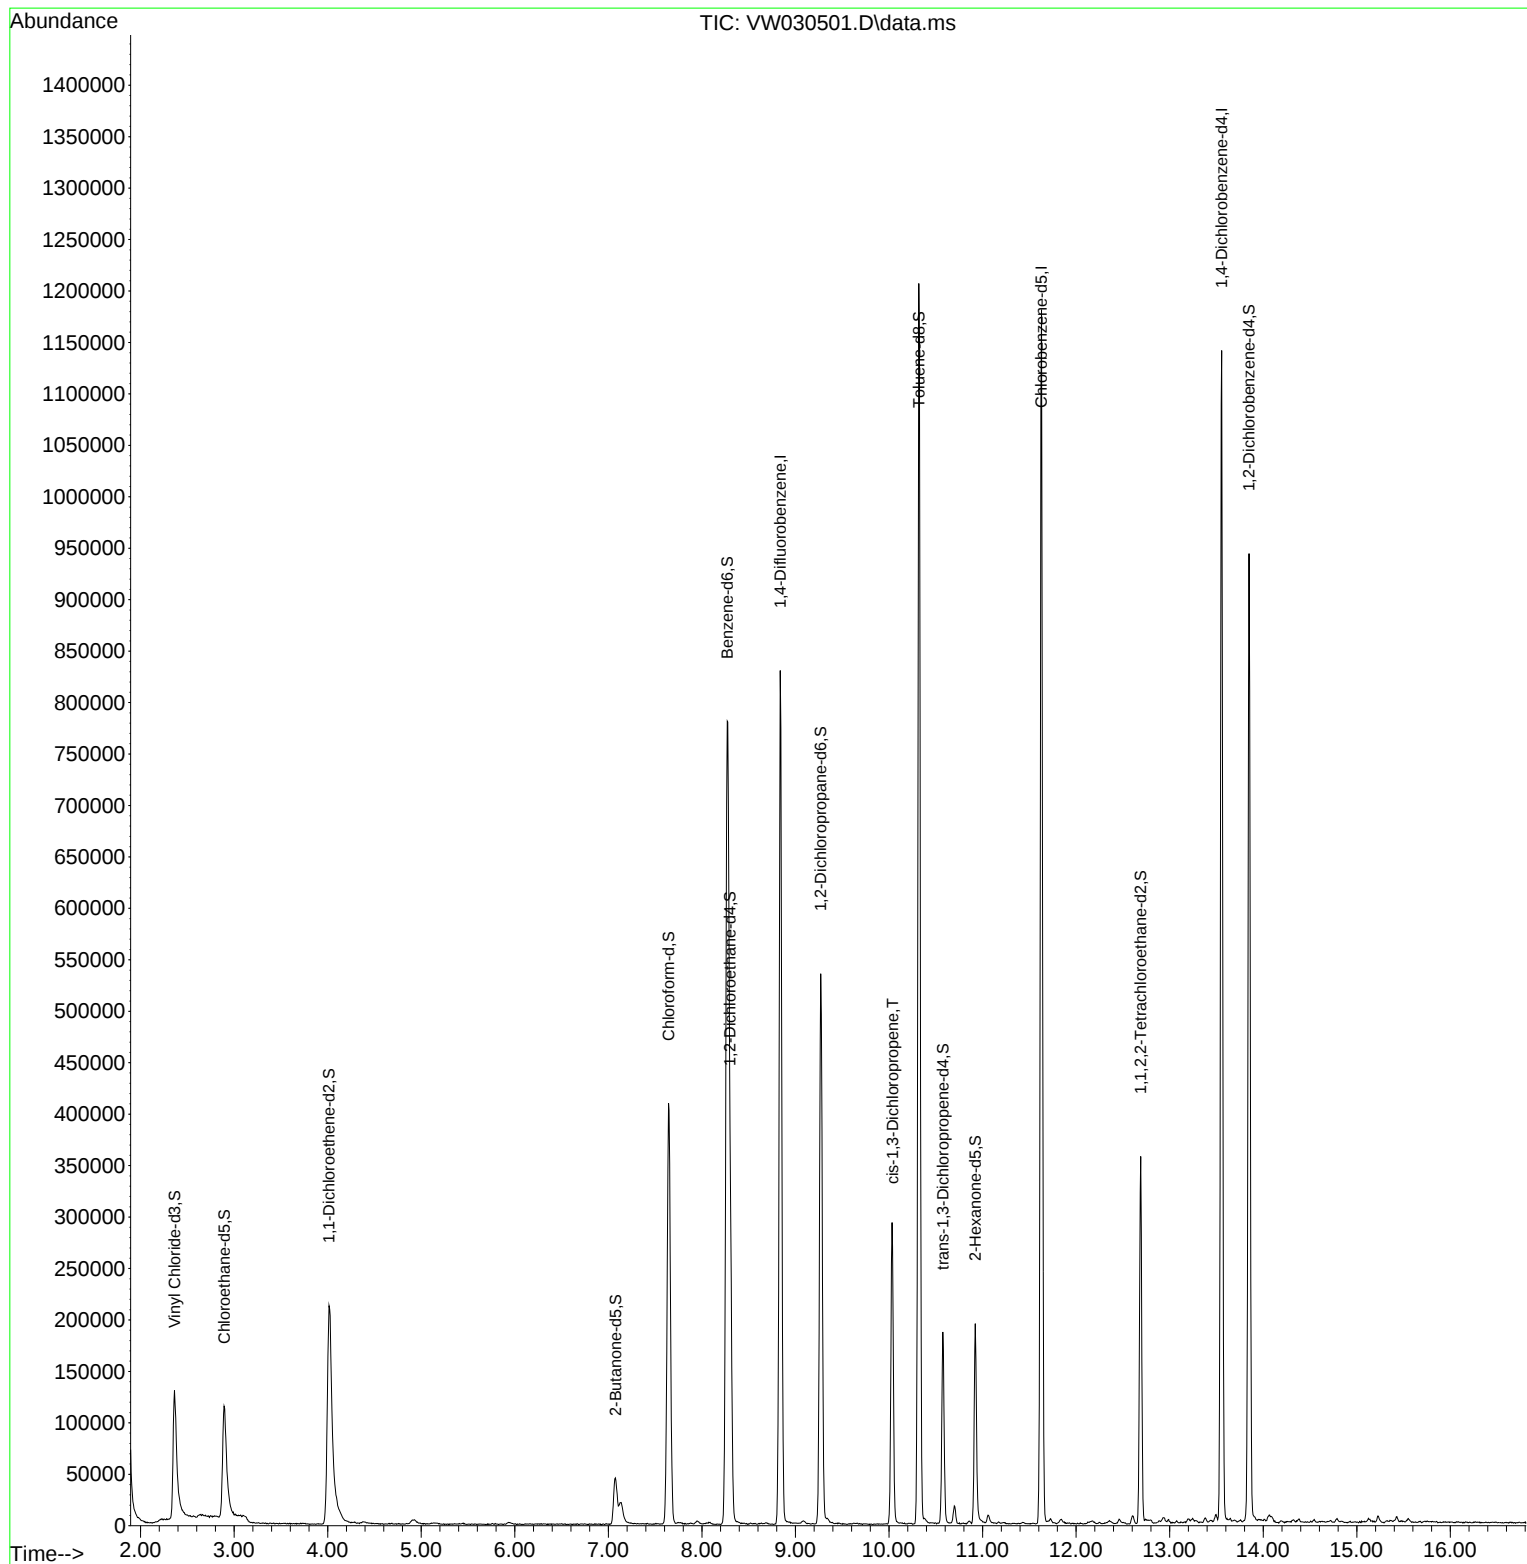

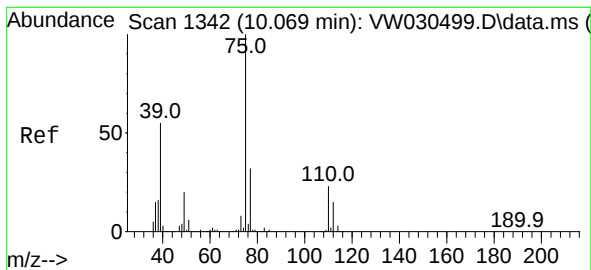

#39
 cis-1,3-Dichloropropene
 Concen: 0.565 ug/L
 RT: 10.038 min Scan# 14
 Delta R.T. -0.030 min
 Lab File: VW030501.D
 Acq: 10 Oct 2024 10:08

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion: 75 Resp: 8417
 Ion Ratio Lower Upper
 75 100
 77 41.7 21.1 39.1#

