

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101024\
 Data File : VW030526.D
 Acq On : 10 Oct 2024 22:41
 Operator : SY/MD
 Sample : P4351-04
 Misc : 5.73g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Oct 11 03:26:47 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Oct 11 02:35:02 2024
 Response via : Initial Calibration

Compound			R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards								
1) 1,4-Difluorobenzene			8.843	114	172809	25.000	ug/L	0.00
28) Chlorobenzene-d5			11.629	117	160371	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4			13.556	152	54410	25.000	ug/L	0.00
System Monitoring Compounds								
4) Vinyl Chloride-d3			2.357	65	81806	30.117	ug/L	-0.01
Spiked Amount 25.000			Range 30 - 150		Recovery = 120.480%			
7) Chloroethane-d5			2.893	69	72948	35.478	ug/L	-0.01
Spiked Amount 25.000			Range 30 - 150		Recovery = 141.920%			
11) 1,1-Dichloroethene-d2			4.021	65	32341	28.626	ug/L	0.00
Spiked Amount 25.000			Range 45 - 110		Recovery = 114.520%#			
21) 2-Butanone-d5			7.075	46	64131	131.193	ug/L	0.00
Spiked Amount 50.000			Range 20 - 135		Recovery = 262.380%#			
24) Chloroform-d			7.648	84	172662	34.938	ug/L	0.00
Spiked Amount 25.000			Range 40 - 150		Recovery = 139.760%			
26) 1,2-Dichloroethane-d4			8.307	65	116297	45.255	ug/L	0.00
Spiked Amount 25.000			Range 70 - 130		Recovery = 181.000%#			
32) Benzene-d6			8.270	84	310677	33.378	ug/L	0.00
Spiked Amount 25.000			Range 20 - 135		Recovery = 133.520%			
36) 1,2-Dichloropropane-d6			9.270	67	103532	37.897	ug/L	0.00
Spiked Amount 25.000			Range 70 - 120		Recovery = 151.600%#			
41) Toluene-d8			10.319	98	256098	30.140	ug/L	0.00
Spiked Amount 25.000			Range 30 - 130		Recovery = 120.560%			
43) trans-1,3-Dichloroprop...			10.575	79	42644	37.277	ug/L	0.00
Spiked Amount 25.000			Range 30 - 135		Recovery = 149.120%#			
47) 2-Hexanone-d5			10.922	63	42763	121.529	ug/L	0.00
Spiked Amount 50.000			Range 20 - 135		Recovery = 243.060%#			
56) 1,1,2,2-Tetrachloroeth...			12.690	84	88750	44.235	ug/L	0.00
Spiked Amount 25.000			Range 45 - 120		Recovery = 176.920%#			
66) 1,2-Dichlorobenzene-d4			13.855	152	66391	36.062	ug/L	0.00
Spiked Amount 25.000			Range 75 - 120		Recovery = 144.240%#			
Target Compounds								
39) cis-1,3-Dichloropropene			10.032	75	3628	0.923	ug/L	Qvalue 85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101024\
Data File : VW030526.D
Acq On : 10 Oct 2024 22:41
Operator : SY/MD
Sample : P4351-04
Misc : 5.73g/10mL/MSVOA_W/SOIL/A
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Oct 11 03:26:47 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Oct 11 02:35:02 2024
Response via : Initial Calibration

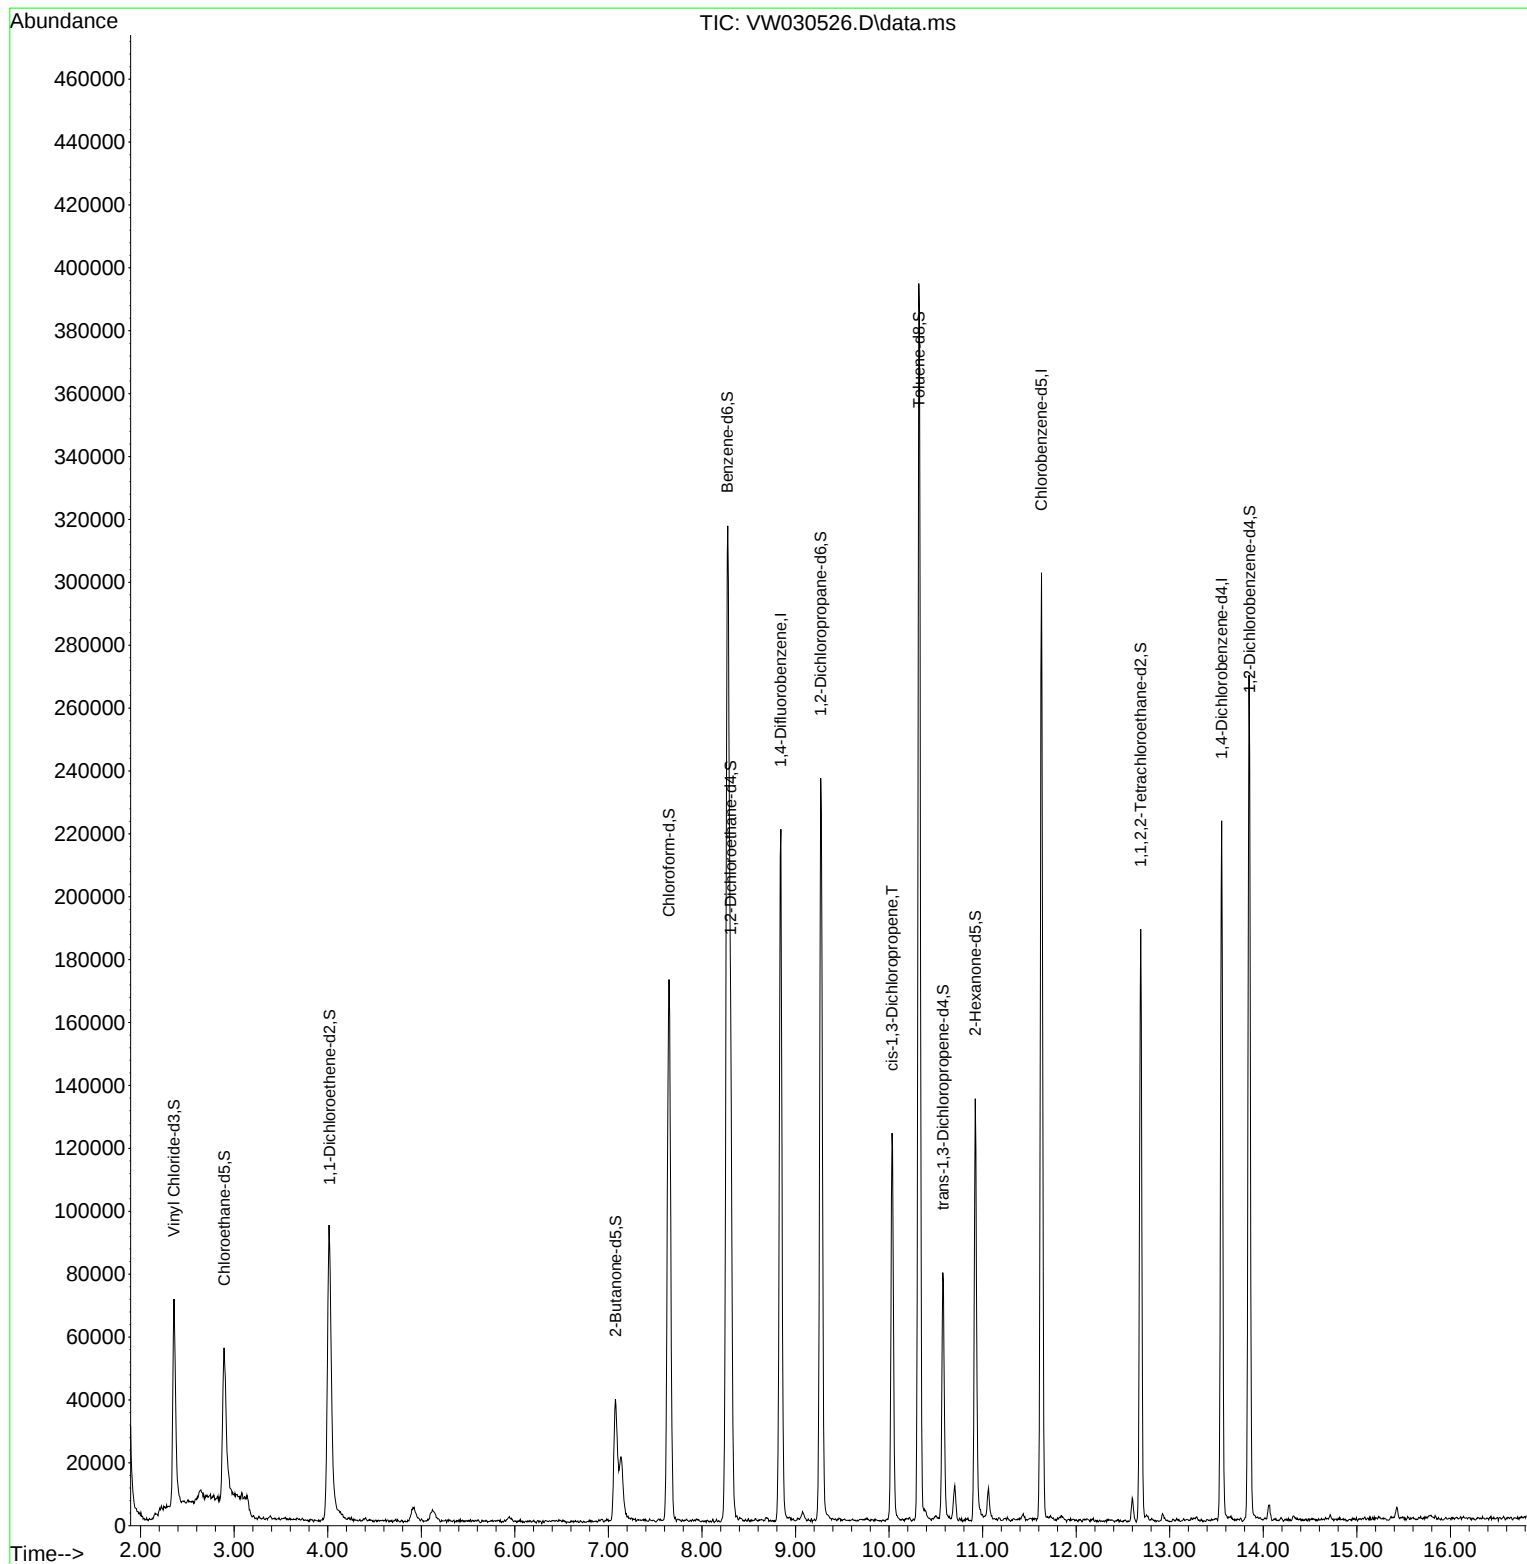

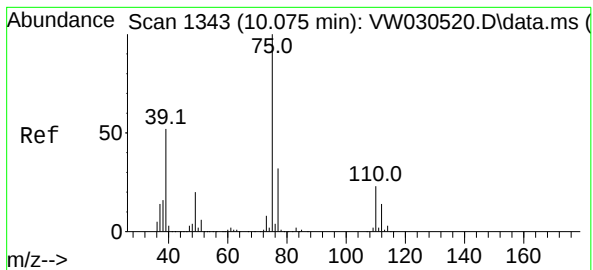

#39
 cis-1,3-Dichloropropene
 Concen: 0.923 ug/L
 RT: 10.032 min Scan# 14
 Delta R.T. -0.043 min
 Lab File: VW030526.D
 Acq: 10 Oct 2024 22:41

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion:	75	Resp:	3628
Ion Ratio	Lower	Upper	
75	100		
77	38.3	21.1	39.1

