




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101024\
 Data File : VW030504.D
 Acq On : 10 Oct 2024 12:41
 Operator : SY/MD
 Sample : P4346-03
 Misc : 3.70g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EOAW5

Manual IntegrationsAPPROVED

Quant Time: Oct 11 01:21:22 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Oct 11 01:19:48 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 10/15/2024
 Supervised By :Semsettin Yesilyurt 10/15/2024

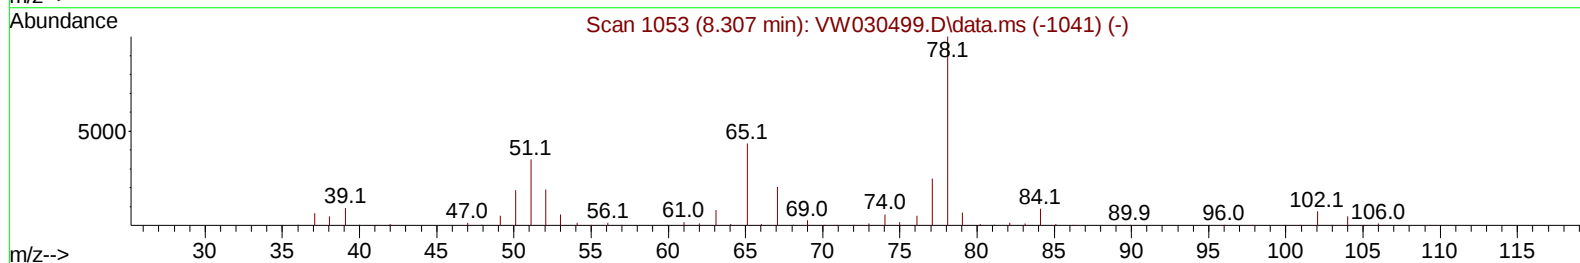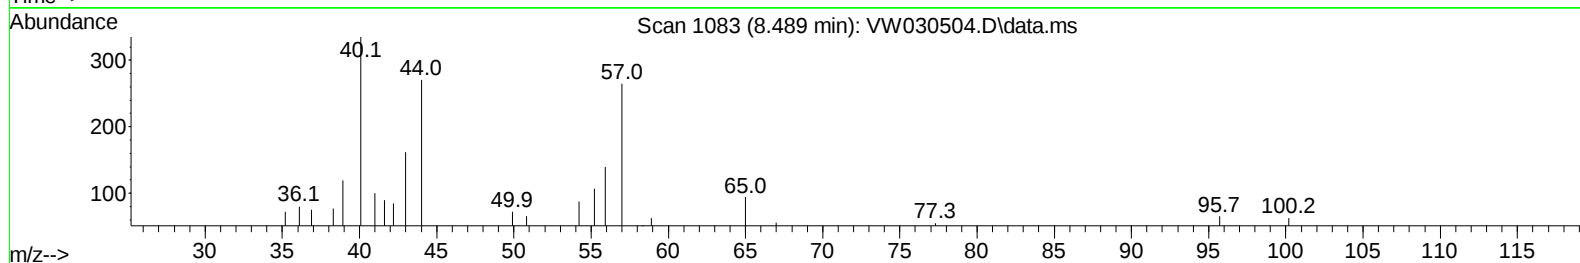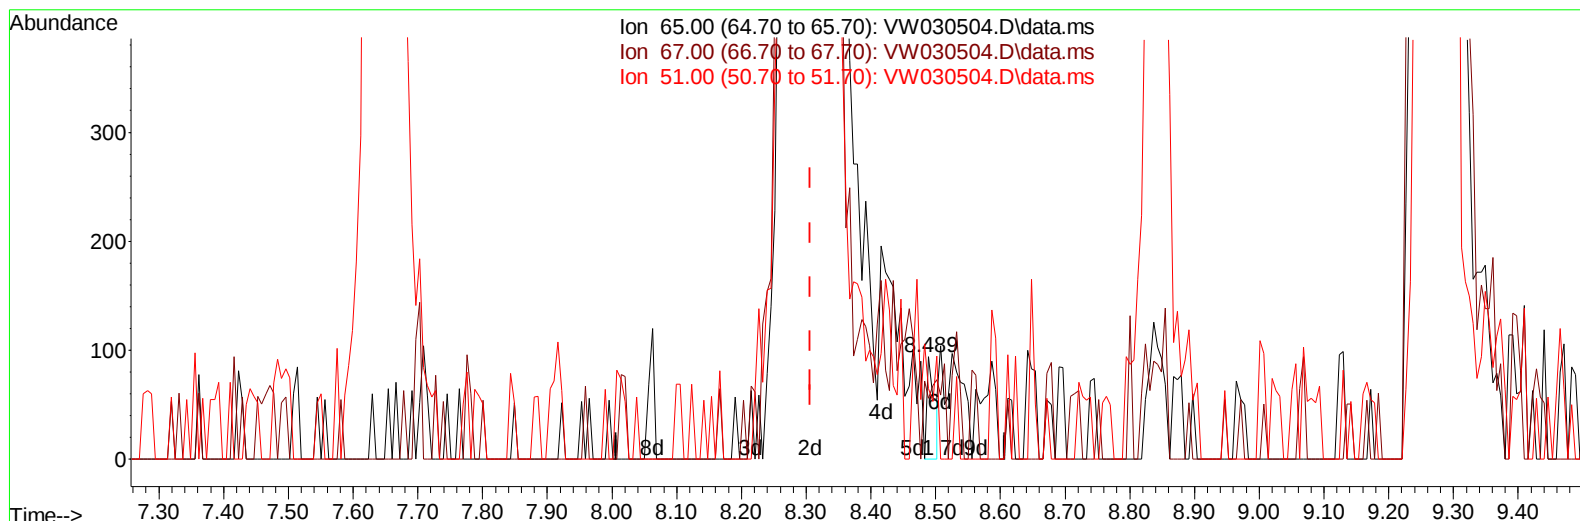

TIC: VW030504.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.489min (+ 0.183) 0.06 ug/L

response 75

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.90	62.67
51.00	109.40	109.33
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101024\
 Data File : VW030504.D
 Acq On : 10 Oct 2024 12:41
 Operator : SY/MD
 Sample : P4346-03
 Misc : 3.70g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EOAW5

Manual IntegrationsAPPROVED

Quant Time: Oct 11 01:21:22 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Oct 11 01:19:48 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 10/15/2024
 Supervised By :Semsettin Yesilyurt 10/15/2024

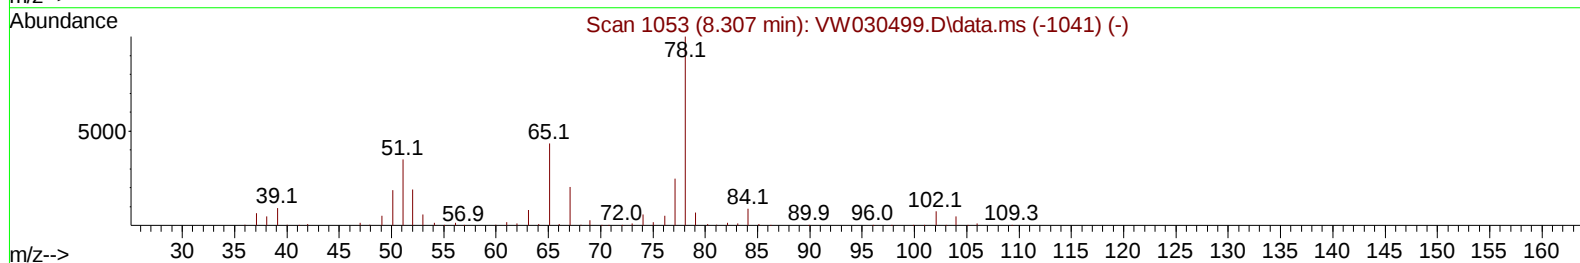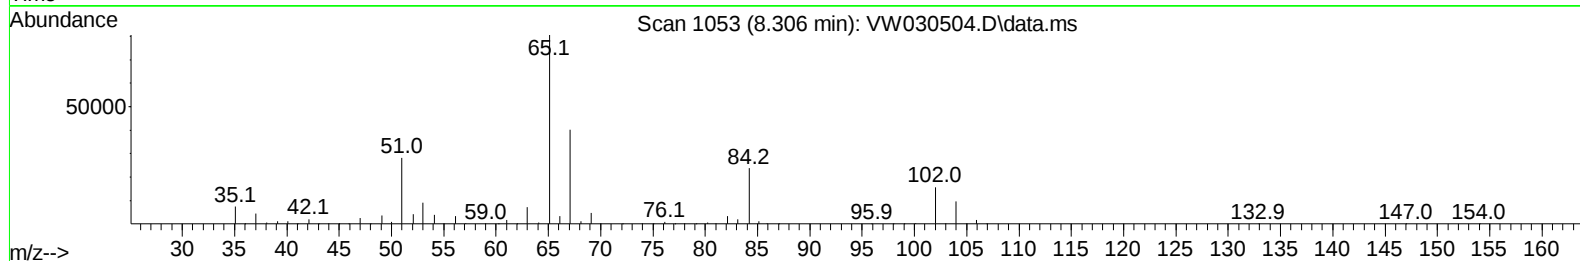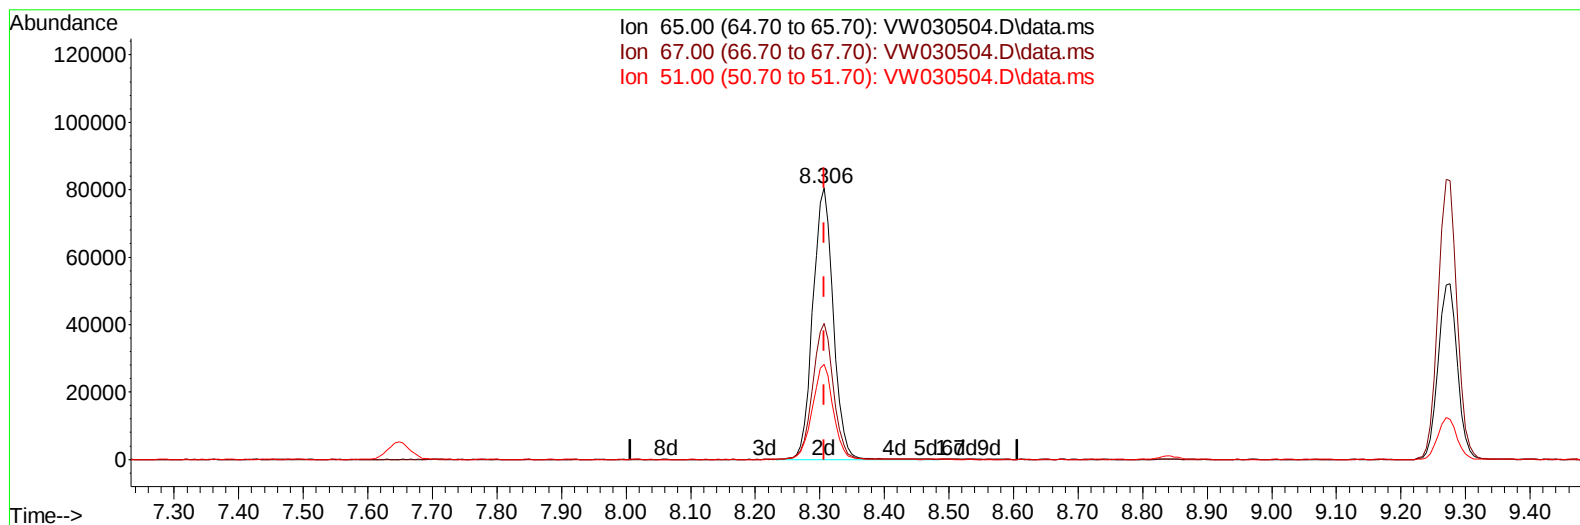

TIC: VW030504.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.306min (-0.000) 139.49 ug/L m

response 176910

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.90	0.03#
51.00	109.40	0.05#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\Vw101024\
 Data File : VW030504.D
 Acq On : 10 Oct 2024 12:41
 Operator : SY/MD
 Sample : P4346-03
 Misc : 3.70g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EOAW5

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 10/15/2024
 Supervised By :Semsettin Yesilyurt 10/15/2024

Quant Time: Oct 11 01:21:22 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Oct 11 01:19:48 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		85284	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		34763	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.555	152		6889	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.362	65		172459	128.649	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	= 514.600%#		
7) Chloroethane-d5	2.899	69		132873	130.944	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	= 523.760%#		
11) 1,1-Dichloroethene-d2	4.021	65		66927	120.035	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	= 480.120%#		
21) 2-Butanone-d5	7.075	46		77570	321.539	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	= 643.080%#		
24) Chloroform-d	7.648	84		292612	119.975	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	= 479.880%#		
26) 1,2-Dichloroethane-d4	8.306	65		176910m	139.491	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	= 557.960%#		
32) Benzene-d6	8.276	84		553786	274.472	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	= 1097.880%#		
36) 1,2-Dichloropropane-d6	9.270	67		168805	285.049	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	= 1140.200%#		
41) Toluene-d8	10.324	98		477842	259.432	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	= 1037.720%#		
43) trans-1,3-Dichloroprop...	10.574	79		70978	286.232	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	= 1144.920%#		
47) 2-Hexanone-d5	10.922	63		61265	803.217	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	= 1606.440%#		
56) 1,1,2,2-Tetrachloroeth...	12.690	84		132560	304.800	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	= 1219.200%#		
66) 1,2-Dichlorobenzene-d4	13.854	152		123687	530.629	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	= 2122.520%#		
Target Compounds							
13) Acetone	4.124	43		9714	27.504	ug/L	Qvalue 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101024\
Data File : VW030504.D
Acq On : 10 Oct 2024 12:41
Operator : SY/MD
Sample : P4346-03
Misc : 3.70g/10mL/MSVOA_W/SOIL/B
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EOAW5

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 10/15/2024
Supervised By :Semsettin Yesilyurt 10/15/2024

Quant Time: Oct 11 01:21:22 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Oct 11 01:19:48 2024
Response via : Initial Calibration

