




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101024\
Data File : VW030509.D
Acq On : 10 Oct 2024 14:42
Operator : SY/MD
Sample : P4346-11RE
Misc : 3.26g/10mL/MSVOA_W/SOIL/B
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EOAX1RE

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 10/15/2024
Supervised By :Semsettin Yesilyurt 10/15/2024

Quant Time: Oct 11 01:22:32 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Oct 11 01:19:48 2024
Response via : Initial Calibration

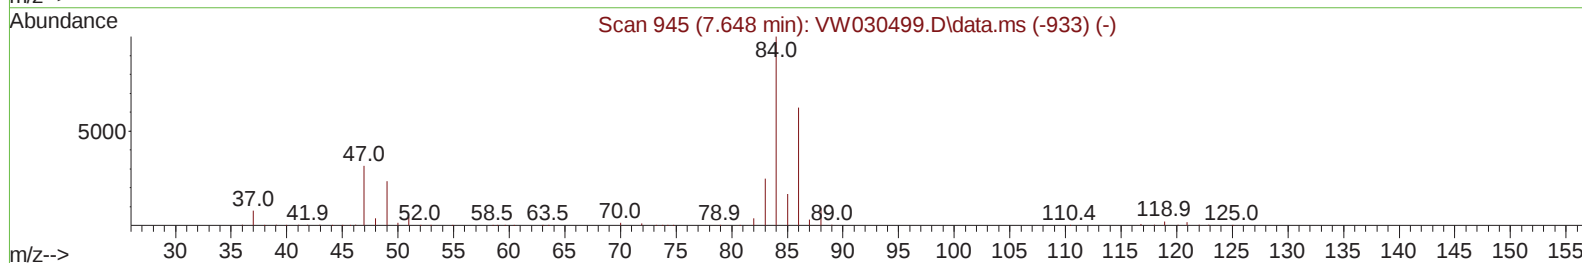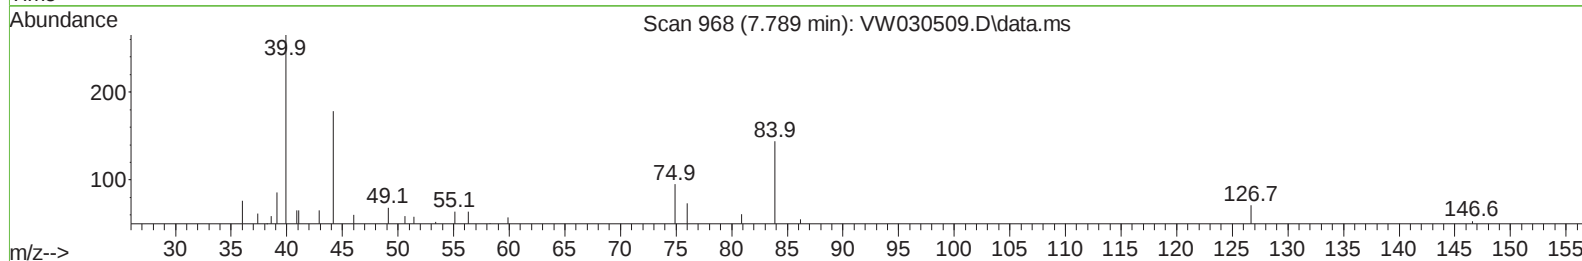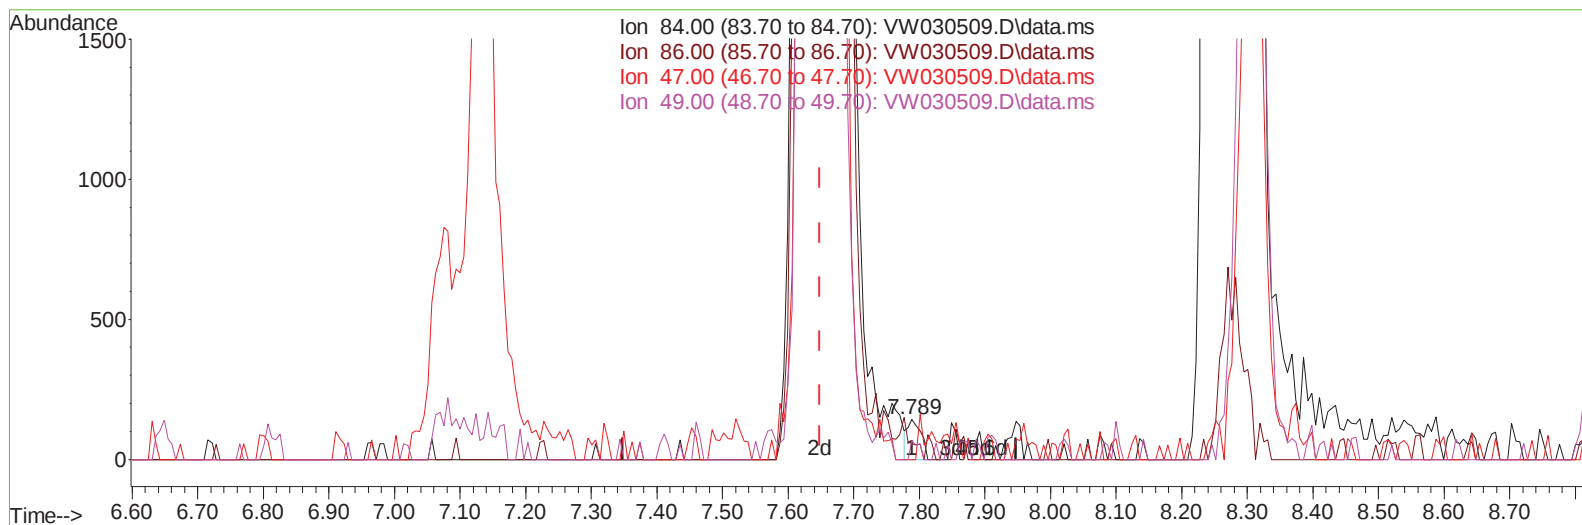

TIC: VW030509.D\data.ms

(24) Chloroform-d (S)

7.789min (+ 0.140) 0.03 ug/L

response 203

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	63.10	73.40
47.00	48.90	38.42
49.00	28.60	31.53




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101024\
Data File : VW030509.D
Acq On : 10 Oct 2024 14:42
Operator : SY/MD
Sample : P4346-11RE
Misc : 3.26g/10mL/MSVOA_W/SOIL/B
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EOAX1RE

Manual IntegrationsAPPROVED

Quant Time: Oct 11 01:22:32 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Oct 11 01:19:48 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 10/15/2024
Supervised By :Semsettin Yesilyurt 10/15/2024

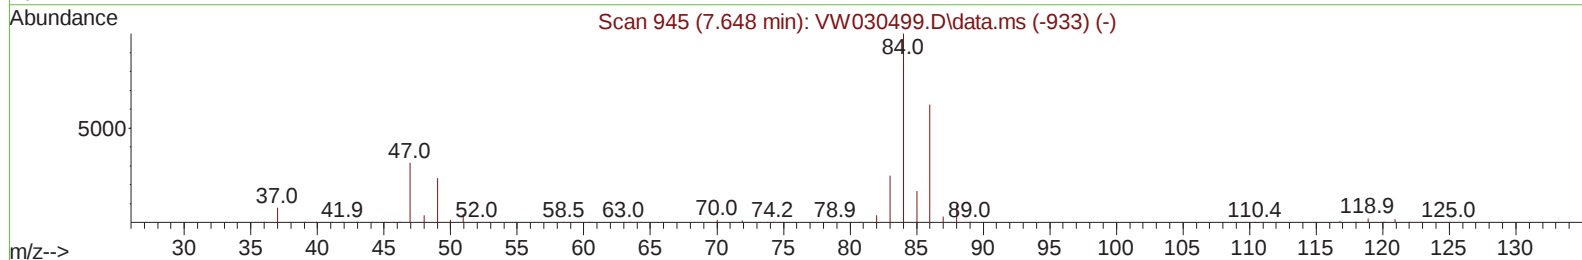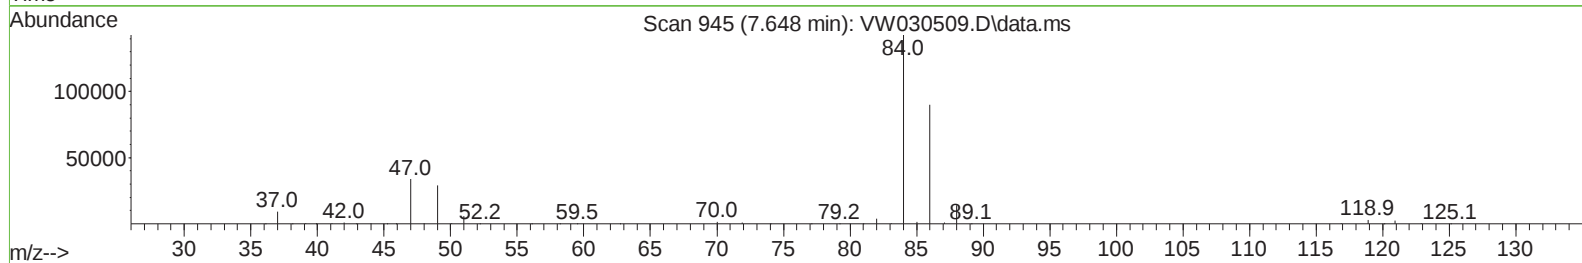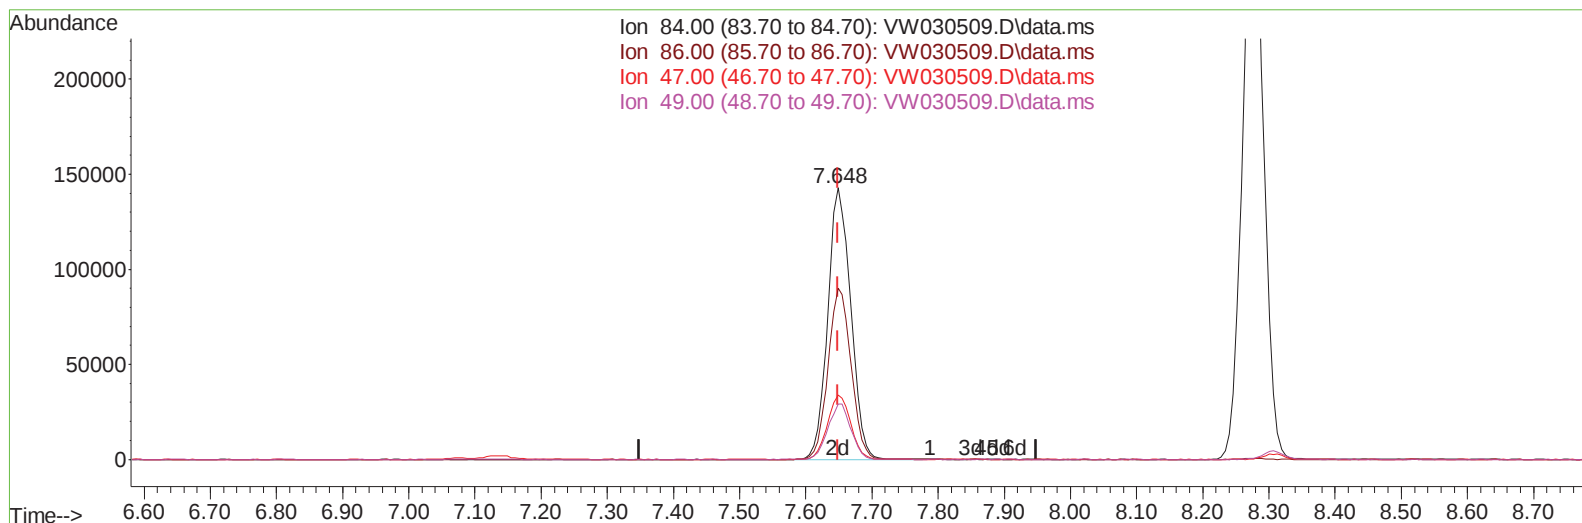

TIC: VW030509.D\data.ms

(24) Chloroform-d (S)

7.648min (+ 0.000) 50.26 ug/L m

response 345351

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	63.10	0.04#
47.00	48.90	0.02#
49.00	28.60	0.02#

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101024\
 Data File : VW030509.D
 Acq On : 10 Oct 2024 14:42
 Operator : SY/MD
 Sample : P4346-11RE
 Misc : 3.26g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EOAX1RE

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 10/15/2024
 Supervised By :Semsettin Yesilyurt 10/15/2024

Quant Time: Oct 11 01:22:32 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Oct 11 01:19:48 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	240266	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	162957	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	47065	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.369	65	187777	49.721	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	198.880%#	
7) Chloroethane-d5	2.905	69	149203	52.192	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	208.760%#	
11) 1,1-Dichloroethene-d2	4.027	65	77440	49.300	ug/L	0.01
Spiked Amount 25.000	Range 45	- 110	Recovery	=	197.200%#	
21) 2-Butanone-d5	7.075	46	82076	120.762	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	241.520%#	
24) Chloroform-d	7.648	84	345351m	50.261	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	201.040%#	
26) 1,2-Dichloroethane-d4	8.307	65	204840	57.330	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	229.320%#	
32) Benzene-d6	8.276	84	662948	70.094	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	280.360%#	
36) 1,2-Dichloropropane-d6	9.276	67	204976	73.838	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	295.360%#	
41) Toluene-d8	10.325	98	588812	68.196	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	272.800%#	
43) trans-1,3-Dichloroprop...	10.575	79	84488	72.683	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	290.720%#	
47) 2-Hexanone-d5	10.922	63	65900	184.311	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	368.620%#	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	158833	77.909	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	311.640%#	
66) 1,2-Dichlorobenzene-d4	13.849	152	169367	106.354	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	425.400%#	
Target Compounds						
13) Acetone	4.131	43	9801	9.850	ug/L	Qvalue 71

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101024\
Data File : VW030509.D
Acq On : 10 Oct 2024 14:42
Operator : SY/MD
Sample : P4346-11RE
Misc : 3.26g/10mL/MSVOA_W/SOIL/B
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EOAX1RE

Manual IntegrationsAPPROVED

Quant Time: Oct 11 01:22:32 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Oct 11 01:19:48 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 10/15/2024
Supervised By :Semsettin Yesilyurt 10/15/2024

