

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101024\
 Data File : VW030502.D
 Acq On : 10 Oct 2024 10:47
 Operator : SY/MD
 Sample : P4346-02
 Misc : 3.12g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EOAW4

Quant Time: Oct 11 01:20:58 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Oct 11 01:19:48 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	408984	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	393520	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	176554	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.357	65	157309	24.470	ug/L	-0.01
Spiked Amount 25.000	Range 30 - 150		Recovery =	97.880%		
7) Chloroethane-d5	2.893	69	120306	24.723	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	98.880%		
11) 1,1-Dichloroethene-d2	4.015	65	62301	23.300	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	93.200%		
21) 2-Butanone-d5	7.075	46	74052	64.009	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	128.020%		
24) Chloroform-d	7.648	84	276251	23.619	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	94.480%		
26) 1,2-Dichloroethane-d4	8.301	65	167158	27.484	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	109.920%		
32) Benzene-d6	8.270	84	524810	22.978	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	91.920%		
36) 1,2-Dichloropropane-d6	9.270	67	159037	23.724	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	94.880%		
41) Toluene-d8	10.325	98	478551	22.952	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	91.800%		
43) trans-1,3-Dichloroprop...	10.575	79	71745	25.559	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	102.240%		
47) 2-Hexanone-d5	10.922	63	57792	66.933	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	133.860%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	144332	29.317	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	117.280%		
66) 1,2-Dichlorobenzene-d4	13.848	152	152020	25.448	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	101.800%		
Target Compounds					Qvalue	
13) Acetone	4.118	43	7505	4.431	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101024\
Data File : VW030502.D
Acq On : 10 Oct 2024 10:47
Operator : SY/MD
Sample : P4346-02
Misc : 3.12g/10mL/MSVOA_W/SOIL/B
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EOAW4

Quant Time: Oct 11 01:20:58 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Oct 11 01:19:48 2024
Response via : Initial Calibration

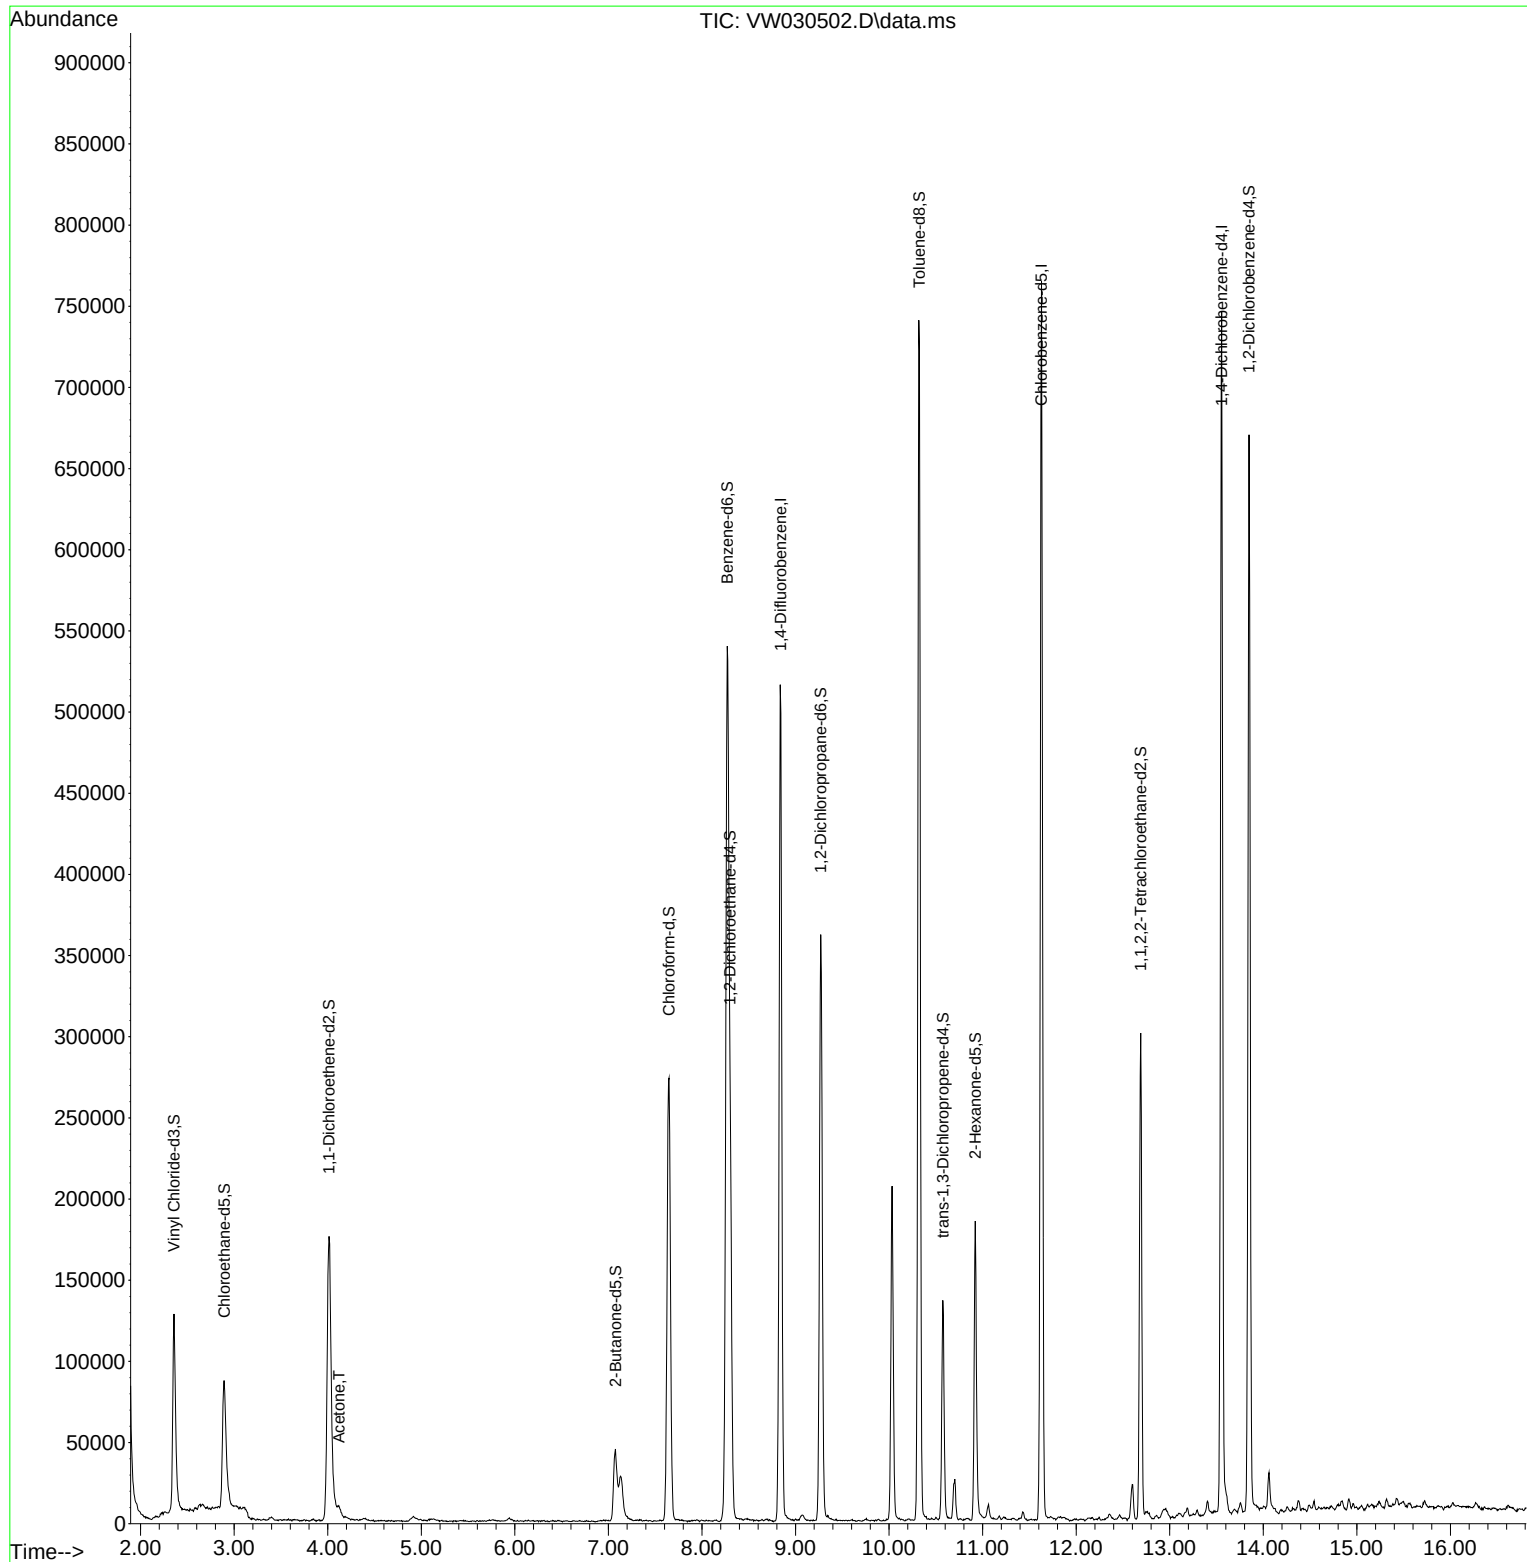

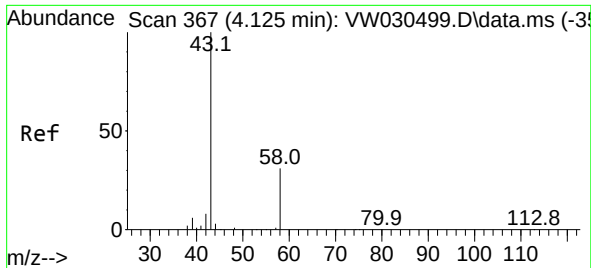

#13
 Acetone
 Concen: 4.431 ug/L
 RT: 4.118 min Scan# 30
 Delta R.T. -0.006 min
 Lab File: VW030502.D
 Acq: 10 Oct 2024 10:47

Instrument :
 MSVOA_W
 ClientSampleId :
 EOAW4

Tgt Ion: 43 Resp: 7505
 Ion Ratio Lower Upper
 43 100
 58 31.8 0.0 57.6

