

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101024\
 Data File : VW030504.D
 Acq On : 10 Oct 2024 12:41
 Operator : SY/MD
 Sample : P4346-03
 Misc : 3.70g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EOAW5

Quant Time: Oct 11 01:21:22 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Oct 11 01:19:48 2024
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By :Mahesh Dadoda 10/15/2024
 Supervised By :Semsettin Yesilyurt 10/15/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	85284	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	34763	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.555	152	6889	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.362	65	172459	128.649	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 514.600%#			
7) Chloroethane-d5	2.899	69	132873	130.944	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 523.760%#			
11) 1,1-Dichloroethene-d2	4.021	65	66927	120.035	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery = 480.120%#			
21) 2-Butanone-d5	7.075	46	77570	321.539	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 643.080%#			
24) Chloroform-d	7.648	84	292612	119.975	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery = 479.880%#			
26) 1,2-Dichloroethane-d4	8.306	65	176910m	139.491	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery = 557.960%#			
32) Benzene-d6	8.276	84	553786	274.472	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery = 1097.880%#			
36) 1,2-Dichloropropane-d6	9.270	67	168805	285.049	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery = 1140.200%#			
41) Toluene-d8	10.324	98	477842	259.432	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery = 1037.720%#			
43) trans-1,3-Dichloroprop...	10.574	79	70978	286.232	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery = 1144.920%#			
47) 2-Hexanone-d5	10.922	63	61265	803.217	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 1606.440%#			
56) 1,1,2,2-Tetrachloroeth...	12.690	84	132560	304.800	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery = 1219.200%#			
66) 1,2-Dichlorobenzene-d4	13.854	152	123687	530.629	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery = 2122.520%#			
Target Compounds					Qvalue	
13) Acetone	4.124	43	9714	27.504	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101024\
Data File : VW030504.D
Acq On : 10 Oct 2024 12:41
Operator : SY/MD
Sample : P4346-03
Misc : 3.70g/10mL/MSVOA_W/SOIL/B
ALS Vial : 10 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
EOAW5

Quant Time: Oct 11 01:21:22 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Oct 11 01:19:48 2024
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Mahesh Dadoda 10/15/2024
Supervised By :Semsettin Yesilyurt 10/15/2024

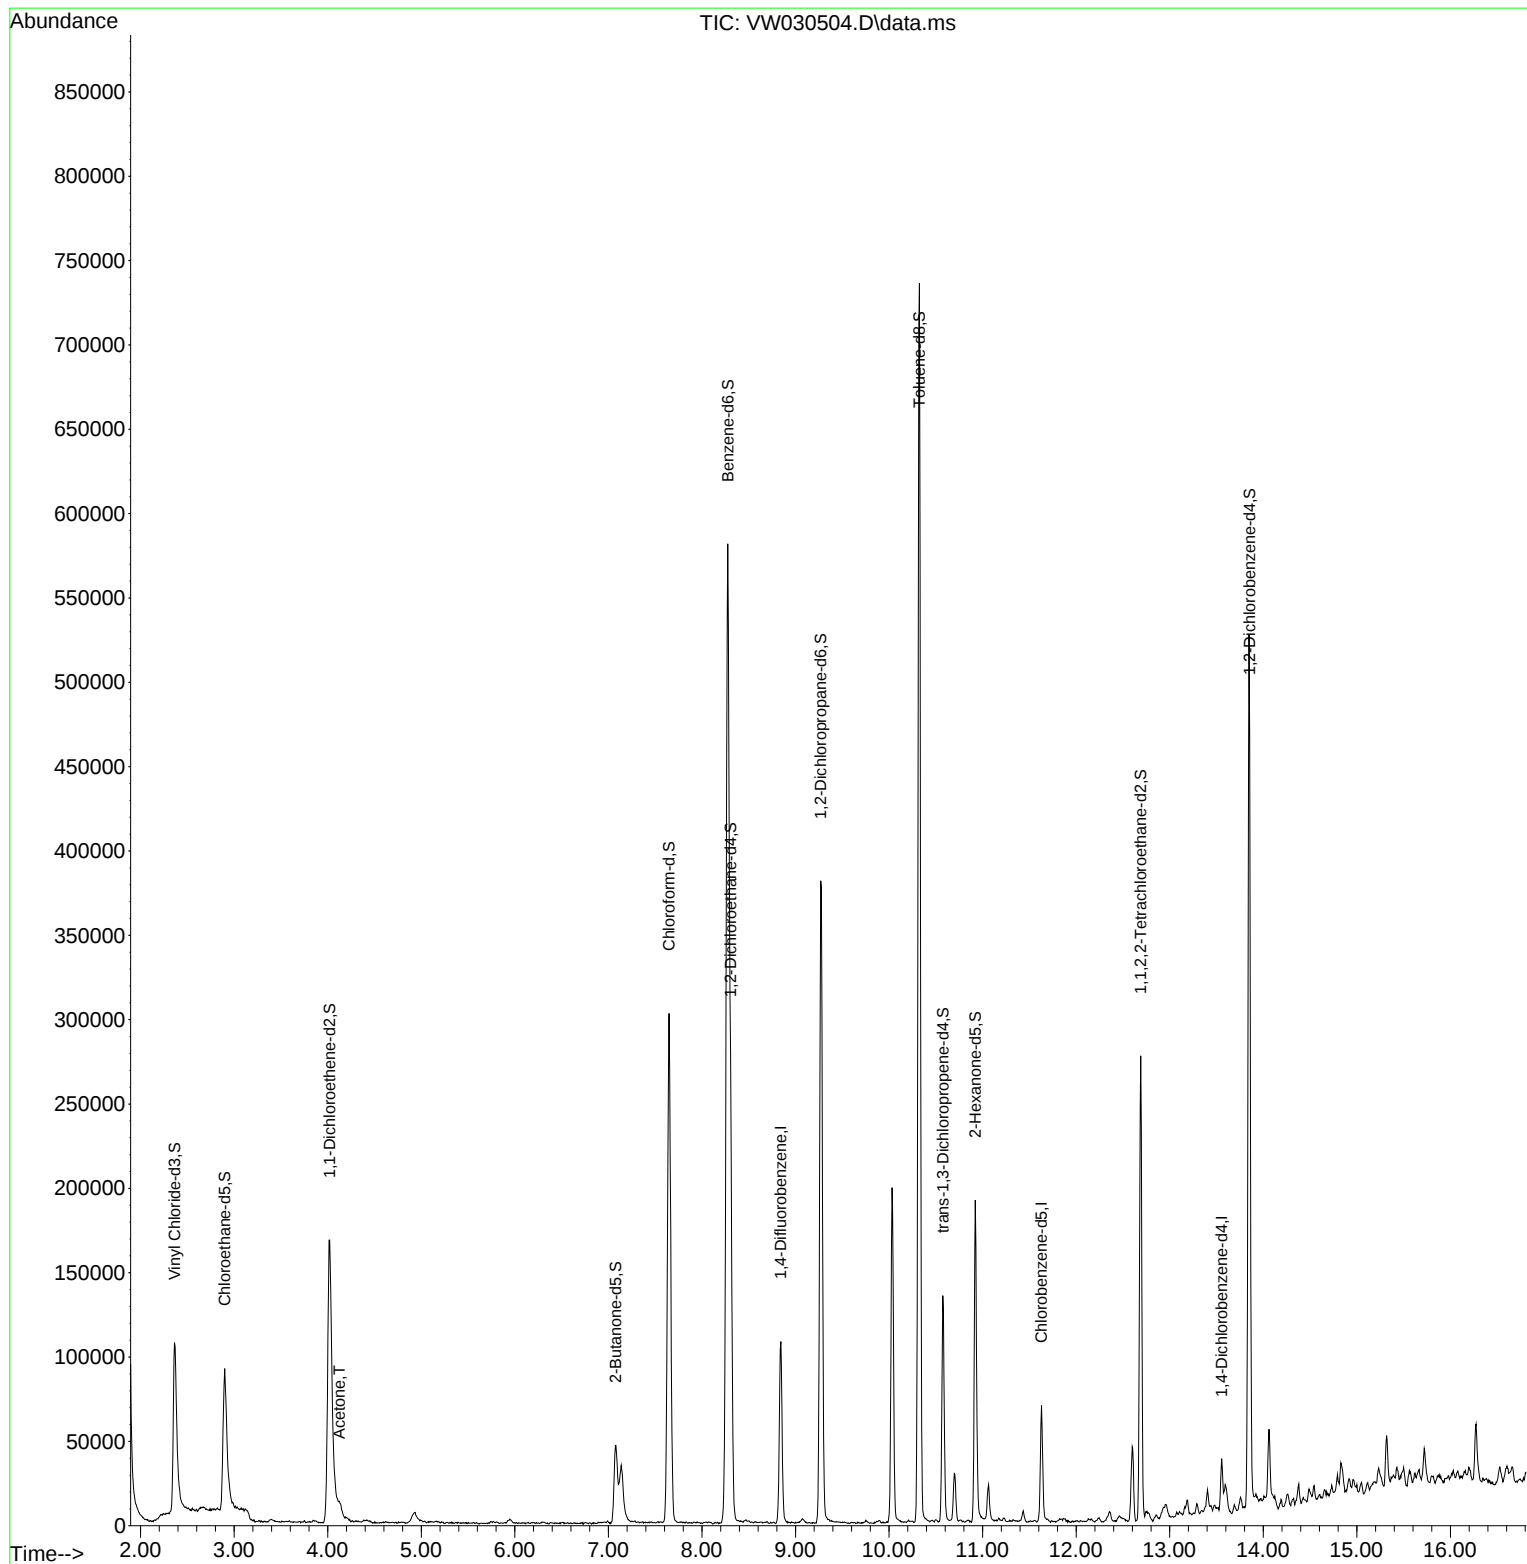

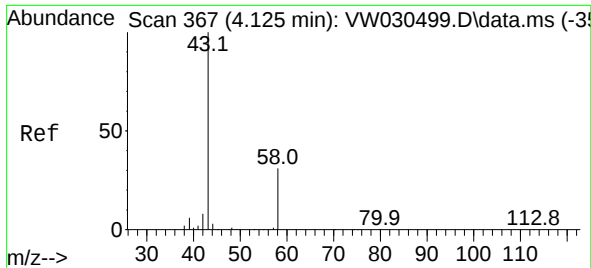

#13
Acetone
Concen: 27.504 ug/L
RT: 4.124 min Scan# 30
Delta R.T. -0.000 min
Lab File: VW030504.D
Acq: 10 Oct 2024 12:41

Instrument :
MSVOA_W
ClientSampleId :
EOAW5

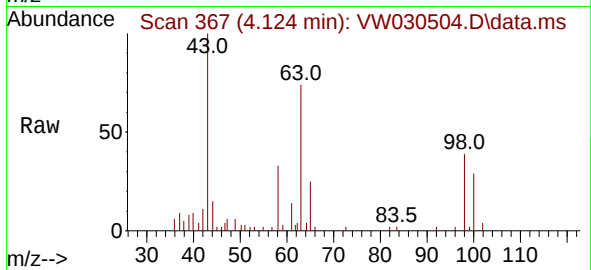

Tgt Ion: 43 Resp: 9714
Ion Ratio Lower Upper
43 100
58 28.3 0.0 57.6

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 10/15/2024
Supervised By :Semsettin Yesilyurt 10/15/2024

