

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101024\
 Data File : VW030505.D
 Acq On : 10 Oct 2024 13:06
 Operator : SY/MD
 Sample : P4346-04
 Misc : 3.50g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EOAW6

Quant Time: Oct 11 01:21:40 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Oct 11 01:19:48 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.837	114	141851	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	103426	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	30014	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	167039	74.916	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	= 299.680%#	
7) Chloroethane-d5	2.899	69	135275	80.150	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	= 320.600%#	
11) 1,1-Dichloroethene-d2	4.021	65	70392	75.904	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	= 303.600%#	
21) 2-Butanone-d5	7.075	46	85961	214.228	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	= 428.460%#	
24) Chloroform-d	7.648	84	319517	78.764	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	= 315.040%#	
26) 1,2-Dichloroethane-d4	8.307	65	195515	92.685	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	= 370.720%#	
32) Benzene-d6	8.276	84	609572	101.547	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	= 406.200%#	
36) 1,2-Dichloropropane-d6	9.276	67	187110	106.199	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	= 424.800%#	
41) Toluene-d8	10.325	98	548081	100.017	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	= 400.080%#	
43) trans-1,3-Dichloroprop...	10.575	79	80681	109.359	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	= 437.440%#	
47) 2-Hexanone-d5	10.922	63	68833	303.323	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	= 606.640%#	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	161811	125.054	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	= 500.200%#	
66) 1,2-Dichlorobenzene-d4	13.849	152	168036	165.463	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	= 661.840%#	
Target Compounds						
13) Acetone	4.119	43	10607	18.056	ug/L	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101024\
Data File : VW030505.D
Acq On : 10 Oct 2024 13:06
Operator : SY/MD
Sample : P4346-04
Misc : 3.50g/10mL/MSVOA_W/SOIL/B
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EOAW6

Quant Time: Oct 11 01:21:40 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Oct 11 01:19:48 2024
Response via : Initial Calibration

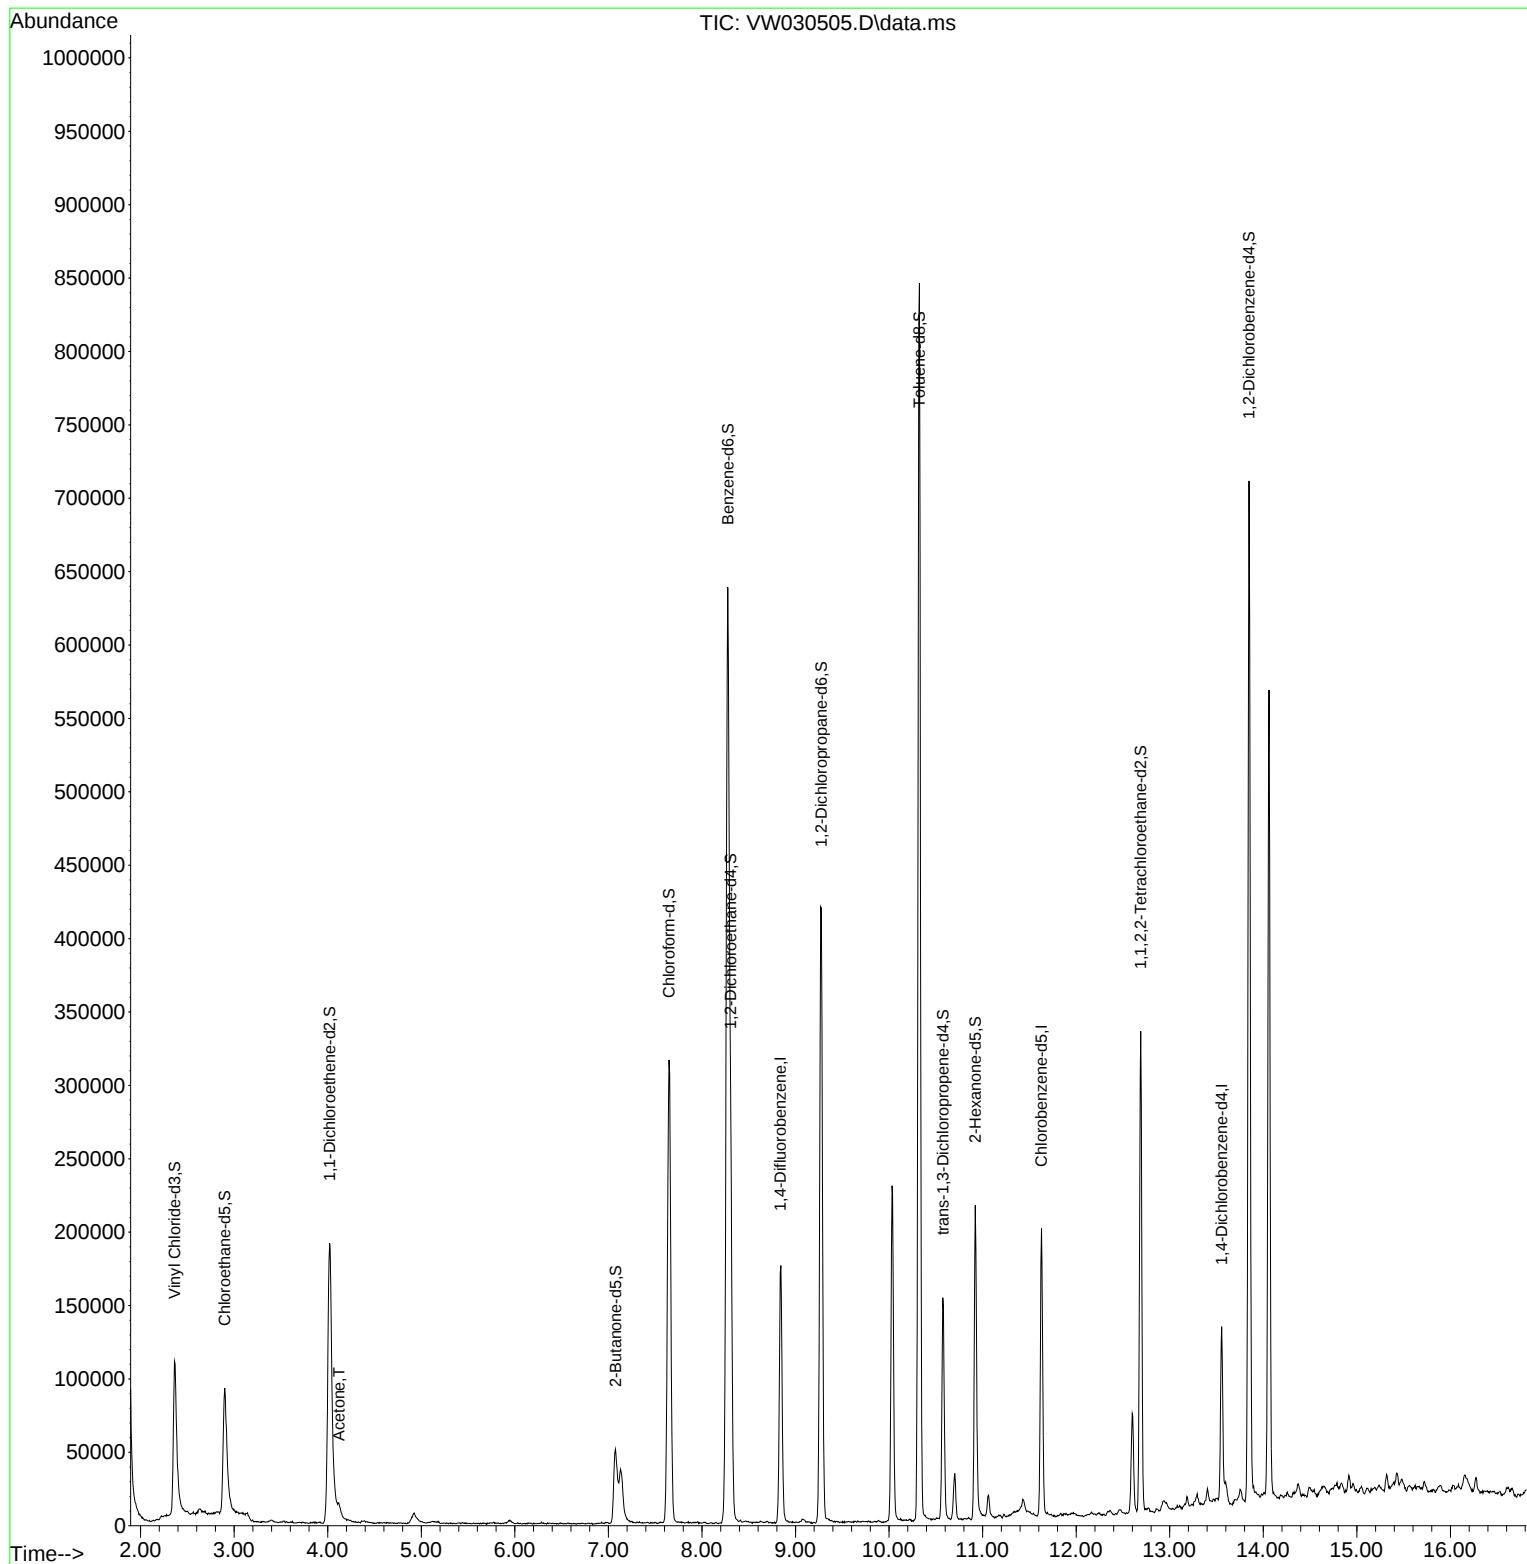

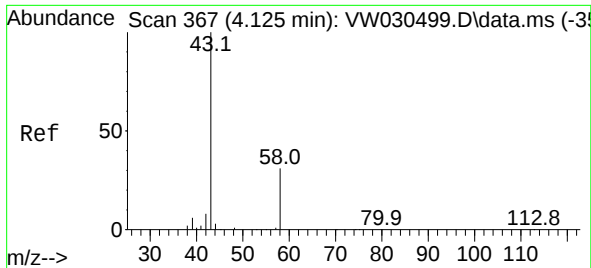

#13
 Acetone
 Concen: 18.056 ug/L
 RT: 4.119 min Scan# 30
 Delta R.T. -0.006 min
 Lab File: VW030505.D
 Acq: 10 Oct 2024 13:06

Instrument :
 MSVOA_W
 ClientSampleId :
 EOAW6

Tgt Ion: 43 Resp: 10607
 Ion Ratio Lower Upper
 43 100
 58 30.8 0.0 57.6

