

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101024\
 Data File : VW030506.D
 Acq On : 10 Oct 2024 13:30
 Operator : SY/MD
 Sample : P4346-06
 Misc : 3.16g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EOAW8

Quant Time: Oct 11 01:21:56 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Oct 11 01:19:48 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	495050	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	476361	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	228824	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.369	65	197011	25.318	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	101.280%
7) Chloroethane-d5	2.899	69	151380	25.700	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	102.800%
11) 1,1-Dichloroethene-d2	4.021	65	79537	24.575	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	98.320%
21) 2-Butanone-d5	7.075	46	88813	63.421	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	126.840%
24) Chloroform-d	7.648	84	343370	24.254	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	97.000%
26) 1,2-Dichloroethane-d4	8.307	65	203277	27.612	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	110.440%
32) Benzene-d6	8.276	84	658698	23.824	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	95.280%
36) 1,2-Dichloropropane-d6	9.276	67	201085	24.780	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	99.120%
41) Toluene-d8	10.325	98	585632	23.203	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	92.800%
43) trans-1,3-Dichloroprop...	10.575	79	85208	25.076	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	100.320%
47) 2-Hexanone-d5	10.922	63	70525	67.475	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	134.960%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	163840	27.492	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	109.960%
66) 1,2-Dichlorobenzene-d4	13.855	152	154149	19.910	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	79.640%
Target Compounds						
					Qvalue	
13) Acetone	4.125	43	13337	6.505	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101024\
Data File : VW030506.D
Acq On : 10 Oct 2024 13:30
Operator : SY/MD
Sample : P4346-06
Misc : 3.16g/10mL/MSVOA_W/SOIL/B
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EOAW8

Quant Time: Oct 11 01:21:56 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Oct 11 01:19:48 2024
Response via : Initial Calibration

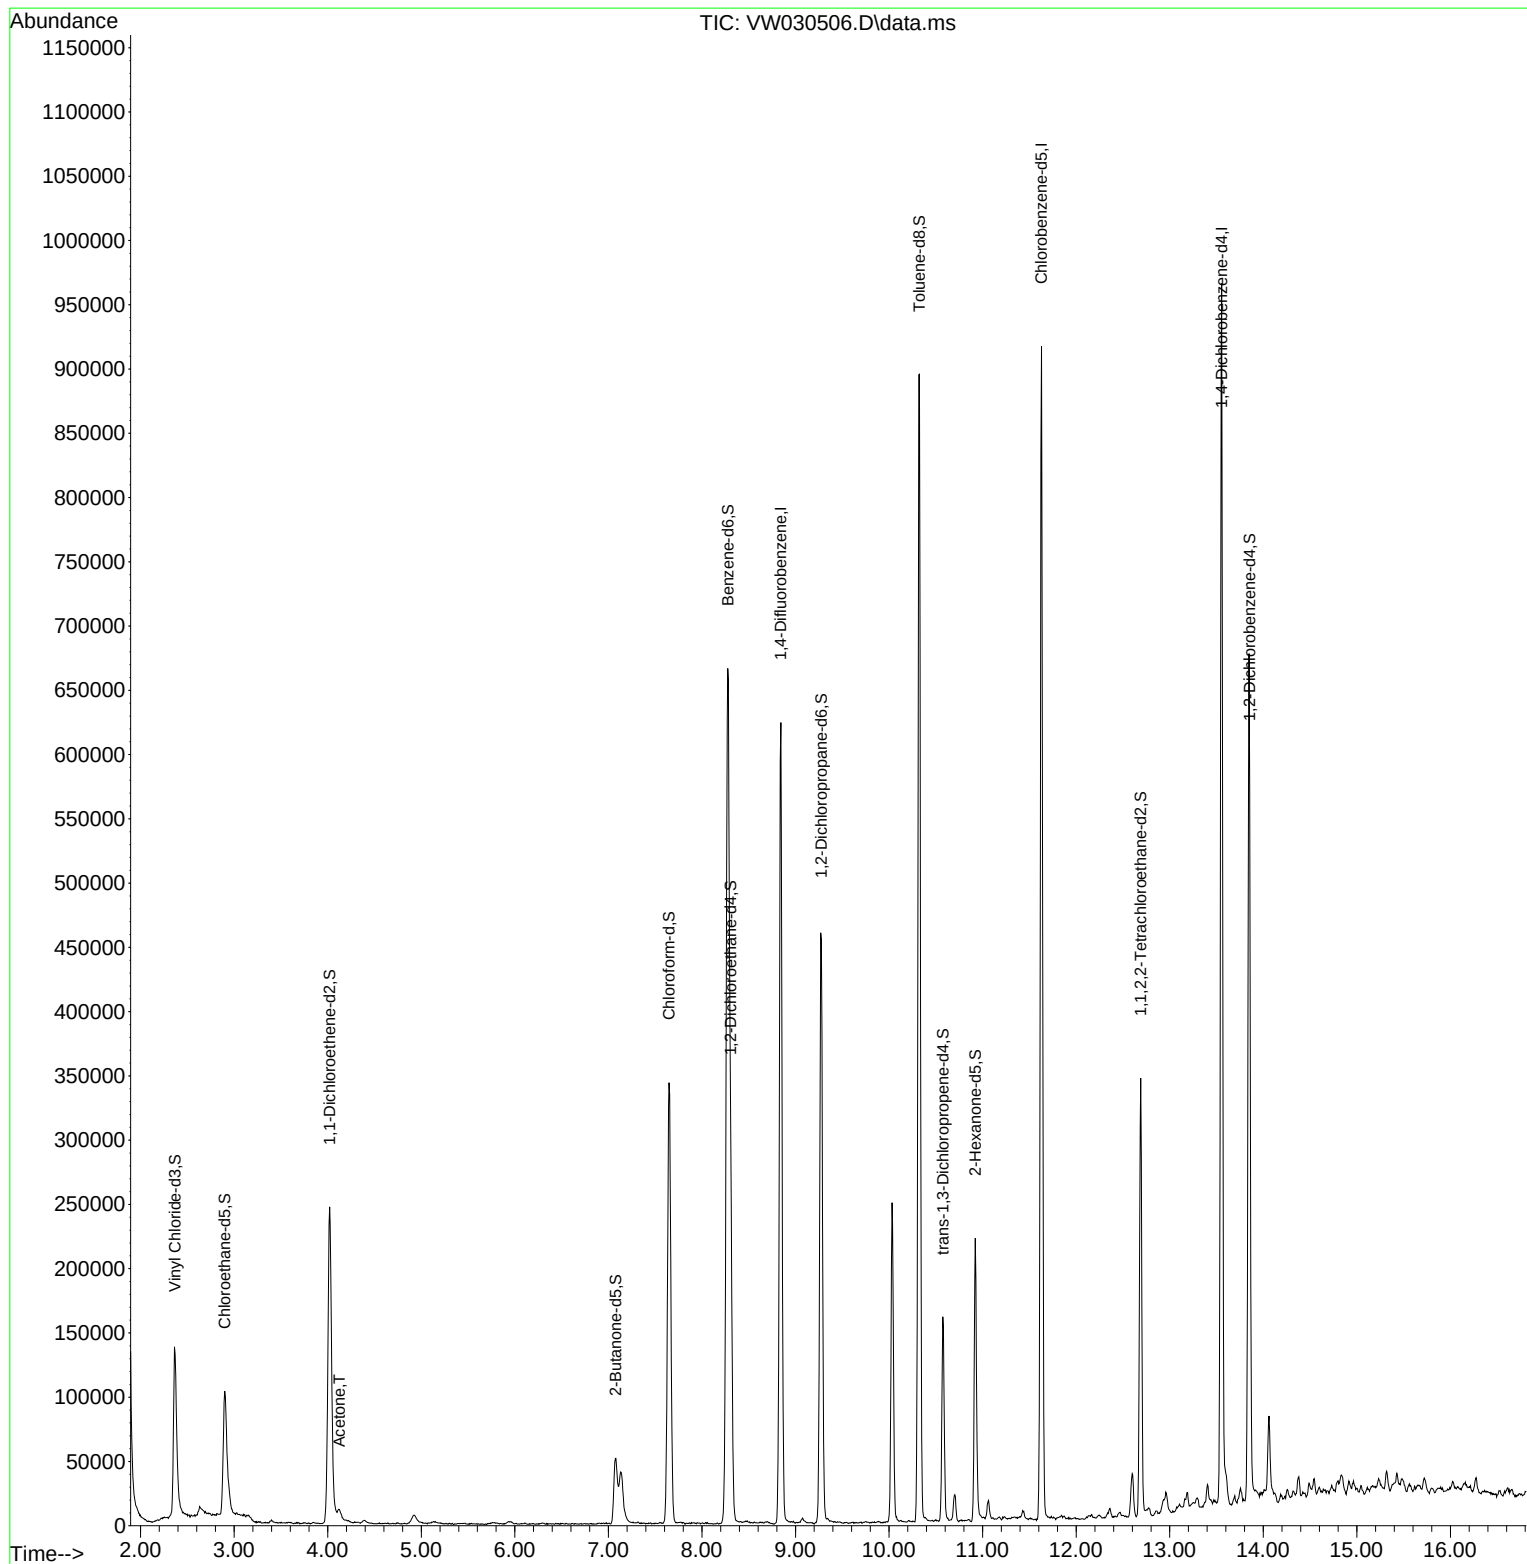

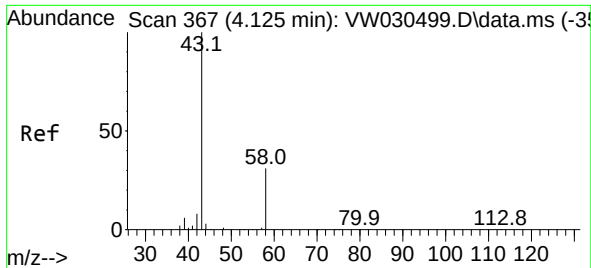

#13

Acetone

Concen: 6.505 ug/L

RT: 4.125 min Scan# 30

Delta R.T. -0.000 min

Lab File: VW030506.D

Acq: 10 Oct 2024 13:30

Instrument :

MSVOA_W

ClientSampleId :

EOAW8

Tgt Ion: 43 Resp: 13337

Ion Ratio Lower Upper

43 100

58 27.0 0.0 57.6

