

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101024\
 Data File : VW030507.D
 Acq On : 10 Oct 2024 13:54
 Operator : SY/MD
 Sample : P4346-07
 Misc : 2.94g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EOAW9

Quant Time: Oct 11 01:22:08 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Oct 11 01:19:48 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	611641	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	558424	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	256206	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	200654	20.871	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	83.480%
7) Chloroethane-d5	2.899	69	157675	21.666	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	86.680%
11) 1,1-Dichloroethene-d2	4.021	65	85215	21.310	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	85.240%
21) 2-Butanone-d5	7.075	46	85700	49.533	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	99.060%
24) Chloroform-d	7.648	84	362947	20.750	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	83.000%
26) 1,2-Dichloroethane-d4	8.307	65	213886	23.515	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	94.080%
32) Benzene-d6	8.276	84	708847	21.871	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	87.480%
36) 1,2-Dichloropropane-d6	9.270	67	215780	22.683	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	90.720%
41) Toluene-d8	10.325	98	642351	21.710	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	86.840%
43) trans-1,3-Dichloroprop...	10.575	79	91428	22.952	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	91.800%
47) 2-Hexanone-d5	10.922	63	67875	55.397	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	110.800%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	171815	24.593	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	98.360%
66) 1,2-Dichlorobenzene-d4	13.848	152	203362	23.459	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	93.840%
Target Compounds						
13) Acetone	4.118	43	11704	4.621	ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101024\
Data File : VW030507.D
Acq On : 10 Oct 2024 13:54
Operator : SY/MD
Sample : P4346-07
Misc : 2.94g/10mL/MSVOA_W/SOIL/B
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EOAW9

Quant Time: Oct 11 01:22:08 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Oct 11 01:19:48 2024
Response via : Initial Calibration

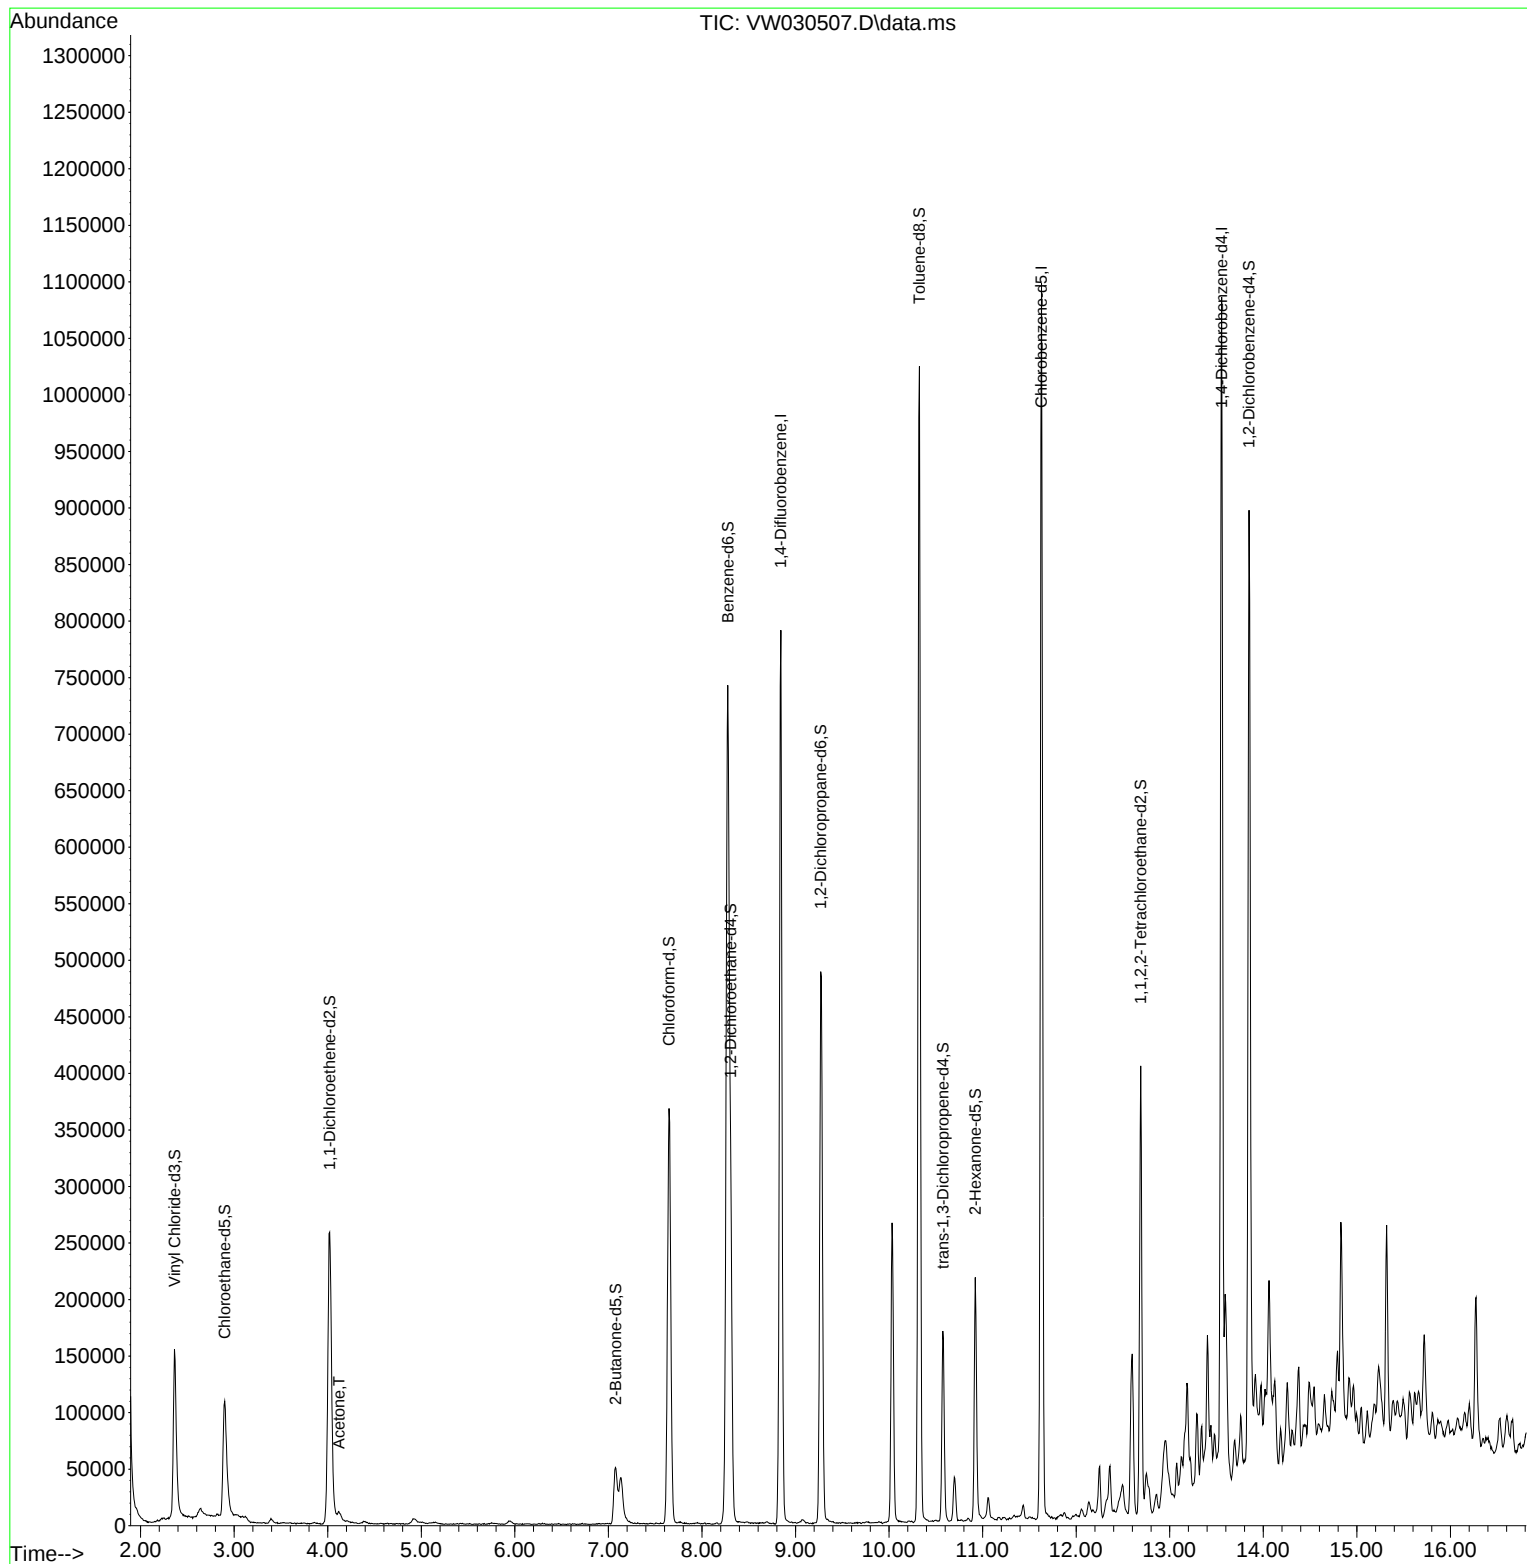

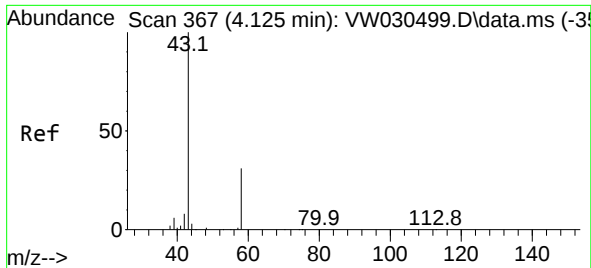

#13
 Acetone
 Concen: 4.621 ug/L
 RT: 4.118 min Scan# 30
 Delta R.T. -0.006 min
 Lab File: VW030507.D
 Acq: 10 Oct 2024 13:54

Instrument :
 MSVOA_W
 ClientSampleId :
 EOAW9

Tgt Ion: 43 Resp: 11704
 Ion Ratio Lower Upper
 43 100
 58 32.9 0.0 57.6

