

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101024\
 Data File : VW030508.D
 Acq On : 10 Oct 2024 14:18
 Operator : SY/MD
 Sample : P4346-10
 Misc : 3.28g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EOAX0

Quant Time: Oct 11 01:22:20 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Oct 11 01:19:48 2024
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By :Mahesh Dadoda 10/15/2024
 Supervised By :Semsettin Yesilyurt 10/15/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	500696	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	441003	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	190441	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	113900	14.472	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	57.880%		
7) Chloroethane-d5	2.899	69	90426	15.179	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	60.720%		
11) 1,1-Dichloroethene-d2	4.021	65	39932	12.199	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	48.800%		
21) 2-Butanone-d5	7.075	46	43228	30.521	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	61.040%		
24) Chloroform-d	7.648	84	178833	12.489	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	49.960%		
26) 1,2-Dichloroethane-d4	8.307	65	112012m	15.044	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	60.160%#		
32) Benzene-d6	8.276	84	331395	12.947	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	51.800%		
36) 1,2-Dichloropropane-d6	9.276	67	104986	13.975	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	55.880%#		
41) Toluene-d8	10.325	98	250469	10.719	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	42.880%		
43) trans-1,3-Dichloroprop...	10.581	79	36892	11.727	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	46.920%		
47) 2-Hexanone-d5	10.922	63	31401	32.452	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	64.900%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	68936	12.495	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	49.960%		
66) 1,2-Dichlorobenzene-d4	13.848	152	53269	8.267	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	33.080%#		
Target Compounds					Qvalue	
13) Acetone	4.125	43	12169	5.869	ug/L	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101024\
Data File : VW030508.D
Acq On : 10 Oct 2024 14:18
Operator : SY/MD
Sample : P4346-10
Misc : 3.28g/10mL/MSVOA_W/SOIL/B
ALS Vial : 14 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
EOAX0

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 10/15/2024
Supervised By :Semsettin Yesilyurt 10/15/2024


Quant Time: Oct 11 01:22:20 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Oct 11 01:19:48 2024
Response via : Initial Calibration

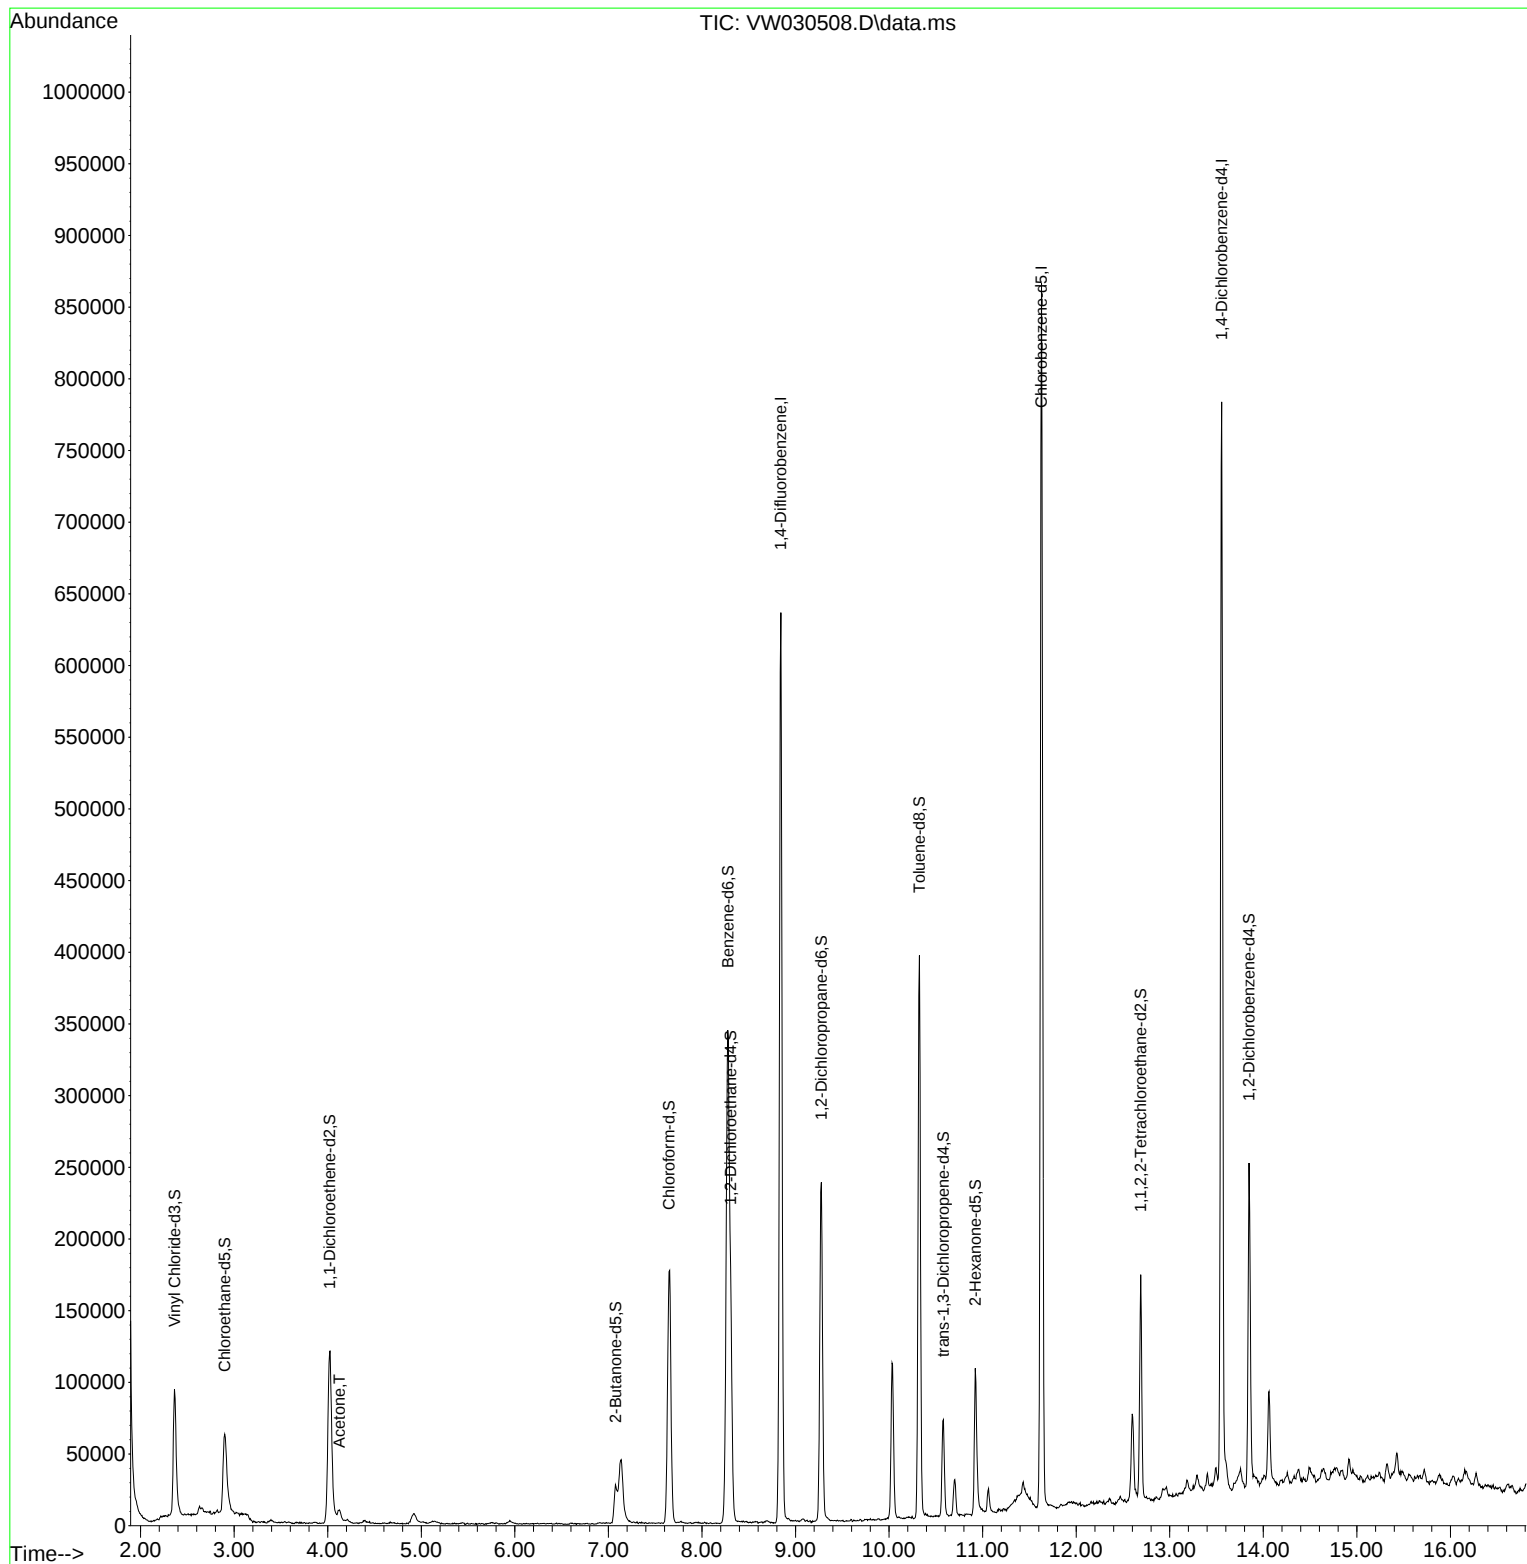

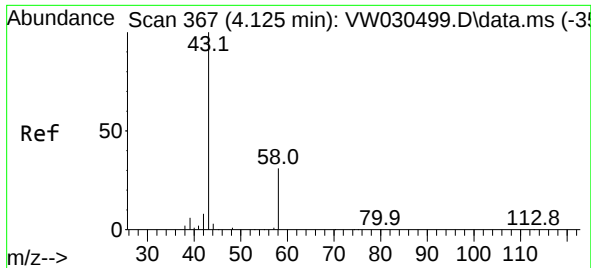

#13
 Acetone
 Concen: 5.869 ug/L
 RT: 4.125 min Scan# 30
 Delta R.T. 0.000 min
 Lab File: VW030508.D
 Acq: 10 Oct 2024 14:18

Instrument :
 MSVOA_W
 ClientSampleId :
 EOAX0

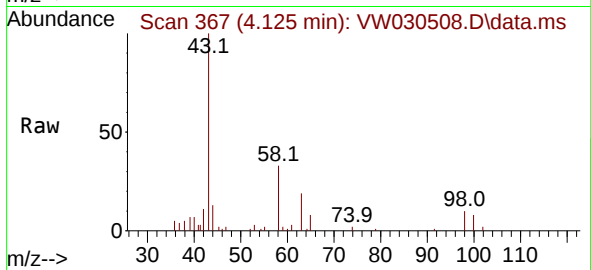

Tgt Ion: 43 Resp: 12169
 Ion Ratio Lower Upper
 43 100
 58 32.4 0.0 57.6

Manual Integrations
 APPROVED

Reviewed By :Mahesh Dadoda 10/15/2024
 Supervised By :Semsettin Yesilyurt 10/15/2024

