

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101024\
 Data File : VW030509.D
 Acq On : 10 Oct 2024 14:42
 Operator : SY/MD
 Sample : P4346-11RE
 Misc : 3.26g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EOAX1RE

Quant Time: Oct 11 01:22:32 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Oct 11 01:19:48 2024
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By :Mahesh Dadoda 10/15/2024
 Supervised By :Semsettin Yesilyurt 10/15/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	240266	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	162957	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	47065	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.369	65	187777	49.721	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	= 198.880%#	
7) Chloroethane-d5	2.905	69	149203	52.192	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	= 208.760%#	
11) 1,1-Dichloroethene-d2	4.027	65	77440	49.300	ug/L	0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	= 197.200%#	
21) 2-Butanone-d5	7.075	46	82076	120.762	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	= 241.520%#	
24) Chloroform-d	7.648	84	345351m	50.261	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	= 201.040%#	
26) 1,2-Dichloroethane-d4	8.307	65	204840	57.330	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	= 229.320%#	
32) Benzene-d6	8.276	84	662948	70.094	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	= 280.360%#	
36) 1,2-Dichloropropane-d6	9.276	67	204976	73.838	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	= 295.360%#	
41) Toluene-d8	10.325	98	588812	68.196	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	= 272.800%#	
43) trans-1,3-Dichloroprop...	10.575	79	84488	72.683	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	= 290.720%#	
47) 2-Hexanone-d5	10.922	63	65900	184.311	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	= 368.620%#	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	158833	77.909	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	= 311.640%#	
66) 1,2-Dichlorobenzene-d4	13.849	152	169367	106.354	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	= 425.400%#	
Target Compounds						
13) Acetone	4.131	43	9801	9.850	ug/L	Qvalue 71

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101024\
Data File : VW030509.D
Acq On : 10 Oct 2024 14:42
Operator : SY/MD
Sample : P4346-11RE
Misc : 3.26g/10mL/MSVOA_W/SOIL/B
ALS Vial : 15 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
EOAX1RE

Quant Time: Oct 11 01:22:32 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Oct 11 01:19:48 2024
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Mahesh Dadoda 10/15/2024
Supervised By :Semsettin Yesilyurt 10/15/2024

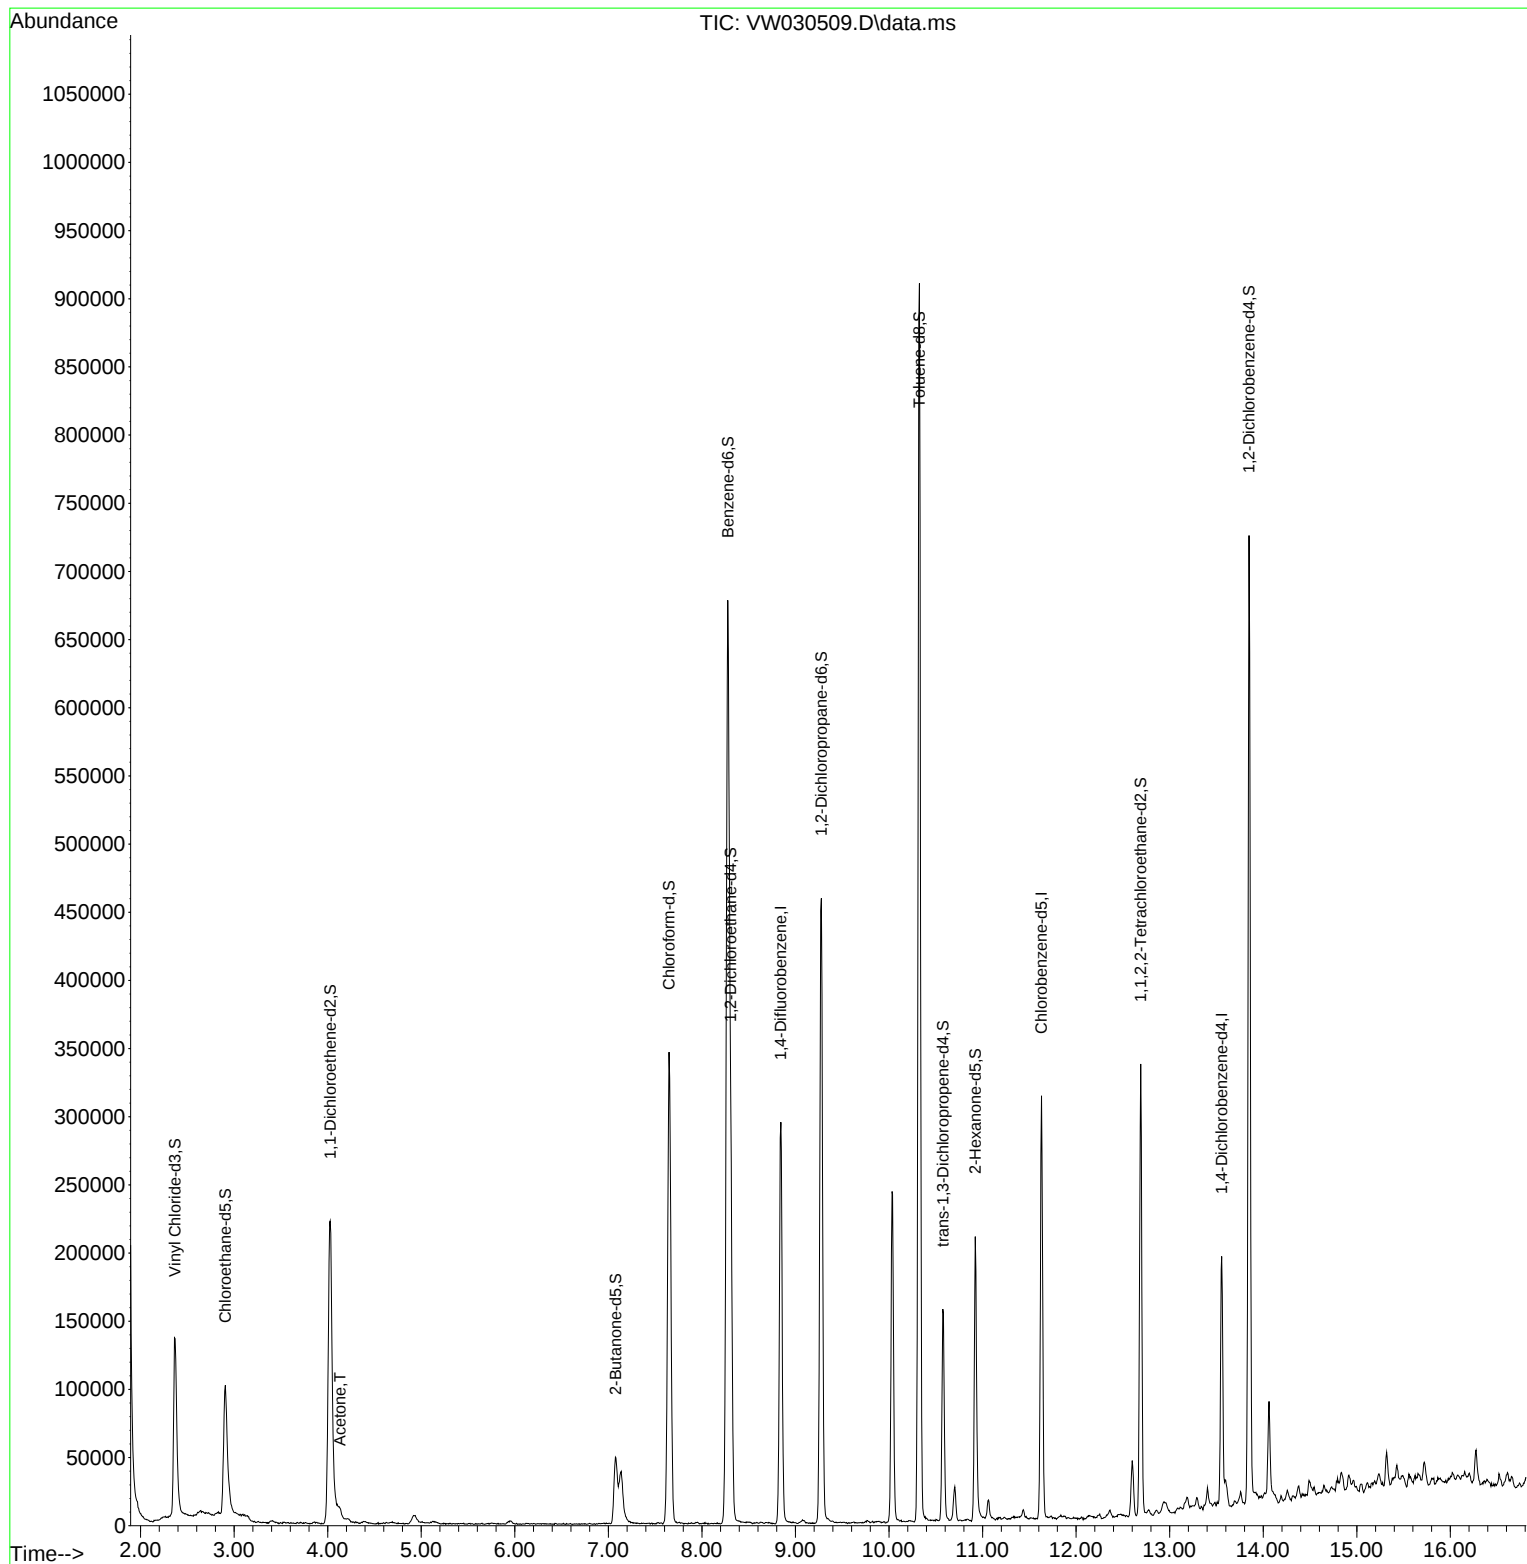

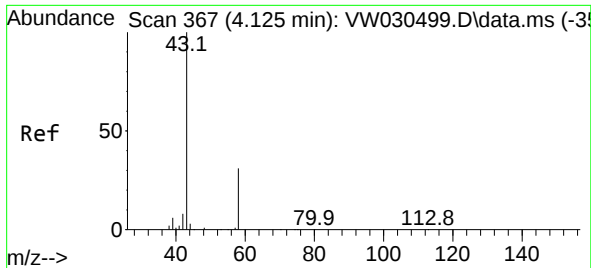

#13
 Acetone
 Concen: 9.850 ug/L
 RT: 4.131 min Scan# 30
 Delta R.T. 0.006 min
 Lab File: VW030509.D
 Acq: 10 Oct 2024 14:42

Instrument :
 MSVOA_W
 ClientSampleId :
 EOAX1RE

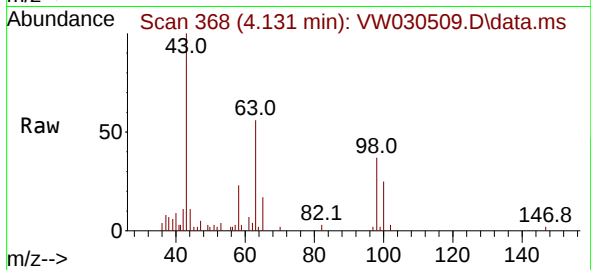

Tgt Ion: 43 Resp: 980
 Ion Ratio Lower Upper
 43 100
 58 13.3 0.0 57.6

Manual Integrations
 APPROVED

Reviewed By :Mahesh Dadoda 10/15/2024
 Supervised By :Semsettin Yesilyurt 10/15/2024

