

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101024\
 Data File : VW030514.D
 Acq On : 10 Oct 2024 16:41
 Operator : SY/MD
 Sample : P4346-15RE
 Misc : 2.81g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EOAX5RE

Quant Time: Oct 11 01:23:40 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Oct 11 01:19:48 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	190923	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	130960	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	42289	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	146296	48.749	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	195.000%#
7) Chloroethane-d5	2.905	69	113870	50.127	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	200.520%#
11) 1,1-Dichloroethene-d2	4.027	65	54677	43.805	ug/L	0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	175.200%#
21) 2-Butanone-d5	7.075	46	58910	109.078	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	218.160%#
24) Chloroform-d	7.648	84	247461	45.322	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	181.280%#
26) 1,2-Dichloroethane-d4	8.307	65	149474	52.646	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	210.600%#
32) Benzene-d6	8.276	84	457679	60.214	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	240.840%#
36) 1,2-Dichloropropane-d6	9.276	67	144495	64.769	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	259.080%#
41) Toluene-d8	10.325	98	370771	53.435	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	213.720%#
43) trans-1,3-Dichloroprop...	10.575	79	52581	56.286	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	225.160%#
47) 2-Hexanone-d5	10.922	63	45631	158.803	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	317.600%#
56) 1,1,2,2-Tetrachloroeth...	12.690	84	108023	65.932	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	263.720%#
66) 1,2-Dichlorobenzene-d4	13.848	152	87133	60.895	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	243.560%#
Target Compounds					Qvalue	
13) Acetone	4.125	43	11113	14.055	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101024\
Data File : VW030514.D
Acq On : 10 Oct 2024 16:41
Operator : SY/MD
Sample : P4346-15RE
Misc : 2.81g/10mL/MSVOA_W/SOIL/B
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EOAX5RE

Quant Time: Oct 11 01:23:40 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Oct 11 01:19:48 2024
Response via : Initial Calibration

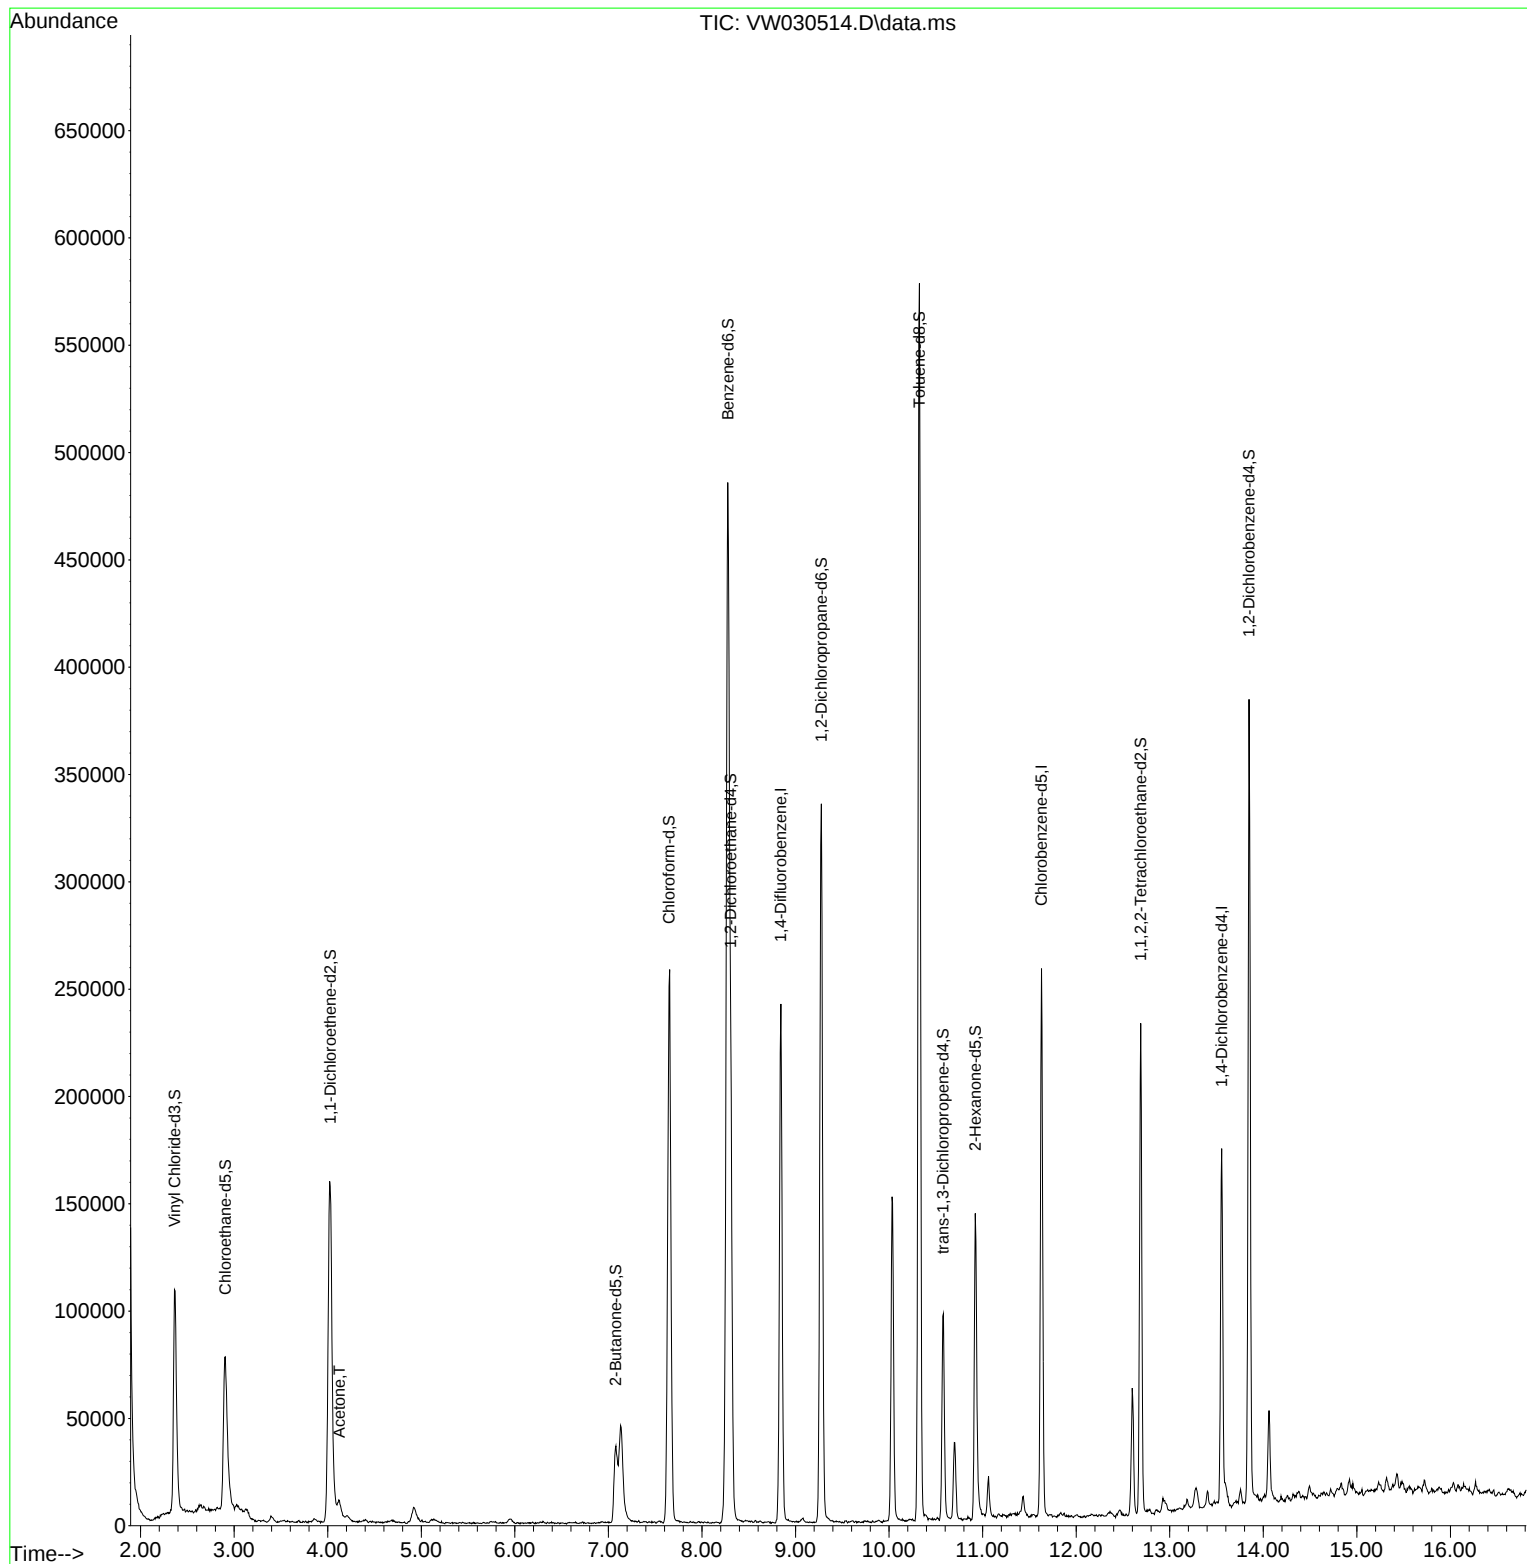

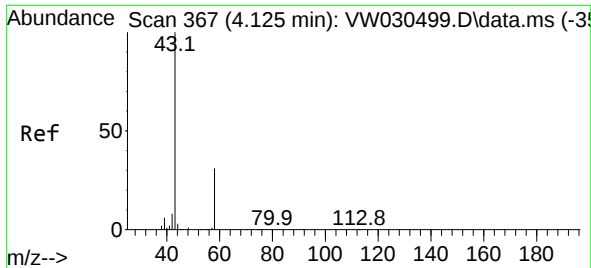

#13
 Acetone
 Concen: 14.055 ug/L
 RT: 4.125 min Scan# 30
 Delta R.T. -0.000 min
 Lab File: VW030514.D
 Acq: 10 Oct 2024 16:41

Instrument :
 MSVOA_W
 ClientSampleId :
 EOAX5RE

Tgt Ion: 43 Resp: 11113
 Ion Ratio Lower Upper
 43 100
 58 28.9 0.0 57.6

