
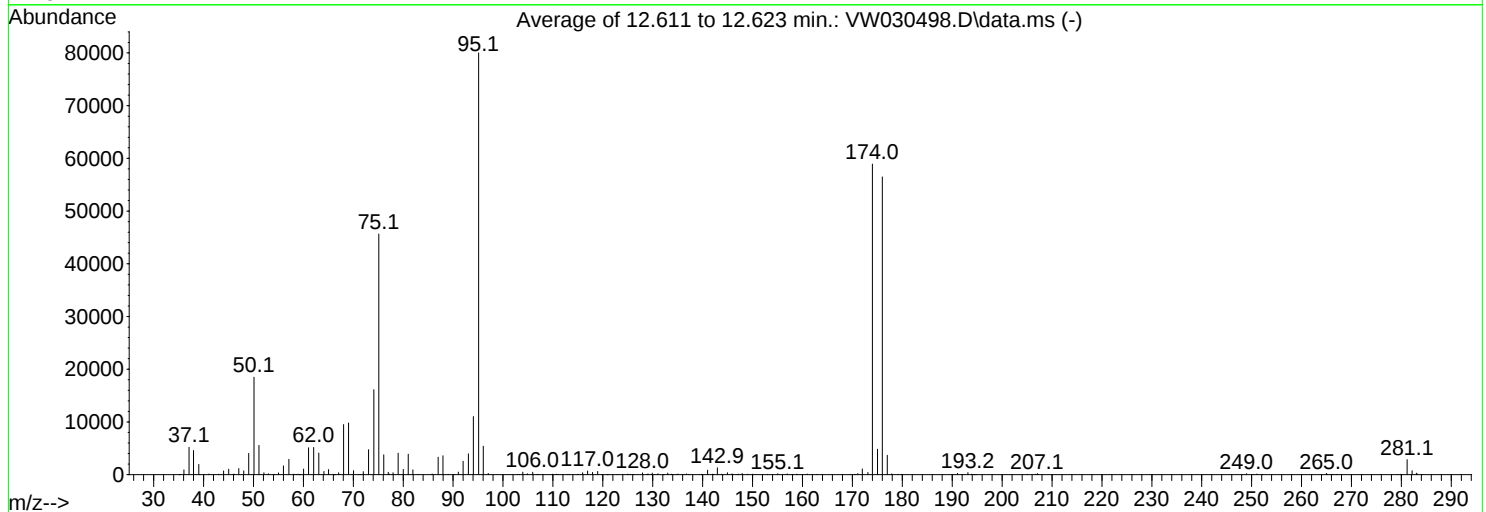


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101024\
Data File : VW030498.D
Acq On : 10 Oct 2024 08:00
Operator : SY/MD
Sample : BFB573
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB573

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Title : SFAM01.0
Last Update : Tue Oct 15 01:09:12 2024

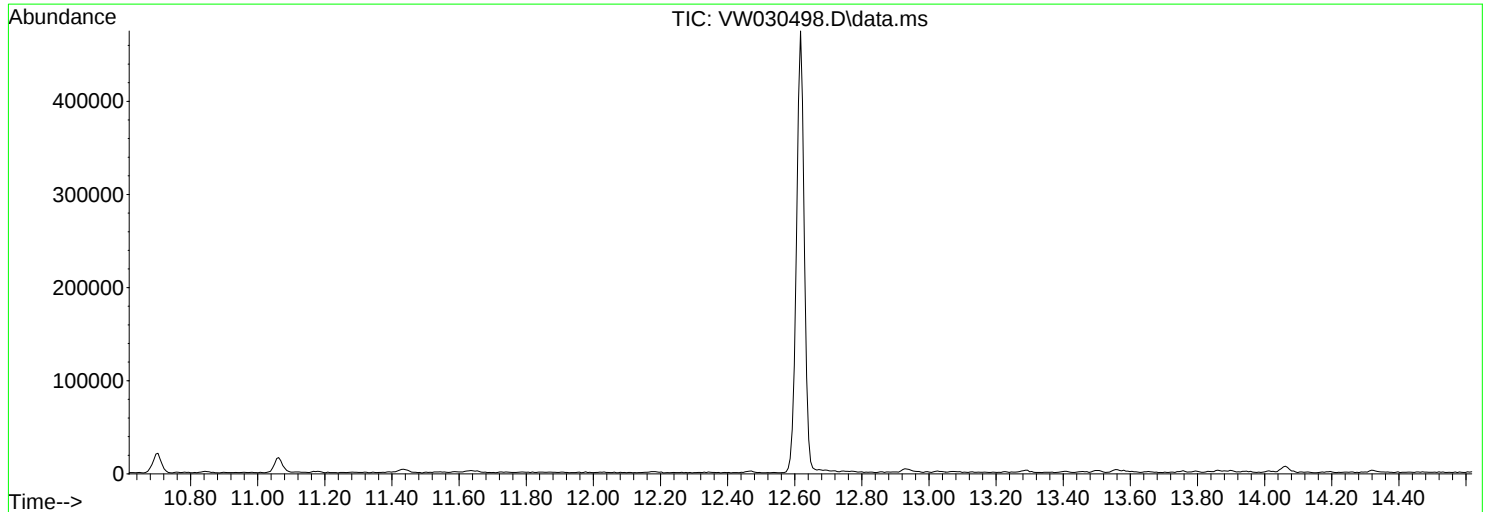

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1751

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	23.1	18498	PASS
75	95	30	80	57.0	45643	PASS
95	95	100	100	100.0	80019	PASS
96	95	5	9	6.7	5398	PASS
173	174	0.00	2	0.7	418	PASS
174	95	50	120	73.6	58912	PASS
175	174	5	9	8.2	4820	PASS
176	174	95	101	95.9	56507	PASS
177	176	5	9	6.5	3673	PASS

m/z	Abundance
35.10	62.0
38.00	71.0
40.00	321.0
41.30	63.0
42.20	50.0
43.90	206.0
45.30	74.0
48.60	78.0
53.80	57.0
55.40	62.0
56.00	66.0
57.10	76.0
59.40	65.0
63.20	54.0
64.80	61.0
97.40	57.0

Instrument :
MSVOA_W
ClientSampleId :
BFB573

m/z	Abundance
35.10	73.0
36.00	811.0
37.10	5332.0
38.00	5010.0
39.10	1948.0
40.10	342.0
41.10	115.0
43.00	99.0
44.10	739.0
45.10	1161.0
45.90	158.0
47.00	1098.0
48.00	620.0
49.10	3939.0
50.10	18832.0
51.10	5807.0
52.10	418.0
53.00	218.0
53.90	122.0
55.00	361.0
56.10	1499.0
57.10	3266.0
58.00	147.0
58.90	129.0
59.30	121.0
60.00	1074.0
61.00	5178.0
62.10	5500.0
63.10	4157.0
64.10	703.0
65.10	1121.0
66.00	104.0
67.10	362.0
68.00	9073.0
69.00	9655.0
70.10	783.0
71.40	91.0
72.00	542.0
73.10	4780.0
74.10	15867.0
75.10	43584.0
76.10	3899.0
77.00	730.0
77.90	284.0
79.00	3996.0
80.00	975.0
81.00	3884.0
81.90	887.0
82.90	125.0
85.80	168.0
87.00	3377.0
88.00	3597.0
89.00	145.0
91.00	497.0
92.00	2438.0
93.10	3700.0
94.00	10325.0
95.10	74944.0
96.00	5224.0
97.10	231.0
103.30	136.0
104.00	496.0
104.80	189.0
105.90	333.0
106.80	83.0
107.10	96.0
108.00	71.0
109.90	99.0
110.70	122.0
113.00	66.0
114.80	98.0
115.20	86.0
116.00	396.0
116.90	606.0
117.90	427.0
119.00	820.0
119.90	75.0
120.90	55.0
122.90	56.0
124.00	75.0
124.90	146.0
125.50	152.0
126.00	90.0
128.00	285.0
128.90	273.0
129.90	359.0
131.00	194.0
133.00	453.0
133.70	276.0
134.70	177.0
136.90	232.0
139.80	114.0

Instrument :
MSVOA_W
ClientSampleId :
BFB573

141.00	840.0
142.00	109.0
143.00	1331.0
143.90	115.0
144.90	398.0
145.90	225.0
146.90	126.0
148.00	151.0
149.10	91.0
152.00	74.0
155.00	199.0
156.90	175.0
158.80	136.0
161.00	100.0
162.90	125.0
170.70	149.0
171.10	300.0
172.00	1099.0
174.00	46624.0
175.10	4216.0
176.00	47216.0
177.00	3572.0
177.90	115.0
179.20	117.0
179.80	59.0
191.00	396.0
191.90	122.0
193.10	710.0
194.00	125.0
194.80	100.0
205.10	105.0
207.10	219.0
249.00	423.0
250.30	68.0
251.00	162.0
252.10	103.0
265.10	419.0
265.80	113.0
266.30	176.0
266.90	165.0
279.10	67.0
279.90	145.0
281.10	4725.0
282.10	1050.0
283.00	662.0
284.10	159.0

Instrument :
MSVOA_W
ClientSampleId :
BFB573

m/z	Abundance
35.10	68.0
36.10	1117.0
37.10	5773.0
38.10	5203.0
39.10	2264.0
40.00	259.0
41.10	170.0
42.30	55.0
44.00	1169.0
45.00	1028.0
46.10	238.0
47.10	1301.0
48.00	860.0
49.10	4624.0
50.10	21384.0
51.10	6222.0
52.10	393.0
53.10	183.0
54.10	97.0
55.10	363.0
56.00	1942.0
57.10	3128.0
58.20	167.0
59.10	95.0
60.10	1200.0
61.10	5431.0
62.10	5525.0
63.10	4421.0
64.10	551.0
65.00	1013.0
66.00	134.0
67.10	411.0
68.00	10679.0
69.10	10840.0
70.00	815.0
72.00	765.0
73.10	5254.0
74.10	17704.0
75.10	52288.0
76.10	4223.0
77.00	679.0
78.00	449.0
79.00	4585.0
80.00	1148.0
81.00	4214.0
81.90	1034.0
85.80	179.0
87.00	3542.0
88.00	4311.0
91.10	493.0
92.00	2889.0
93.10	4115.0
94.00	12704.0
95.10	91320.0
96.10	5969.0
97.00	297.0
102.90	143.0
104.00	555.0
104.90	236.0
106.00	604.0
106.80	145.0
108.00	81.0
109.90	52.0
110.70	147.0
111.90	70.0
113.00	149.0
115.00	142.0
115.90	413.0
117.00	765.0
117.90	464.0
118.90	565.0
119.80	65.0
124.00	78.0
125.00	105.0
126.10	52.0
127.90	366.0
129.10	213.0
130.00	291.0
131.00	192.0
133.00	356.0
134.20	62.0
135.00	179.0
136.20	60.0
136.80	130.0
140.00	102.0
141.00	904.0
142.20	236.0
142.90	1420.0
143.80	79.0
144.90	349.0
146.10	195.0
147.10	132.0

Instrument :
MSVOA_W
ClientSampleId :
BFB573

147.90	227.0
149.10	94.0
150.10	147.0
153.00	95.0
155.10	179.0
157.00	220.0
159.00	112.0
160.90	162.0
162.90	55.0
170.40	132.0
171.90	1250.0
174.00	66096.0
175.00	5489.0
176.00	63880.0
177.00	3465.0
177.90	230.0
179.10	115.0
191.10	257.0
192.20	98.0
193.20	437.0
193.80	83.0
194.40	52.0
204.90	89.0
206.90	235.0
207.20	226.0
249.00	131.0
251.10	91.0
264.90	308.0
266.00	170.0
267.10	81.0
279.20	56.0
280.10	94.0
281.20	2578.0
282.20	808.0
283.20	367.0

Instrument :
MSVOA_W
ClientSampleId :
BFB573

m/z	Abundance
35.10	55.0
36.00	827.0
37.10	4497.0
38.10	3717.0
39.00	1638.0
39.90	312.0
40.90	79.0
42.20	75.0
43.10	158.0
44.00	793.0
45.10	897.0
46.10	139.0
47.00	1085.0
48.10	682.0
49.00	3590.0
50.10	15277.0
51.10	4652.0
52.20	269.0
52.90	171.0
54.20	57.0
54.90	268.0
56.00	1767.0
57.10	2623.0
58.00	143.0
58.60	127.0
59.00	114.0
60.00	959.0
61.00	4721.0
62.00	4478.0
63.10	3846.0
64.10	561.0
65.10	777.0
66.20	52.0
67.00	356.0
68.10	8712.0
69.00	8932.0
70.00	676.0
71.10	70.0
72.00	448.0
73.00	4214.0
74.10	14817.0
75.10	41056.0
76.10	3227.0
77.20	395.0
77.90	356.0
79.00	3589.0
80.00	935.0
81.00	3587.0
82.00	785.0
83.00	79.0
87.00	3052.0
87.90	2814.0
90.20	67.0
91.10	496.0
92.00	2328.0
93.00	4010.0
94.10	10053.0
95.10	73792.0
96.10	5002.0
97.00	186.0
103.90	444.0
104.90	159.0
106.00	452.0
107.00	122.0
108.00	81.0
110.00	109.0
111.00	164.0
112.00	149.0
113.30	71.0
114.90	62.0
116.00	308.0
116.90	694.0
118.00	365.0
119.00	483.0
122.70	76.0
124.00	64.0
125.20	94.0
126.20	62.0
128.00	345.0
129.00	150.0
129.80	230.0
131.10	163.0
132.10	54.0
133.10	142.0
133.90	66.0
135.10	197.0
136.70	117.0
137.20	158.0
139.80	97.0
141.00	858.0
141.90	144.0
142.90	1201.0

Instrument :
MSVOA_W
ClientSampleId :
BFB573

143.80	127.0
145.00	356.0
145.90	209.0
147.20	110.0
147.80	226.0
149.00	65.0
149.90	112.0
153.00	101.0
155.00	183.0
156.90	99.0
157.90	109.0
158.80	104.0
161.00	145.0
169.60	76.0
171.10	326.0
172.10	943.0
173.10	1255.0
174.00	64016.0
175.00	4754.0
176.00	58424.0
177.00	3981.0
177.90	133.0
191.00	76.0
193.00	86.0
193.80	74.0
206.70	166.0
207.30	71.0
251.10	76.0
265.20	155.0
281.00	1260.0
282.10	407.0
282.90	145.0

Instrument :
MSVOA_W
ClientSampleId :
BFB573